

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
 Data File : BN029242.D
 Acq On : 16 Jan 2024 10:22
 Operator : MA/JU
 Sample : PB158293BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK293

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	45	48	57	rVB	37512	53511	0.94%	0.108%
2	3.781	114	118	143	rBV	475573	842047	14.78%	1.696%
3	4.117	171	175	179	rBV2	5981	7963	0.14%	0.016%
4	4.340	209	213	217	rVB7	4205	5856	0.10%	0.012%
5	4.581	250	254	258	rBV7	3404	6800	0.12%	0.014%
6	4.752	279	283	289	rVB7	3024	5856	0.10%	0.012%
7	7.099	672	682	695	rBV	699718	1099300	19.29%	2.214%
8	7.281	706	713	727	rVB	570973	890368	15.63%	1.793%
9	7.464	737	744	757	rVB	670504	1084609	19.04%	2.185%
10	7.940	815	825	833	rBV	518411	818794	14.37%	1.649%
11	8.646	936	945	955	rBV	859355	1366279	23.98%	2.752%
12	9.105	1016	1023	1035	rBV	661290	1122937	19.71%	2.262%
13	9.828	1136	1146	1157	rBV	469137	757185	13.29%	1.525%
14	10.358	1229	1236	1249	rBV	809684	1369727	24.04%	2.759%
15	10.746	1294	1302	1312	rVB	708713	1221350	21.44%	2.460%
16	10.887	1317	1326	1341	rBV	976900	1642091	28.82%	3.307%
17	12.334	1566	1572	1579	rBV	16214	25738	0.45%	0.052%
18	13.487	1759	1768	1773	rBV5	10580	19166	0.34%	0.039%
19	14.004	1847	1856	1863	rBV	1828749	2559697	44.93%	5.156%
20	14.275	1894	1902	1910	rBV	1954035	2878856	50.53%	5.798%
21	14.581	1947	1954	1964	rVB	1201294	1767066	31.01%	3.559%
22	14.781	1980	1988	2000	rBV	798386	1196587	21.00%	2.410%
23	15.575	2116	2123	2131	rBV	2605247	3625430	63.63%	7.302%
24	15.693	2137	2143	2154	rBV	520055	728926	12.79%	1.468%
25	15.816	2159	2164	2171	rVB4	10872	16072	0.28%	0.032%
26	16.363	2253	2257	2260	rBV5	9049	12047	0.21%	0.024%
27	17.334	2415	2422	2430	rBV	1607465	2270045	39.84%	4.572%
28	17.434	2432	2439	2450	rBV	3046499	4149644	72.83%	8.358%
29	19.134	2725	2728	2732	rVB4	7966	9514	0.17%	0.019%
30	19.292	2750	2755	2762	rBV	34651	51674	0.91%	0.104%
31	19.363	2762	2767	2772	rVV	32412	42618	0.75%	0.086%
32	19.734	2823	2830	2839	rVB	3762425	4991212	87.60%	10.053%
33	21.533	3130	3136	3144	rBV	2052290	2723783	47.81%	5.486%
34	22.722	3334	3338	3343	rBV2	47980	66543	1.17%	0.134%
35	22.833	3352	3357	3361	rBV4	23853	44588	0.78%	0.090%
36	23.292	3430	3435	3445	rVB	98301	173489	3.05%	0.349%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029242.D
Acq On : 16 Jan 2024 10:22
Operator : MA/JU
Sample : PB158293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK293

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION

37	23.551	3476	3479	3486	rVB4	34350	54833	0.96%	0.110%
38	23.798	3512	3521	3533	rBV	2867562	5697467	100.00%	11.475%
39	23.951	3538	3547	3563	rVB	1640086	3333757	58.51%	6.715%
40	24.692	3666	3673	3680	rVB	128280	267764	4.70%	0.539%
41	25.569	3815	3822	3831	rVB	128890	317950	5.58%	0.640%
42	26.598	3991	3997	4017	rVB6	82403	299638	5.26%	0.604%
43	27.821	4202	4205	4206	rBV2	28708	30816	0.54%	0.062%




Sum of corrected areas: 49649593

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029242.D
Acq On : 16 Jan 2024 10:22
Operator : MA/JU
Sample : PB158293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK293

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

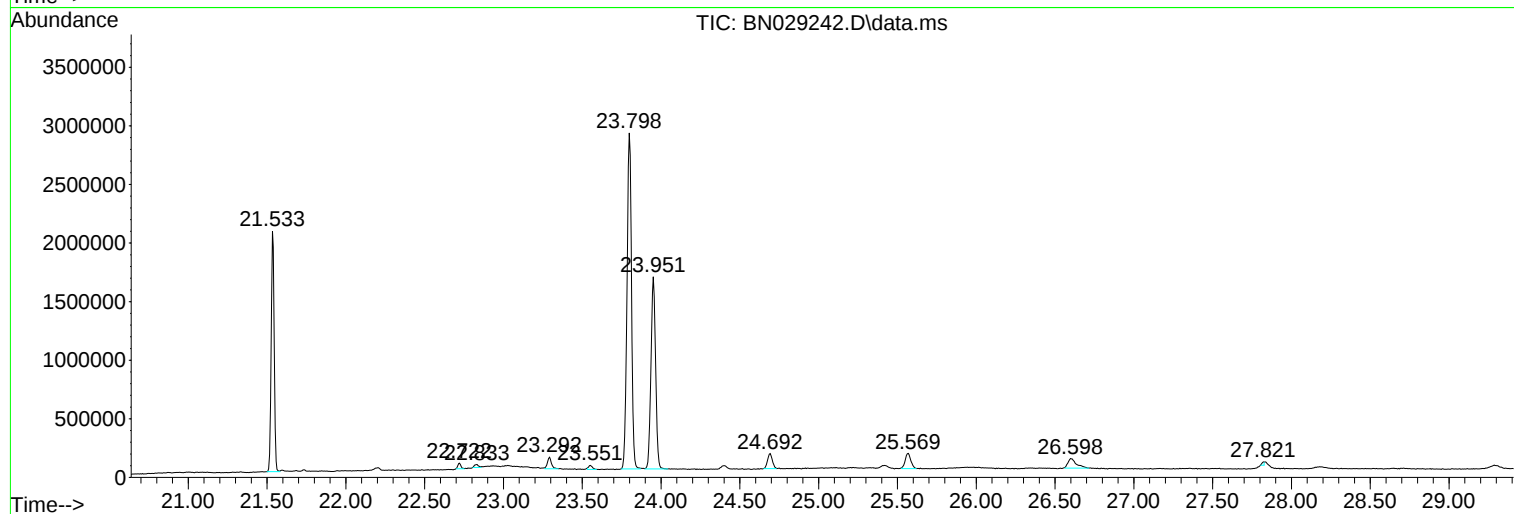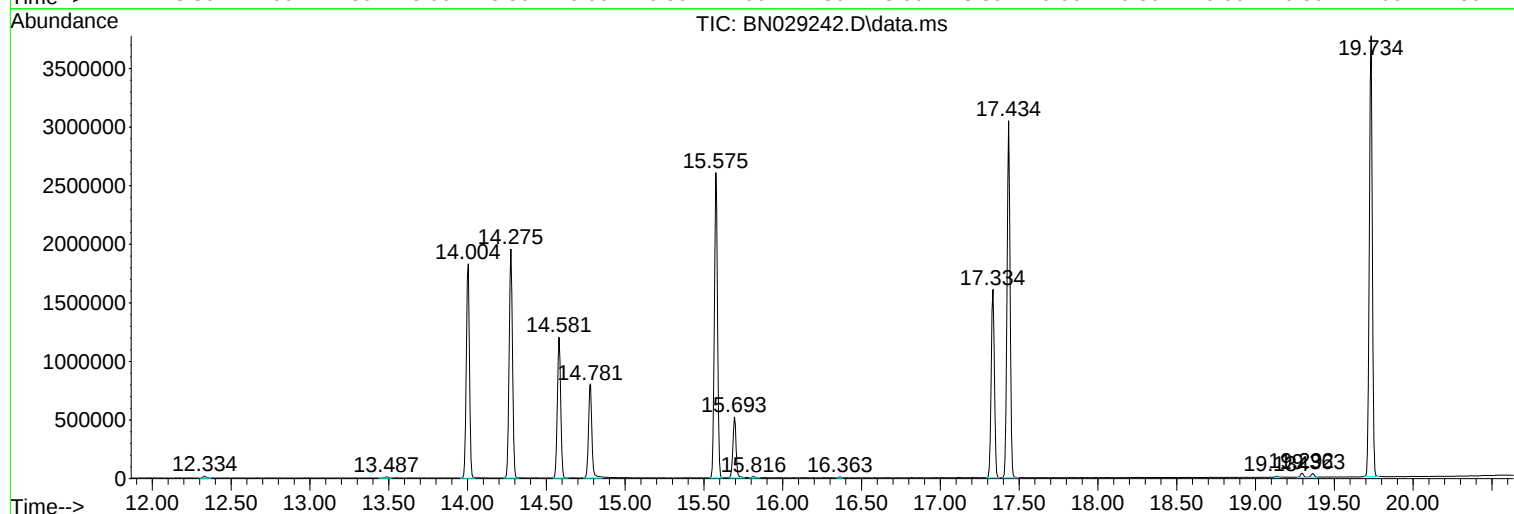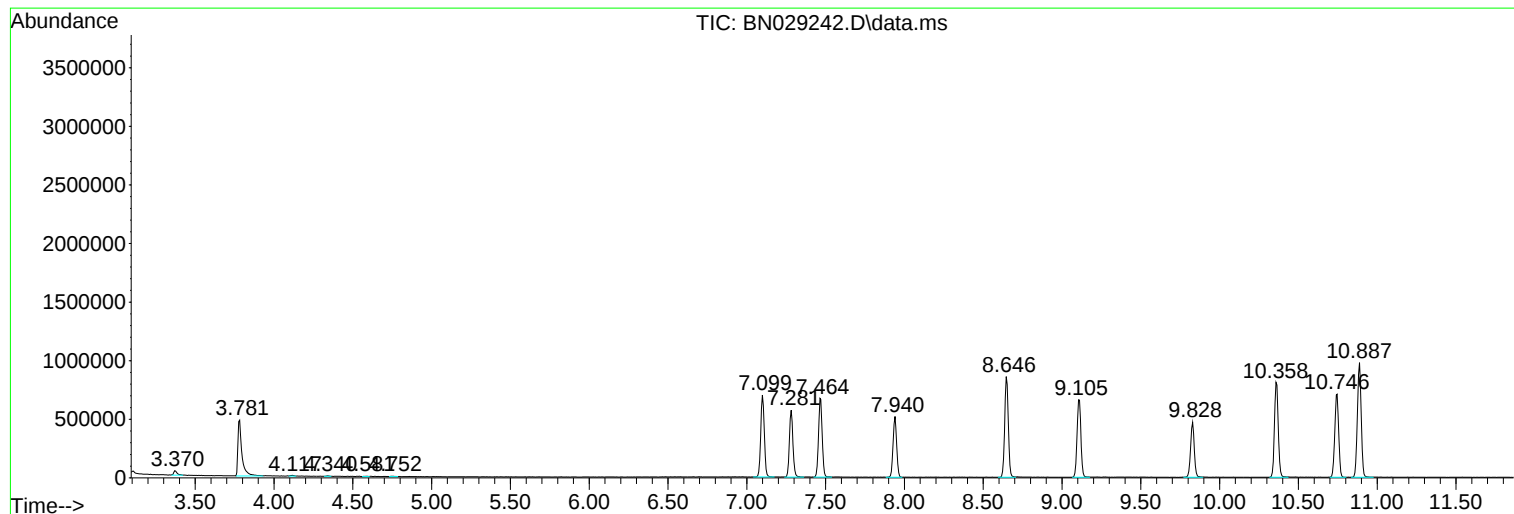

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029242.D
Acq On : 16 Jan 2024 10:22
Operator : MA/JU
Sample : PB158293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK293

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029242.D
Acq On : 16 Jan 2024 10:22
Operator : MA/JU
Sample : PB158293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK293

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------