

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
 Data File : BN029253.D
 Acq On : 16 Jan 2024 17:32
 Operator : MA/JU
 Sample : PB158295BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	56	rBV	30226	48246	1.11%	0.120%
2	3.781	114	118	139	rBV	428350	713027	16.40%	1.770%
3	4.116	171	175	181	rVB4	6256	9093	0.21%	0.023%
4	7.104	675	683	692	rVB	567612	893337	20.55%	2.218%
5	7.281	707	713	726	rBV	451335	722917	16.63%	1.795%
6	7.469	738	745	755	rBV	566440	881575	20.28%	2.189%
7	7.940	818	825	832	rBV	435627	686612	15.79%	1.705%
8	8.651	938	946	955	rBV	689186	1118226	25.72%	2.776%
9	9.110	1014	1024	1034	rBV	561844	918897	21.13%	2.281%
10	9.828	1138	1146	1161	rBV	369298	601187	13.83%	1.493%
11	10.363	1227	1237	1253	rBV	674165	1119140	25.74%	2.779%
12	10.745	1294	1302	1312	rVB	609131	1042414	23.97%	2.588%
13	10.887	1316	1326	1335	rBV	813944	1357366	31.22%	3.370%
14	12.333	1566	1572	1578	rBV2	12166	20371	0.47%	0.051%
15	13.486	1764	1768	1773	rVB3	10348	15417	0.35%	0.038%
16	14.004	1849	1856	1864	rVB	1579103	2178368	50.10%	5.408%
17	14.275	1895	1902	1911	rBV	1666199	2412265	55.48%	5.989%
18	14.580	1947	1954	1963	rVB	1031034	1534375	35.29%	3.810%
19	14.775	1981	1987	2002	rBV	665604	993162	22.84%	2.466%
20	15.575	2115	2123	2131	rBV	2107988	3012451	69.28%	7.479%
21	15.692	2136	2143	2153	rBV	457973	618763	14.23%	1.536%
22	15.816	2161	2164	2168	rVB4	9421	11020	0.25%	0.027%
23	16.357	2252	2256	2264	rVB5	6465	10640	0.24%	0.026%
24	17.110	2381	2384	2387	rBV4	3214	4562	0.10%	0.011%
25	17.333	2415	2422	2428	rBV	1434320	1963722	45.16%	4.875%
26	17.433	2432	2439	2449	rBV2	2501668	3491598	80.30%	8.669%
27	18.068	2543	2547	2552	rVB4	2596	4387	0.10%	0.011%
28	19.292	2751	2755	2761	rVB3	26462	35718	0.82%	0.089%
29	19.363	2763	2767	2773	rVB2	23464	30850	0.71%	0.077%
30	19.727	2823	2829	2839	rVB	3053894	4055243	93.27%	10.068%
31	21.533	3130	3136	3142	rBV	1697024	2201405	50.63%	5.466%
32	22.180	3242	3246	3253	rVB5	24589	46540	1.07%	0.116%
33	22.715	3333	3337	3342	rVB4	23997	37956	0.87%	0.094%
34	22.815	3350	3354	3359	rVB4	39801	68827	1.58%	0.171%
35	23.286	3431	3434	3441	rVB3	33425	52997	1.22%	0.132%
36	23.533	3472	3476	3483	rVB2	45259	85402	1.96%	0.212%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029253.D
Acq On : 16 Jan 2024 17:32
Operator : MA/JU
Sample : PB158295BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK295

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION

37	23.792	3511	3520	3531	rBV2	2207135	4348049	100.00%	10.795%
38	23.945	3537	3546	3561	rBV	1230904	2533534	58.27%	6.290%
39	24.386	3616	3621	3627	rVB2	45249	92776	2.13%	0.230%
40	24.680	3667	3671	3678	rVB4	48594	96232	2.21%	0.239%
41	25.398	3788	3793	3803	rVB5	41424	104350	2.40%	0.259%
42	25.556	3816	3820	3828	rVB4	46458	104563	2.40%	0.260%




Sum of corrected areas: 40277580

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029253.D
Acq On : 16 Jan 2024 17:32
Operator : MA/JU
Sample : PB158295BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

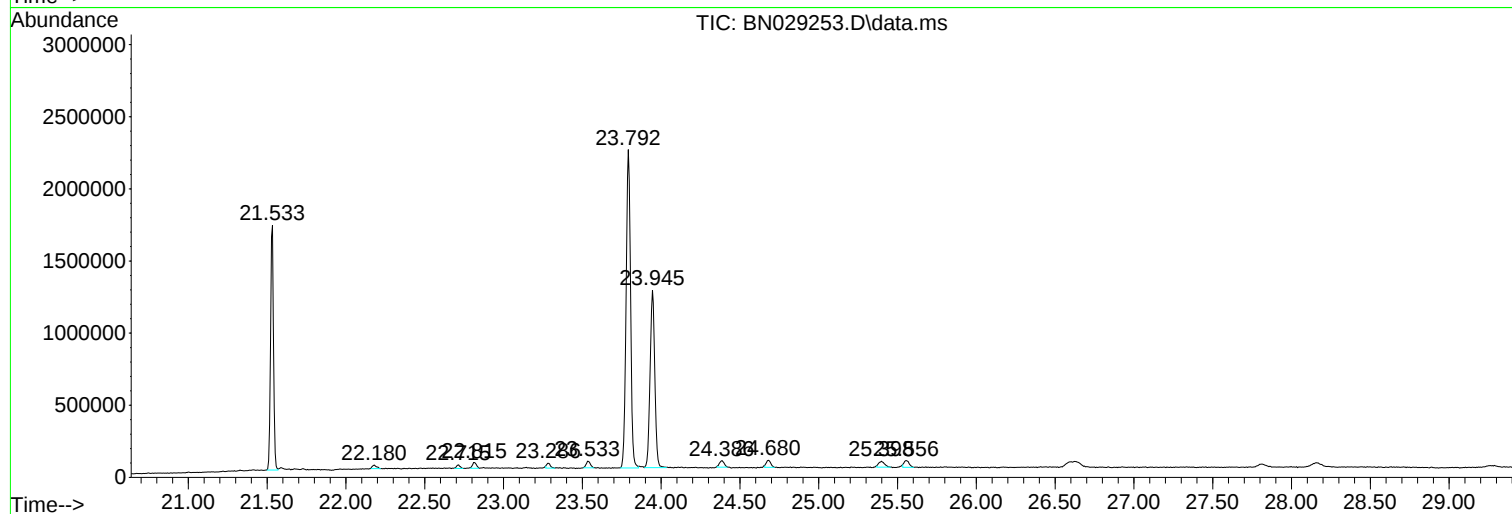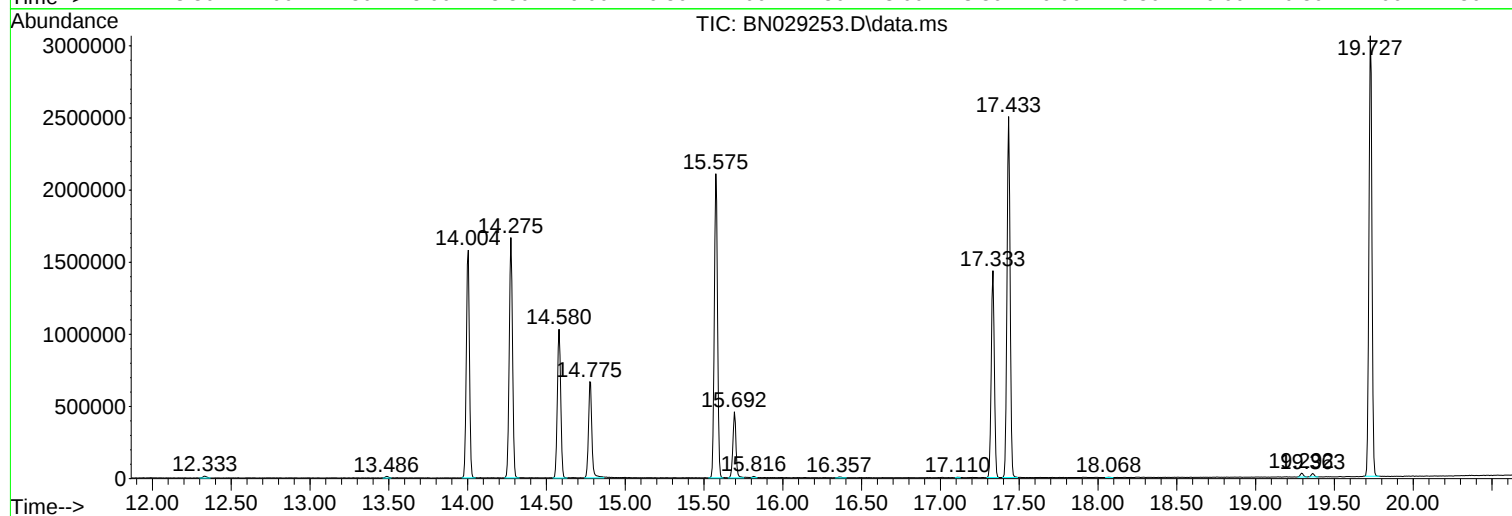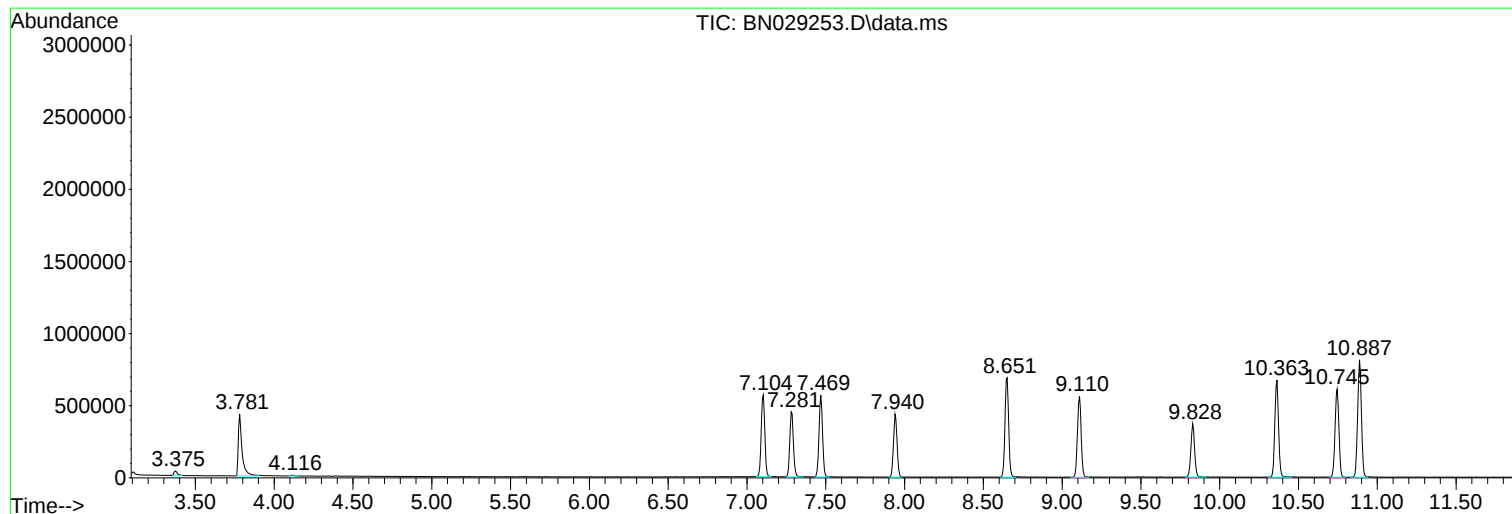

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029253.D
Acq On : 16 Jan 2024 17:32
Operator : MA/JU
Sample : PB158295BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029253.D
Acq On : 16 Jan 2024 17:32
Operator : MA/JU
Sample : PB158295BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc