

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
 Data File : BN029256.D
 Acq On : 16 Jan 2024 19:20
 Operator : MA/JU
 Sample : PB158396BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK396

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	59	rVB	31764	50415	1.18%	0.128%
2	3.781	114	118	138	rBV	415200	699916	16.32%	1.782%
3	4.111	171	174	181	rVB3	7070	12351	0.29%	0.031%
4	7.105	673	683	694	rBV	551928	895324	20.87%	2.279%
5	7.281	707	713	727	rBV	448447	717548	16.73%	1.827%
6	7.469	737	745	752	rBV	560586	868014	20.24%	2.210%
7	7.940	819	825	833	rVB	426042	675888	15.76%	1.721%
8	8.646	937	945	957	rBV	675523	1100852	25.67%	2.802%
9	9.110	1015	1024	1036	rBV	555637	910900	21.24%	2.319%
10	9.828	1136	1146	1157	rBV	361094	593199	13.83%	1.510%
11	10.363	1229	1237	1250	rBV	660798	1098665	25.62%	2.797%
12	10.746	1294	1302	1310	rBV	609409	1016779	23.71%	2.588%
13	10.887	1318	1326	1337	rBV	792563	1321920	30.82%	3.365%
14	12.328	1567	1571	1579	rVB	11328	18154	0.42%	0.046%
15	13.487	1762	1768	1775	rVV2	15761	25109	0.59%	0.064%
16	14.004	1848	1856	1862	rBV	1511538	2097241	48.90%	5.339%
17	14.275	1895	1902	1909	rBV	1609240	2337206	54.49%	5.950%
18	14.581	1947	1954	1962	rVB	1002033	1483177	34.58%	3.776%
19	14.775	1980	1987	2001	rBV	672416	980194	22.85%	2.495%
20	15.575	2116	2123	2131	rBV	2106139	2955642	68.91%	7.524%
21	15.692	2137	2143	2154	rBV	430434	596835	13.92%	1.519%
22	15.822	2160	2165	2168	rVB4	6359	10021	0.23%	0.026%
23	16.363	2253	2257	2263	rVB6	6218	9887	0.23%	0.025%
24	17.334	2415	2422	2430	rBV	1371180	1912765	44.60%	4.869%
25	17.434	2432	2439	2448	rBV	2396330	3398920	79.25%	8.652%
26	18.245	2573	2577	2579	rBV3	3345	4491	0.10%	0.011%
27	19.292	2751	2755	2759	rBV2	25765	33780	0.79%	0.086%
28	19.363	2762	2767	2772	rVB	25017	34883	0.81%	0.089%
29	19.533	2793	2796	2801	rBV6	4005	5935	0.14%	0.015%
30	19.728	2823	2829	2840	rVB	2980919	3992983	93.10%	10.165%
31	21.533	3130	3136	3143	rBV	1675589	2151063	50.15%	5.476%
32	22.174	3242	3245	3247	rBV2	17733	21774	0.51%	0.055%
33	22.716	3333	3337	3342	rVB2	28044	39000	0.91%	0.099%
34	23.280	3430	3433	3440	rVB	49171	76386	1.78%	0.194%
35	23.533	3474	3476	3483	rVB6	30732	50056	1.17%	0.127%
36	23.792	3512	3520	3534	rBV2	2193874	4289029	100.00%	10.918%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029256.D
Acq On : 16 Jan 2024 19:20
Operator : MA/JU
Sample : PB158396BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK396

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION

37	23.945	3538	3546	3555	rVV	1235293	2509385	58.51%	6.388%
38	24.680	3666	3671	3679	rVB4	63445	135252	3.15%	0.344%
39	25.557	3816	3820	3832	rVB3	65425	152233	3.55%	0.388%




Sum of corrected areas: 39283172

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029256.D
Acq On : 16 Jan 2024 19:20
Operator : MA/JU
Sample : PB158396BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK396

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

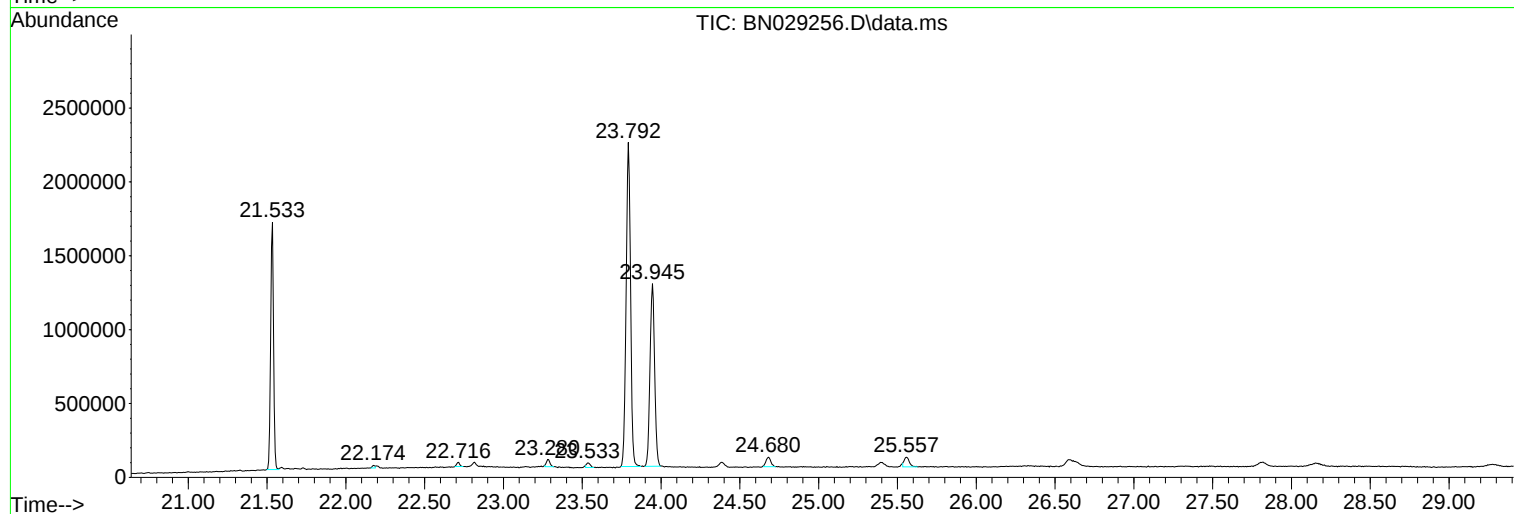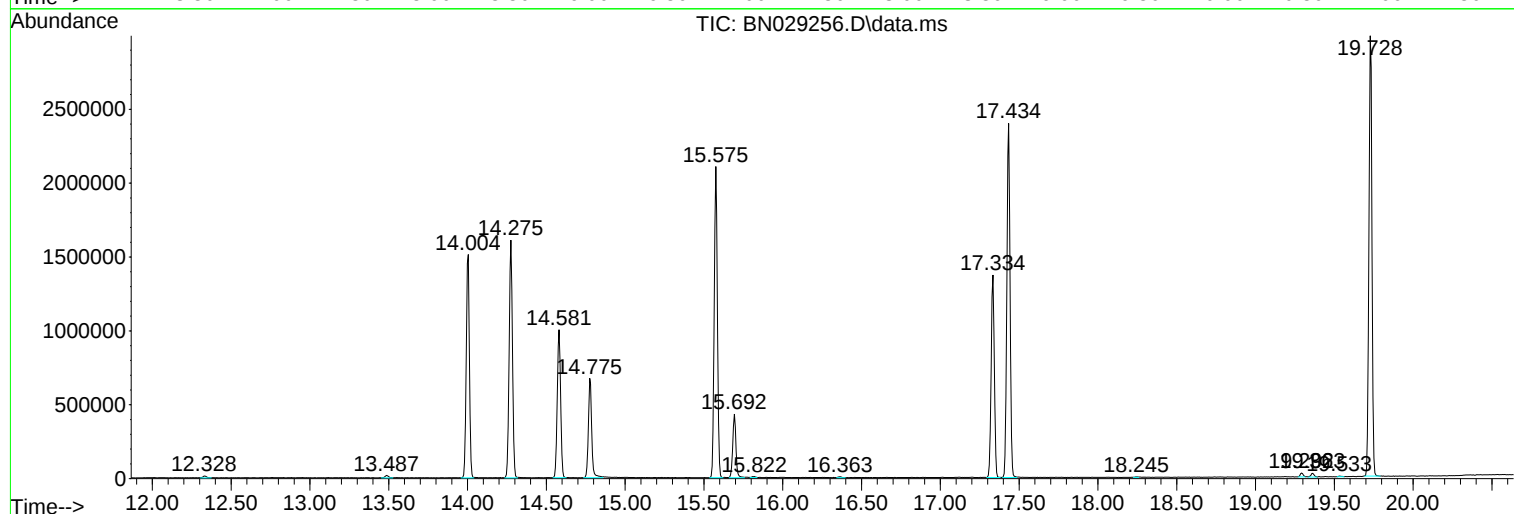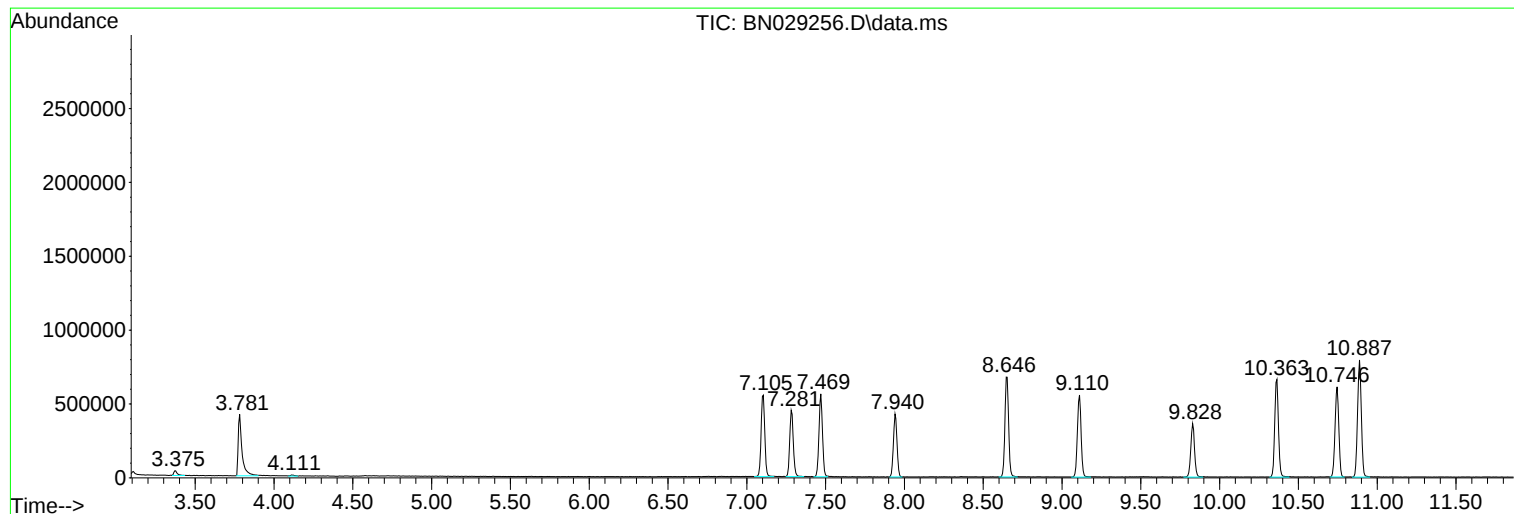

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029256.D
Acq On : 16 Jan 2024 19:20
Operator : MA/JU
Sample : PB158396BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK396

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029256.D
Acq On : 16 Jan 2024 19:20
Operator : MA/JU
Sample : PB158396BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK396

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------