

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
 Data File : BN029257.D
 Acq On : 16 Jan 2024 19:57
 Operator : MA/JU
 Sample : PB158397BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK397

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	54	rBV	30367	41604	0.95%	0.105%
2	3.781	114	118	138	rBV	406440	689083	15.79%	1.733%
3	4.117	171	175	180	rVV2	5641	9479	0.22%	0.024%
4	7.099	673	682	689	rBV	548078	878988	20.14%	2.210%
5	7.281	707	713	724	rVB	455584	706435	16.19%	1.776%
6	7.469	737	745	753	rBV	553939	867363	19.87%	2.181%
7	7.940	819	825	835	rVB	435435	696089	15.95%	1.750%
8	8.646	938	945	953	rBV	670763	1091203	25.00%	2.744%
9	9.110	1016	1024	1033	rBV	551226	906174	20.76%	2.279%
10	9.828	1134	1146	1155	rBV	365802	595630	13.65%	1.498%
11	10.363	1228	1237	1245	rBV	646743	1088476	24.94%	2.737%
12	10.746	1294	1302	1310	rVV	622878	1053108	24.13%	2.648%
13	10.887	1319	1326	1337	rBV	783555	1321834	30.29%	3.324%
14	12.334	1567	1572	1576	rBV	11905	16830	0.39%	0.042%
15	13.487	1762	1768	1774	rBV	12703	19608	0.45%	0.049%
16	14.004	1849	1856	1865	rBV	1518265	2110398	48.36%	5.307%
17	14.275	1895	1902	1910	rBV	1598967	2338748	53.59%	5.881%
18	14.581	1947	1954	1962	rVB	1063369	1540535	35.30%	3.874%
19	14.775	1981	1987	2001	rBV	657112	971815	22.27%	2.444%
20	15.575	2116	2123	2131	rBV	2099523	2951053	67.62%	7.420%
21	15.692	2137	2143	2153	rBV	434378	600349	13.76%	1.510%
22	15.816	2160	2164	2169	rVB4	8499	10672	0.24%	0.027%
23	16.363	2252	2257	2260	rBV4	5512	8341	0.19%	0.021%
24	17.116	2380	2385	2388	rBV7	3362	5422	0.12%	0.014%
25	17.333	2415	2422	2429	rBV	1431135	1989406	45.59%	5.002%
26	17.433	2432	2439	2453	rVB	2391288	3404228	78.00%	8.560%
27	19.292	2750	2755	2760	rVB2	26207	34415	0.79%	0.087%
28	19.363	2762	2767	2773	rVV	24181	31094	0.71%	0.078%
29	19.727	2823	2829	2836	rVV	3055698	4028598	92.31%	10.130%
30	21.533	3130	3136	3142	rBV	1728902	2247848	51.51%	5.652%
31	22.710	3333	3336	3341	rVB2	32631	44411	1.02%	0.112%
32	23.280	3430	3433	3446	rVB	61606	113353	2.60%	0.285%
33	23.792	3511	3520	3535	rBV	2269608	4364134	100.00%	10.974%
34	23.945	3538	3546	3559	rVB	1268443	2660590	60.96%	6.690%
35	24.674	3665	3670	3681	rVB2	74711	163204	3.74%	0.410%
36	25.557	3814	3820	3829	rVB3	68924	169111	3.88%	0.425%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029257.D
Acq On : 16 Jan 2024 19:57
Operator : MA/JU
Sample : PB158397BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK397

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 39769629

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029257.D
Acq On : 16 Jan 2024 19:57
Operator : MA/JU
Sample : PB158397BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK397

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

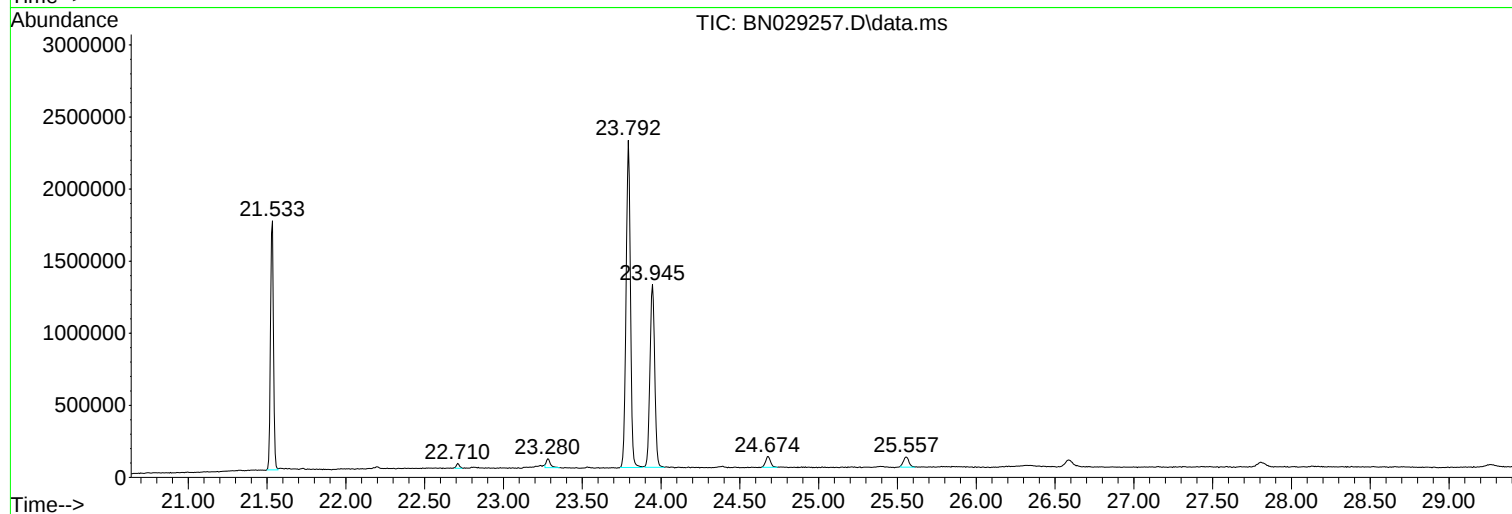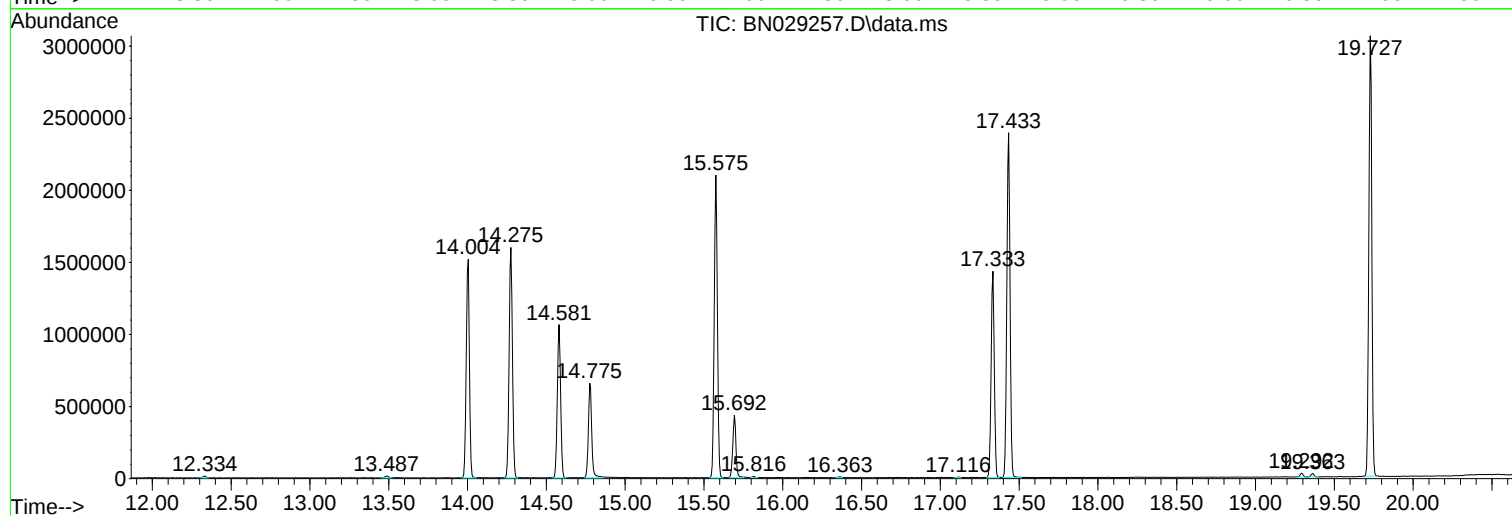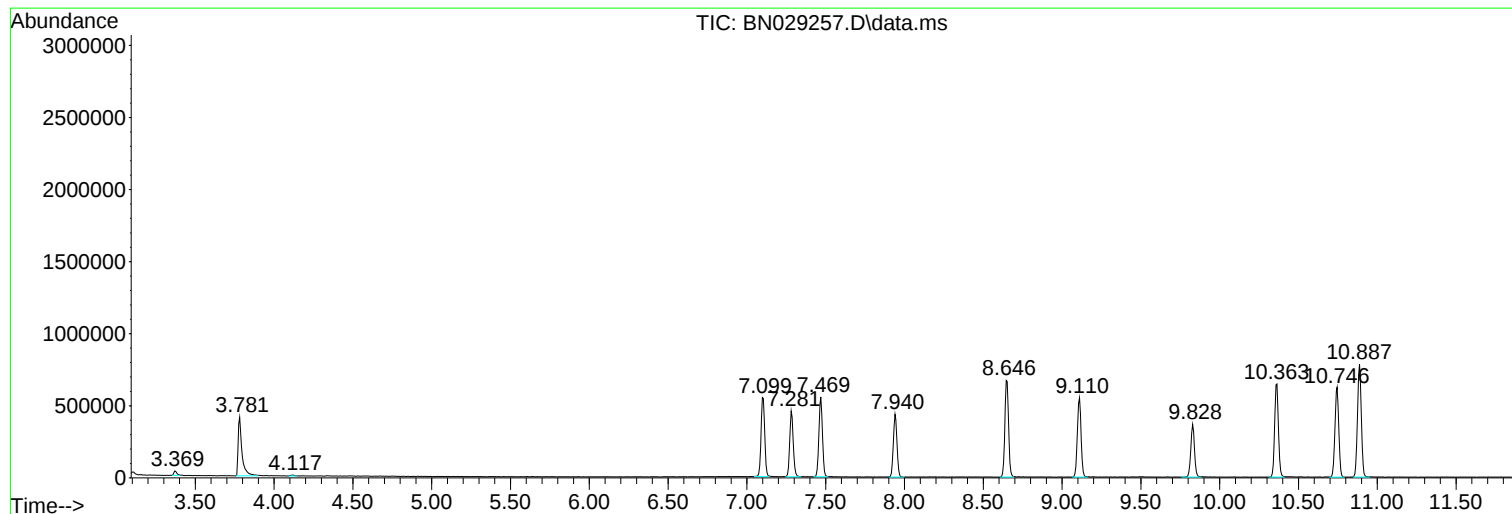

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029257.D
Acq On : 16 Jan 2024 19:57
Operator : MA/JU
Sample : PB158397BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK397

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029257.D
Acq On : 16 Jan 2024 19:57
Operator : MA/JU
Sample : PB158397BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK397

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------