

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
 Data File : BN029258.D
 Acq On : 16 Jan 2024 20:33
 Operator : MA/JU
 Sample : PB158339BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK339

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	54	rBV	33729	46935	0.99%	0.111%
2	3.781	114	118	138	rBV	454201	750969	15.83%	1.780%
3	4.116	172	175	180	rVB3	7213	10336	0.22%	0.024%
4	7.105	675	683	691	rBV	603102	963042	20.30%	2.282%
5	7.281	707	713	727	rVB	482186	773388	16.30%	1.833%
6	7.469	737	745	753	rBV	595586	945647	19.94%	2.241%
7	7.940	818	825	834	rVB	440937	699317	14.74%	1.657%
8	8.651	938	946	955	rBV	738518	1200828	25.32%	2.846%
9	9.110	1015	1024	1038	rBV	615524	1005400	21.20%	2.382%
10	9.828	1137	1146	1157	rBV	408197	666019	14.04%	1.578%
11	10.363	1229	1237	1247	rBV	718423	1199018	25.28%	2.841%
12	10.745	1294	1302	1310	rBV	633202	1060107	22.35%	2.512%
13	10.887	1317	1326	1337	rBV	879934	1463552	30.85%	3.468%
14	12.334	1564	1572	1579	rBV	13910	25221	0.53%	0.060%
15	13.487	1763	1768	1772	rBV3	9097	14534	0.31%	0.034%
16	14.004	1849	1856	1865	rBV	1676348	2331172	49.15%	5.524%
17	14.275	1895	1902	1911	rBV	1793496	2554384	53.85%	6.053%
18	14.581	1947	1954	1966	rVB	1077134	1563730	32.97%	3.705%
19	14.775	1981	1987	2002	rBV	727539	1101057	23.21%	2.609%
20	15.575	2116	2123	2130	rBV	2333390	3263809	68.81%	7.734%
21	15.692	2137	2143	2155	rBV	502696	680775	14.35%	1.613%
22	15.816	2160	2164	2168	rVB3	8214	10920	0.23%	0.026%
23	16.363	2253	2257	2265	rBV7	7793	11600	0.24%	0.027%
24	17.333	2415	2422	2430	rVB	1459081	2002853	42.22%	4.746%
25	17.433	2432	2439	2451	rVV	2707917	3740384	78.85%	8.863%
26	19.292	2751	2755	2760	rVB3	28985	40083	0.85%	0.095%
27	19.363	2760	2767	2772	rBV	28626	41035	0.87%	0.097%
28	19.733	2823	2830	2841	rVB	3127182	4389434	92.54%	10.401%
29	21.533	3130	3136	3143	rBV	1722905	2227198	46.95%	5.278%
30	22.715	3333	3337	3340	rBV5	17234	23970	0.51%	0.057%
31	23.280	3431	3433	3442	rVB7	27371	41395	0.87%	0.098%
32	23.792	3511	3520	3536	rBV2	2381682	4743382	100.00%	11.240%
33	23.945	3538	3546	3558	rVB	1215082	2542523	53.60%	6.025%
34	24.674	3666	3670	3678	rVB4	31180	66645	1.41%	0.158%

Sum of corrected areas: 42200662

Instrument :

BNA_N

ClientSampleId :




SBLK339

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029258.D
Acq On : 16 Jan 2024 20:33
Operator : MA/JU
Sample : PB158339BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK339

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

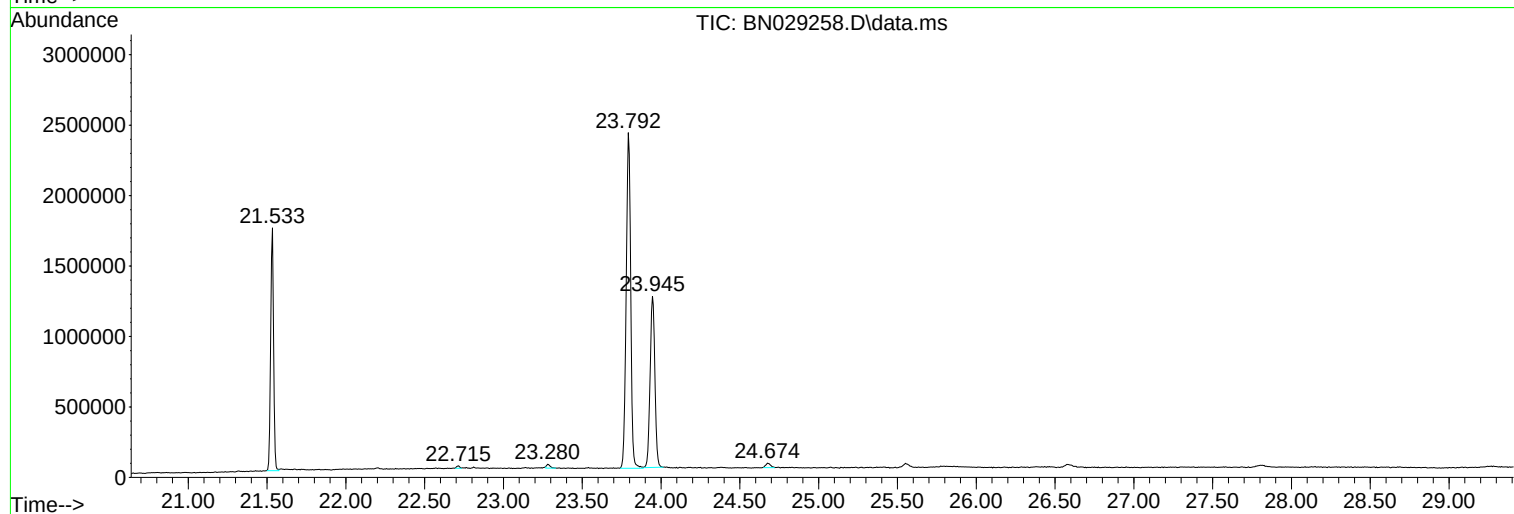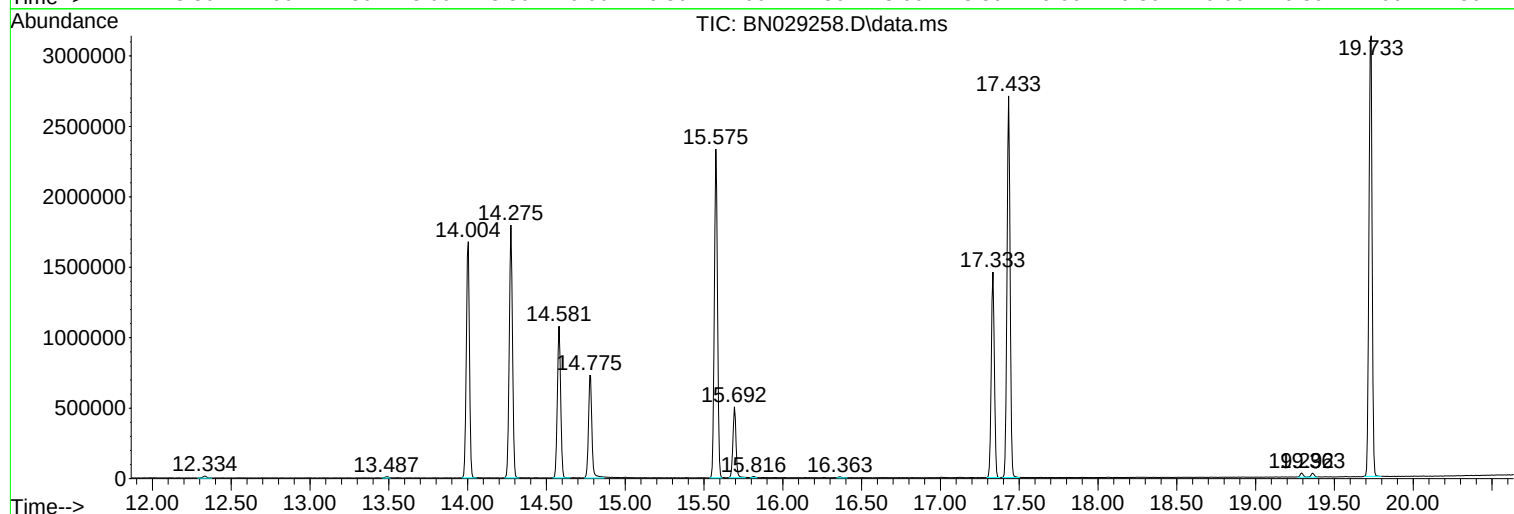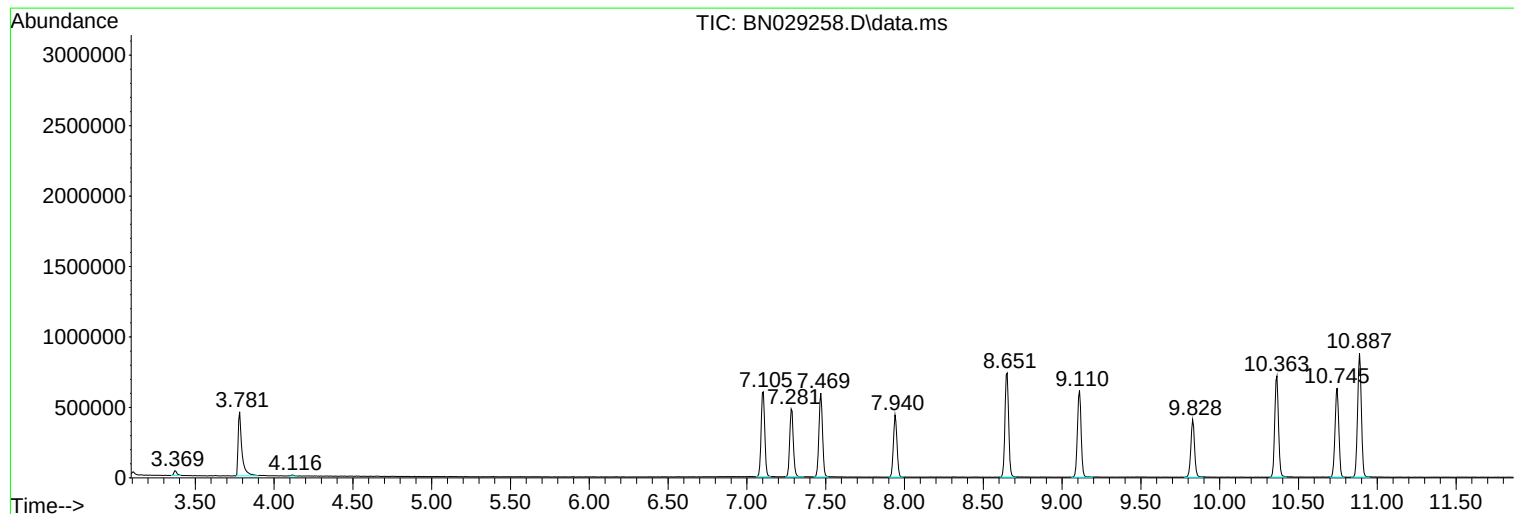

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029258.D
Acq On : 16 Jan 2024 20:33
Operator : MA/JU
Sample : PB158339BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK339

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011624\
Data File : BN029258.D
Acq On : 16 Jan 2024 20:33
Operator : MA/JU
Sample : PB158339BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK339

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc