

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011625\
 Data File : BN035940.D
 Acq On : 16 Jan 2025 11:42
 Operator : RC/JU
 Sample : Q1084-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BA2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/16/2025
 Supervised By :mohammad ahmed 01/20/2025

Quant Time: Jan 16 12:16:20 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 10:40:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	2621	0.400	ng/ul	0.00
4) Naphthalene-d8	10.622	136	5411	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.464	164	3079	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.204	188	6272m	0.400	ng/ul	0.00
17) Chrysene-d12	21.377	240	4774	0.400	ng/ul	0.00
23) Perylene-d12	23.681	264	4209m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	14515	5.493	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.211	152	2625	0.373	ng/ul	0.00
18) Fluoranthene-d10	19.229	212	6152	0.487	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.318	88	4027	1.399	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011625\
Data File : BN035940.D
Acq On : 16 Jan 2025 11:42
Operator : RC/JU
Sample : Q1084-03
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0BA2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/16/2025
Supervised By :mohammad ahmed 01/20/2025


Quant Time: Jan 16 12:16:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 10:40:45 2025
Response via : Initial Calibration

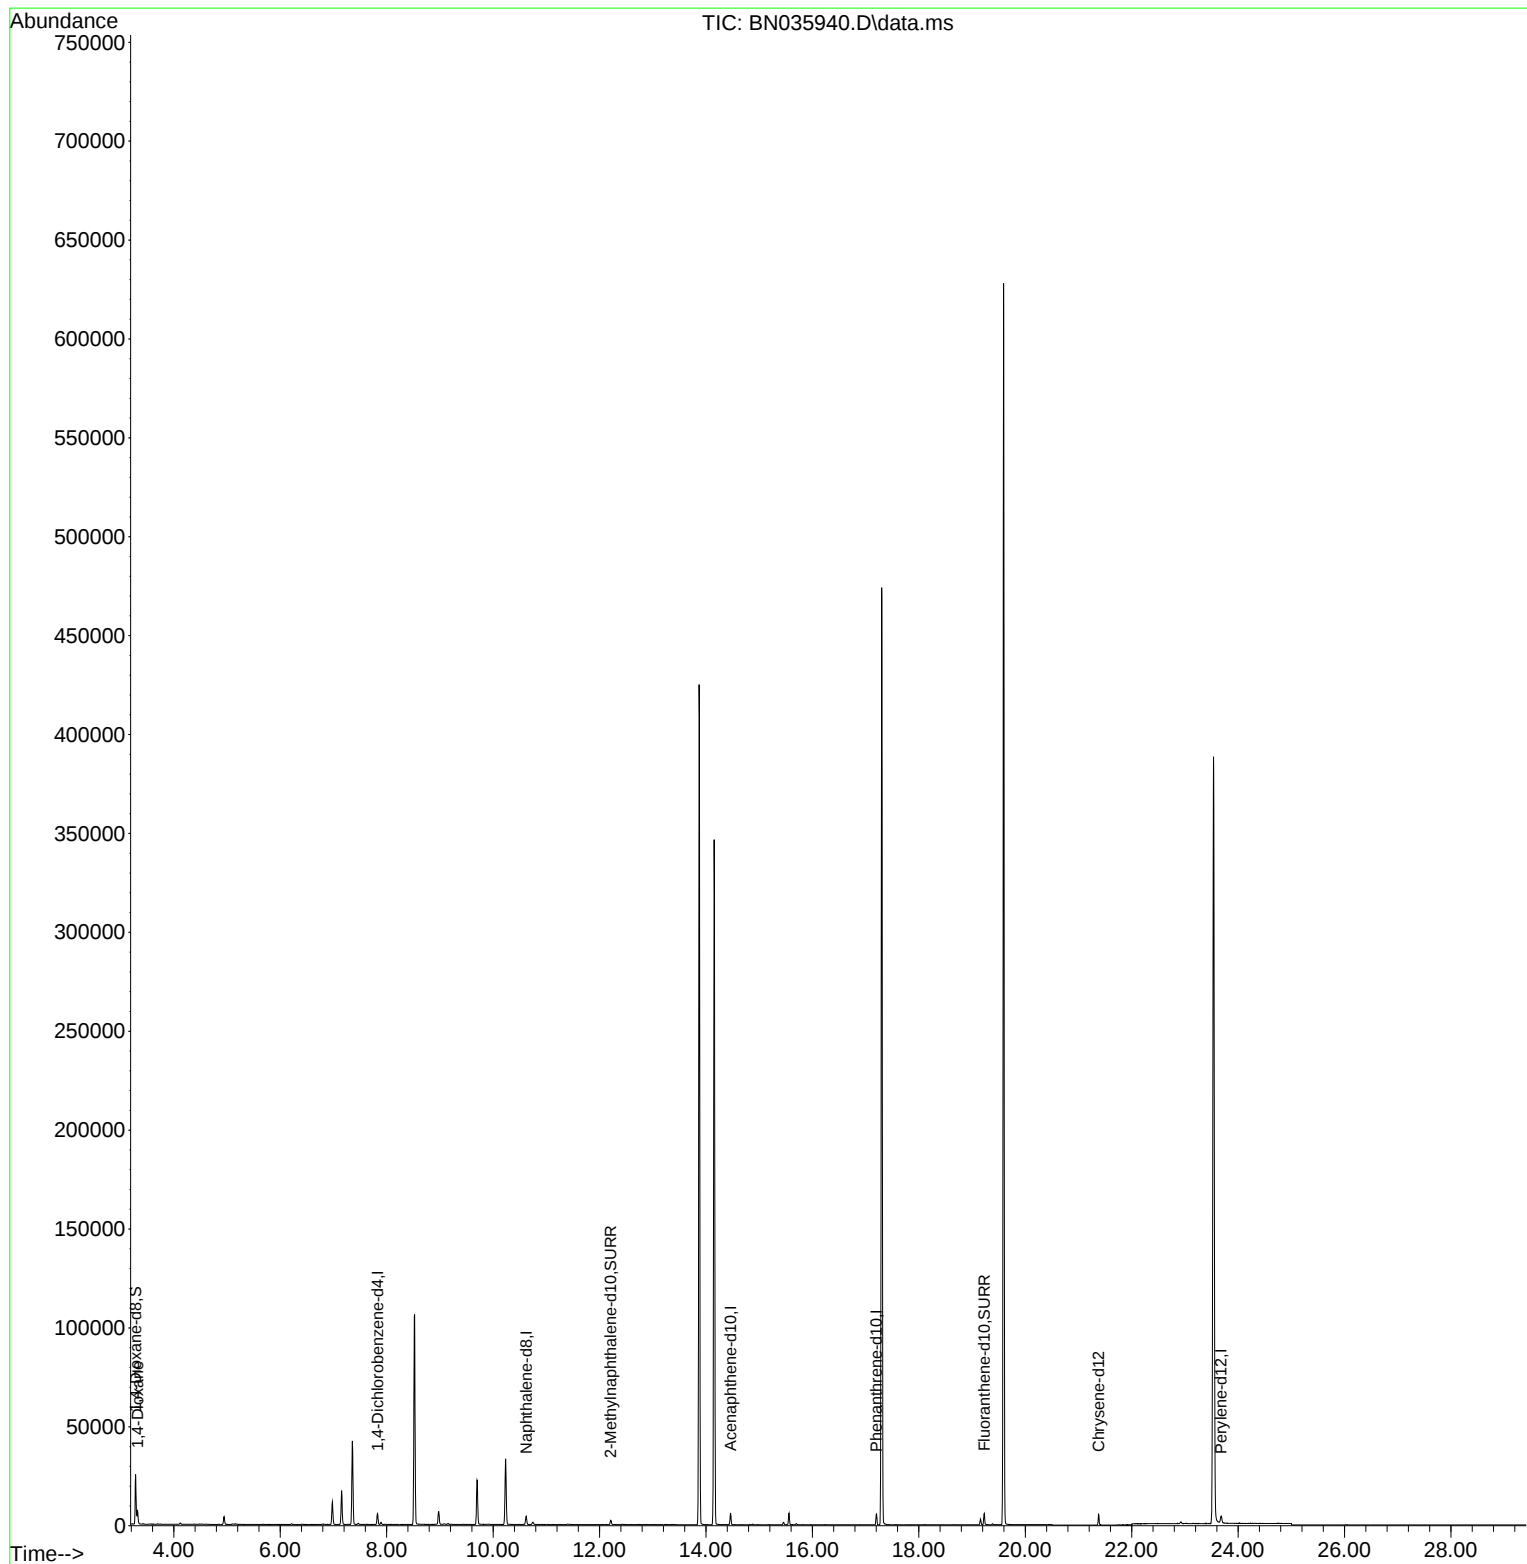

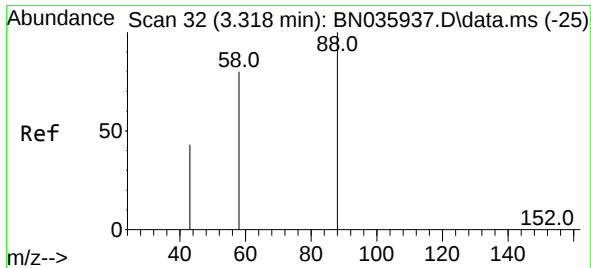

#2
 1,4-Dioxane
 Concen: 1.399 ng/ul
 RT: 3.318 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN035940.D
 Acq: 16 Jan 2025 11:42

Instrument :
 BNA_N
 ClientSampleId :
 C0BA2

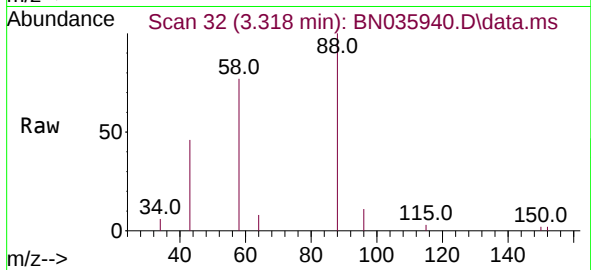

Tgt Ion: 88 Resp: 402
 Ion Ratio Lower Upper
 88 100
 43 45.6 57.8 86.8
 58 76.7 60.0 90.0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/16/2025
 Supervised By :mohammad ahmed 01/20/2025

