
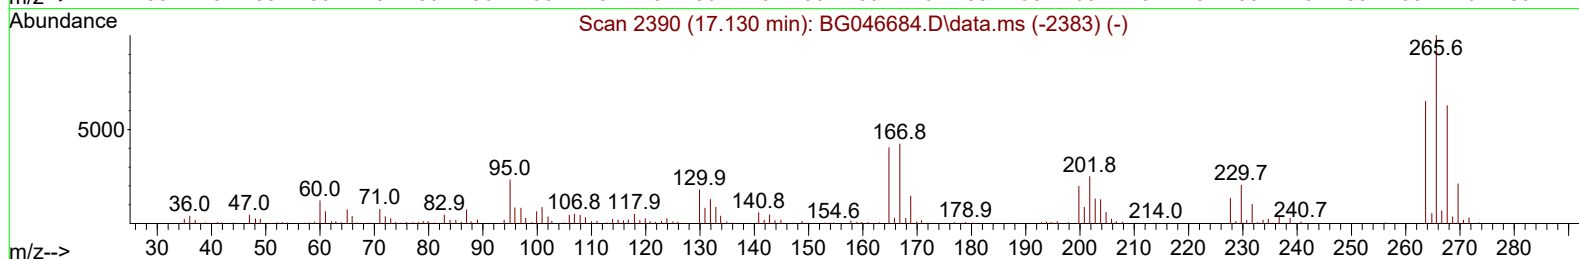
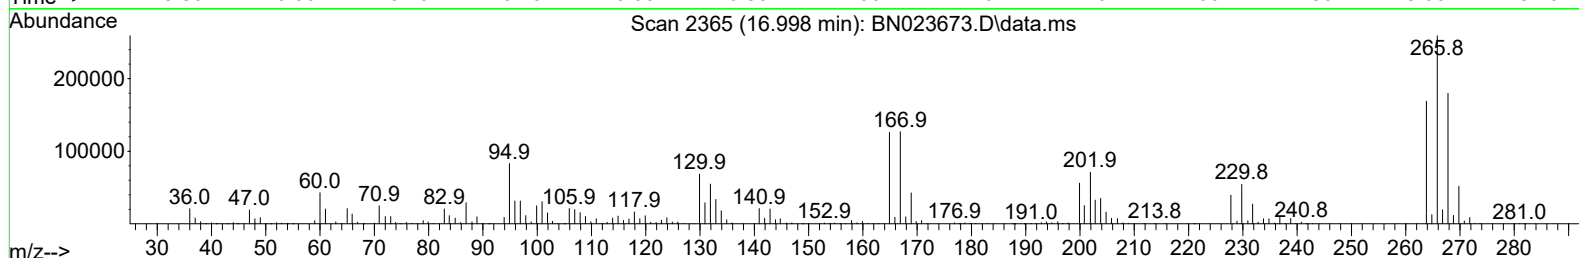


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
Data File : BN023673.D
Acq On : 17 Jan 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:10:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 07:10:10 2023
Response via : Initial Calibration

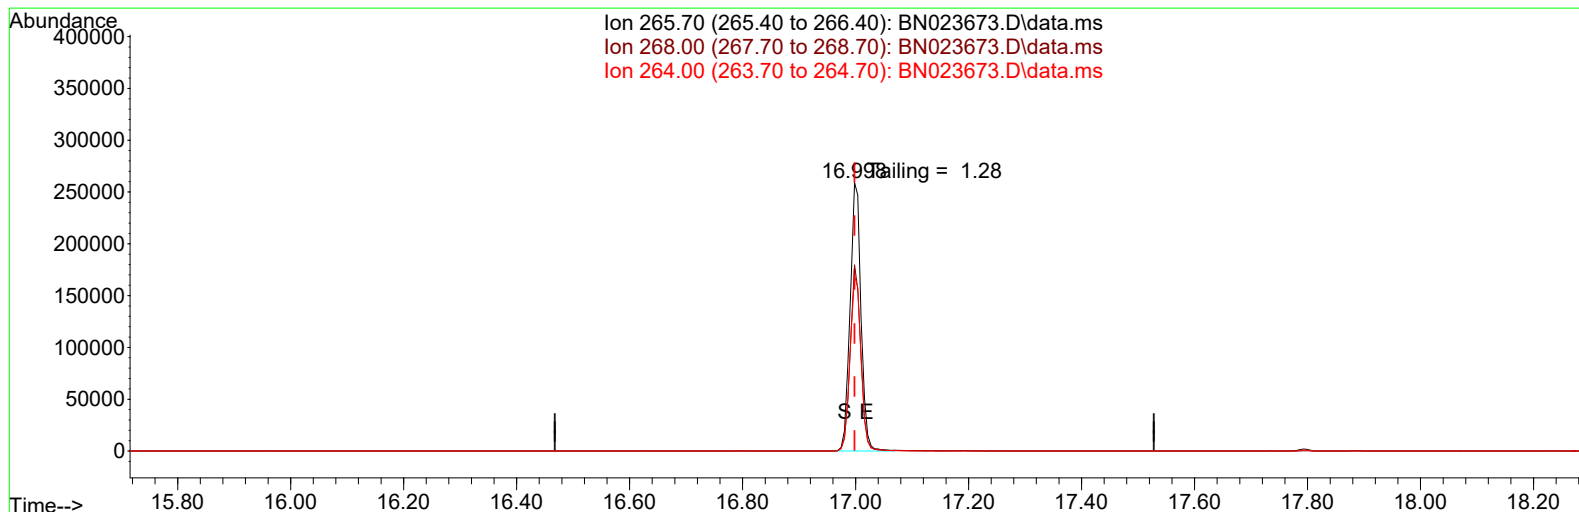

TIC: BN023673.D\data.ms

(70) Pentachlorophenol (C)




16.998min (0.000) 8414.73 ng

response 350721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.37
264.00	61.60	65.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
Data File : BN023673.D
Acq On : 17 Jan 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:10:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 07:10:10 2023
Response via : Initial Calibration

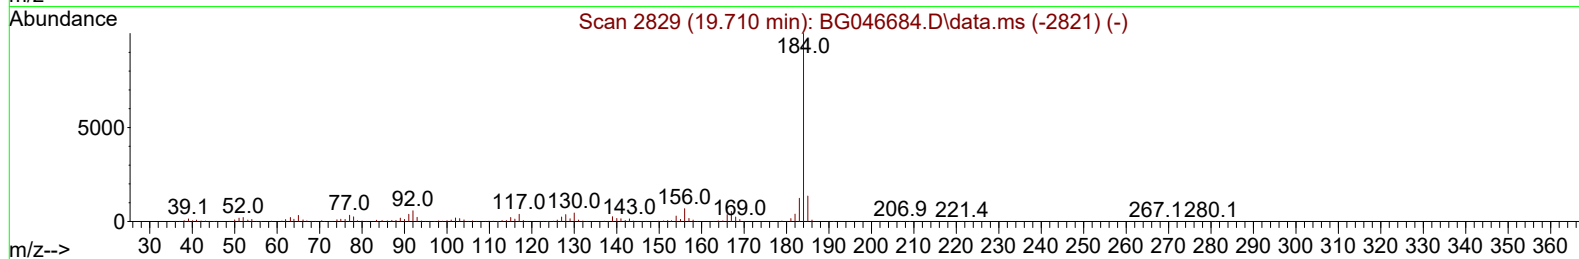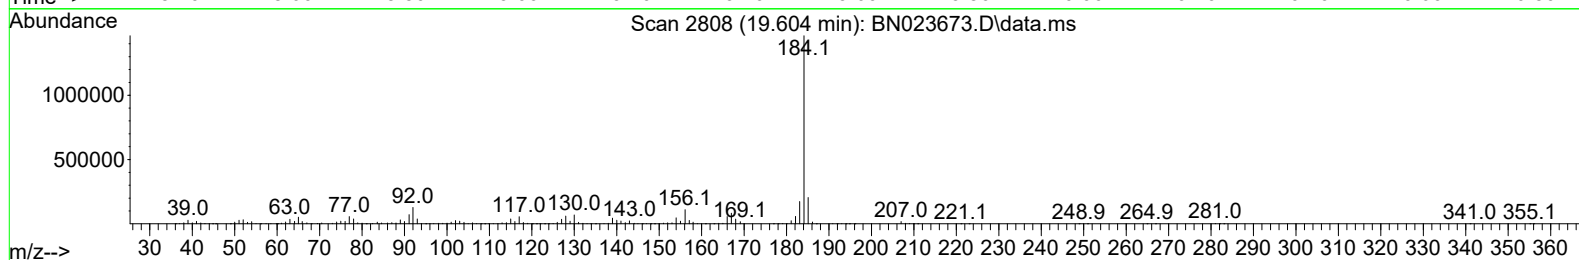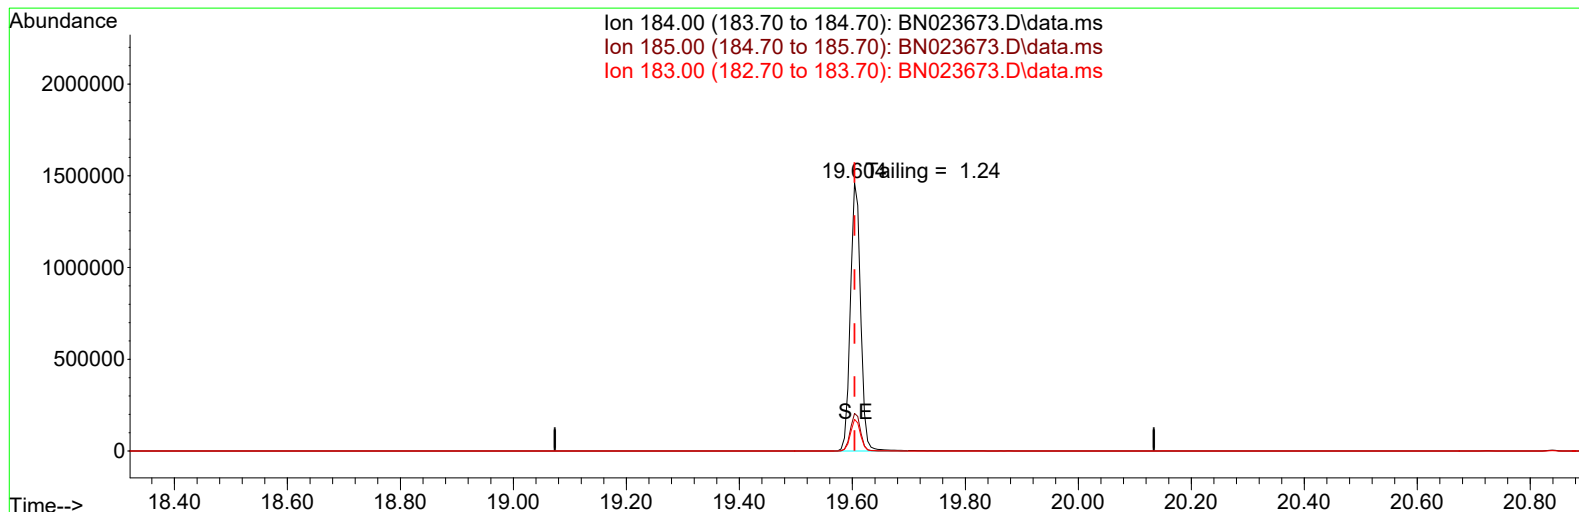

TIC: BN023673.D\data.ms

(77) Benzidine

19.604min (0.000) 0.00 ng

response 1851414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	11.84
0.00	0.00	0.00