
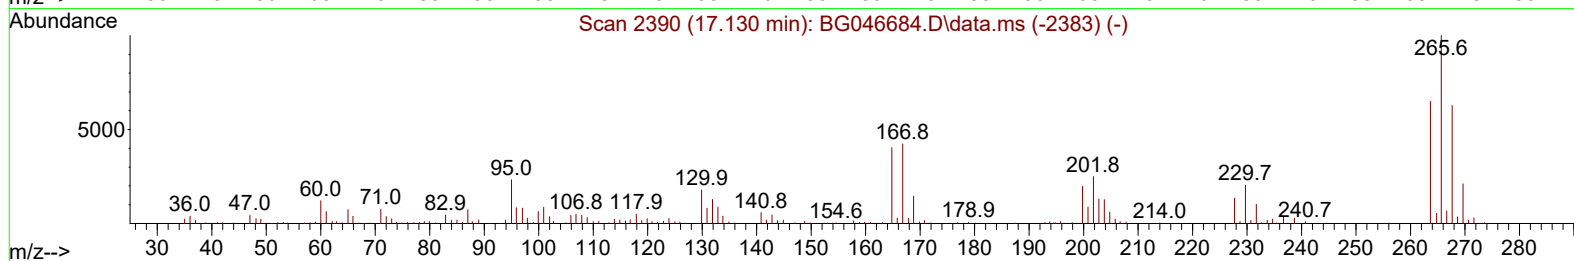
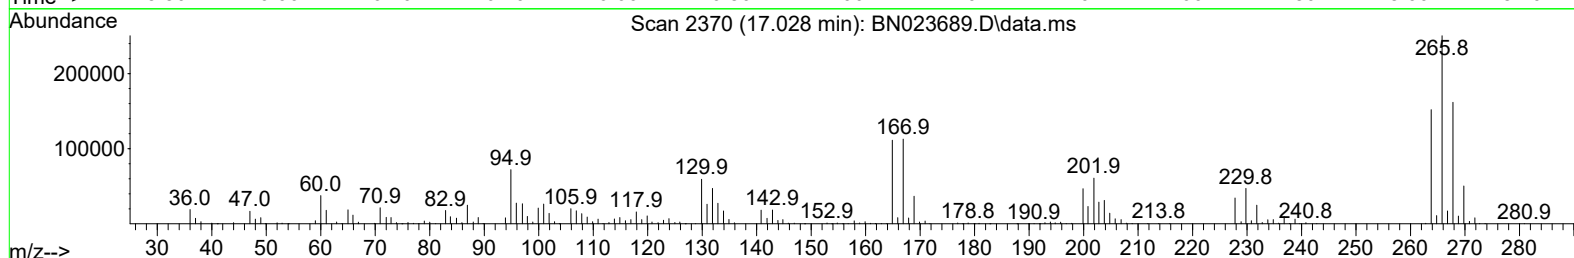


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
 Data File : BN023689.D
 Acq On : 17 Jan 2023 19:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:11:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 18 07:11:53 2023
 Response via : Initial Calibration

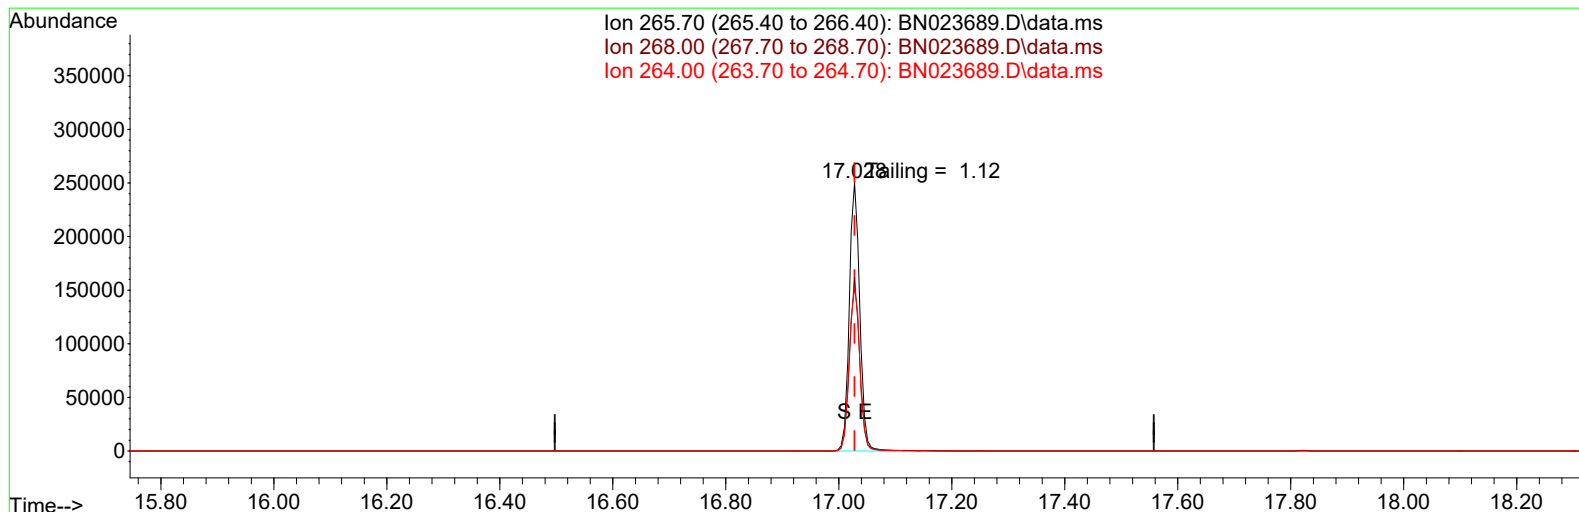

TIC: BN023689.D\data.ms

(70) Pentachlorophenol (C)




17.028min (0.000) 20868.15 ng

response 323278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.62
264.00	61.60	60.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
Data File : BN023689.D
Acq On : 17 Jan 2023 19:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:11:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 07:11:53 2023
Response via : Initial Calibration

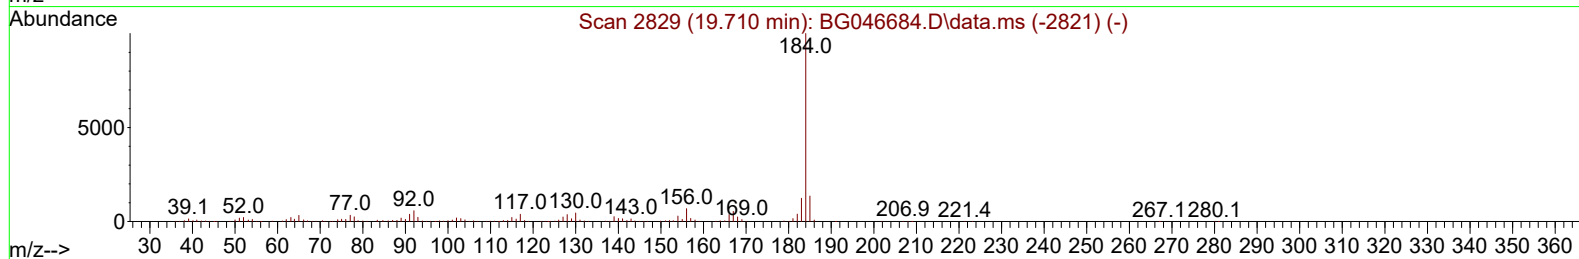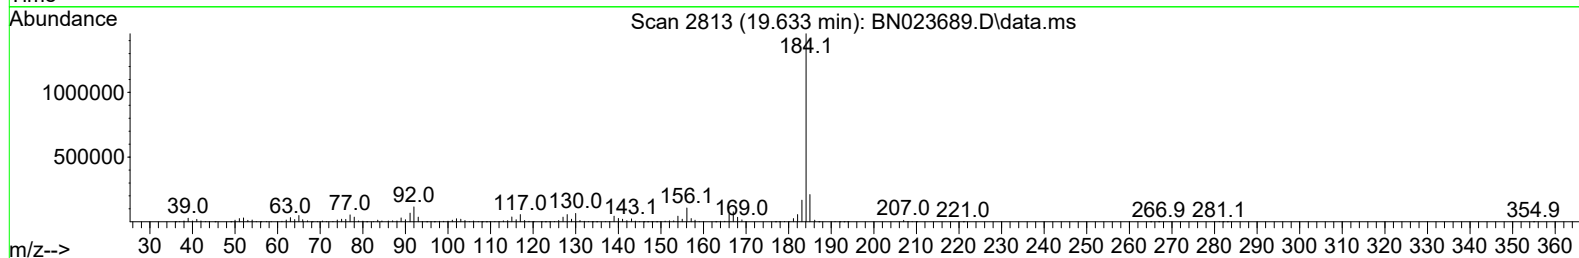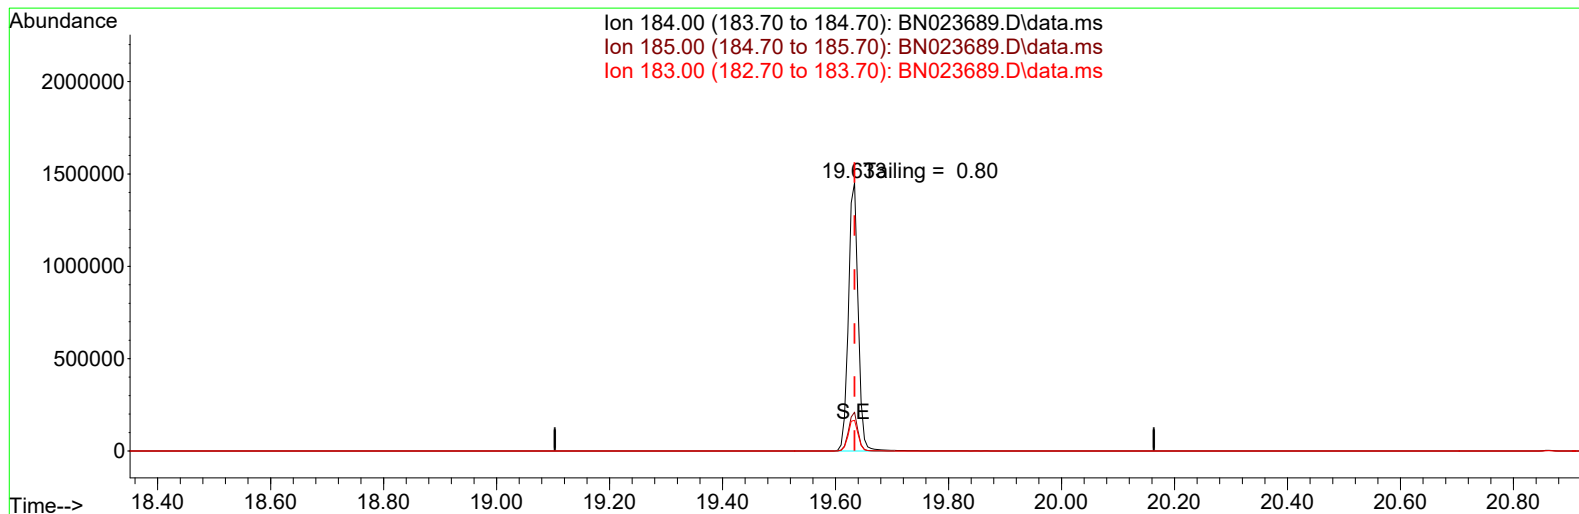

TIC: BN023689.D\data.ms

(77) Benzidine

19.633min (0.000) 0.00 ng

response 1746594

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	11.49
0.00	0.00	0.00