


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
Data File : BN023673.D
Acq On : 17 Jan 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 18 05:42:43 2023

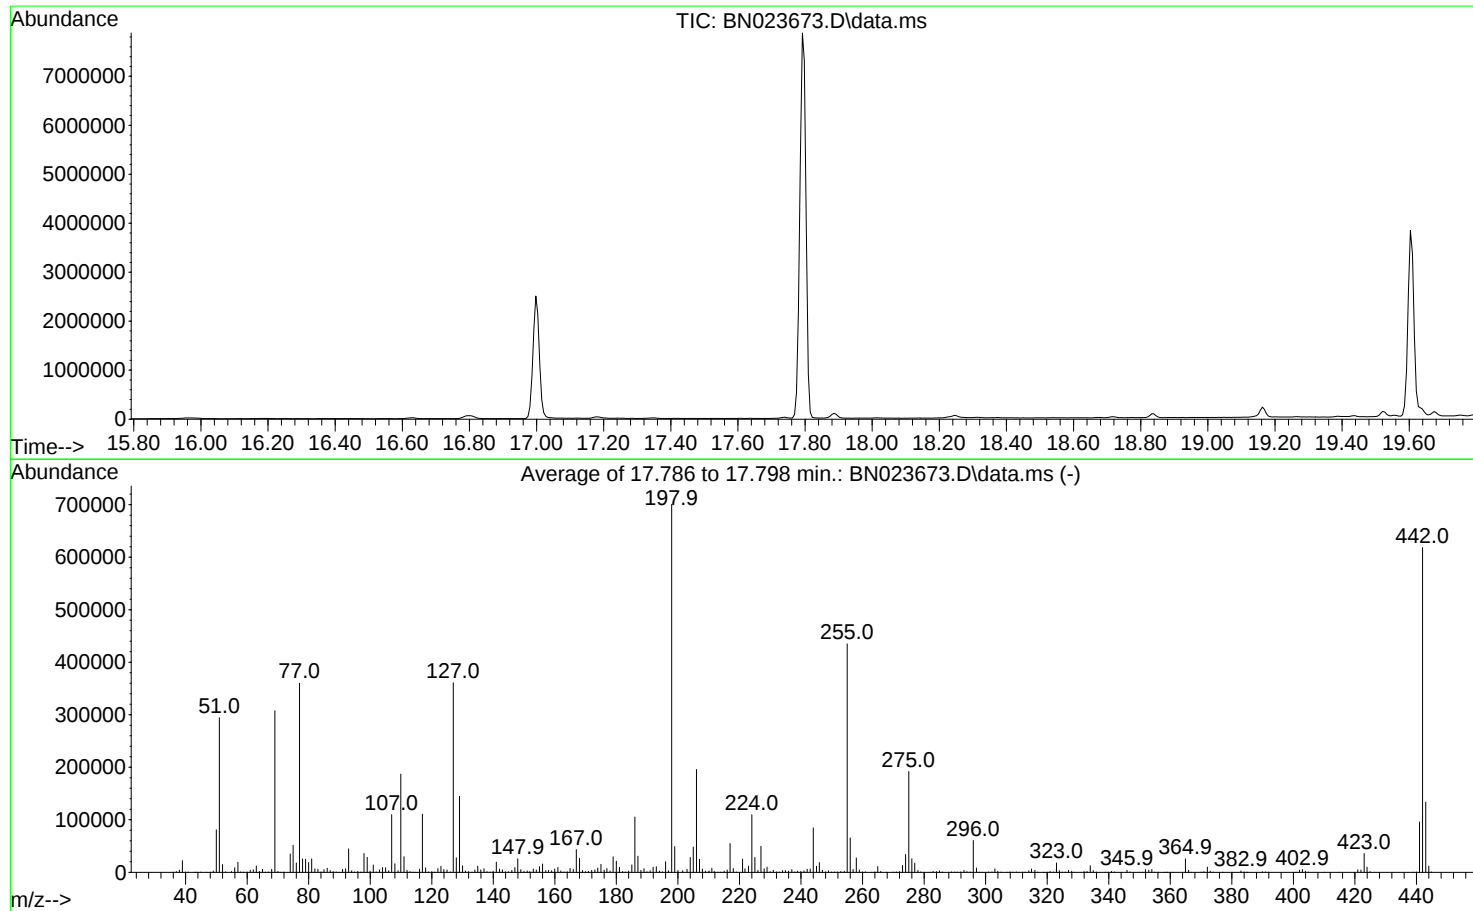




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	294315	PASS
68	69	0.00	2	1.8	5526	PASS
69	198	0.00	100	43.9	307499	PASS
70	69	0.00	2	0.6	1717	PASS
127	198	10	80	51.5	360768	PASS
197	198	0.00	2	0.4	2903	PASS
198	198	100	100	100.0	700523	PASS
199	198	5	9	7.0	48912	PASS
275	198	10	60	27.4	191957	PASS
365	198	1	100	3.7	25696	PASS
441	198	0.01	100	13.7	95757	PASS
442	442	50	100	100.0	618411	PASS
443	442	15	24	21.6	133659	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
Data File : BN023673.D
Acq On : 17 Jan 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 18 07:10:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 07:10:10 2023
Response via : Initial Calibration

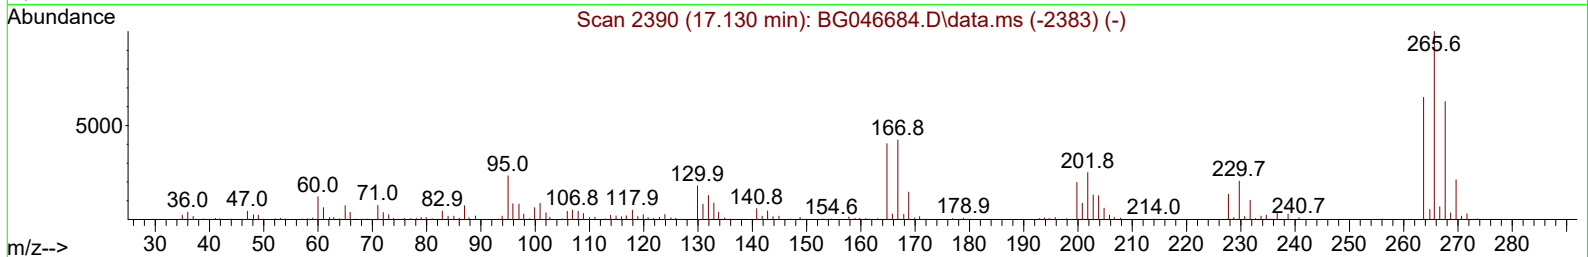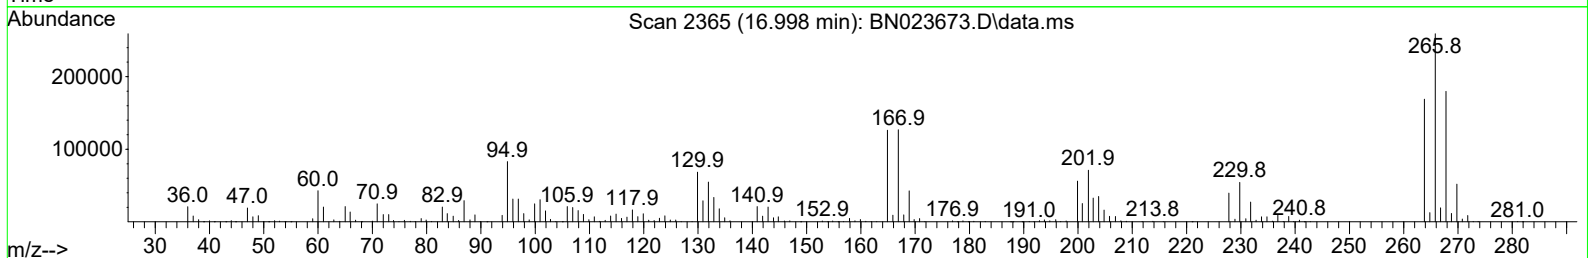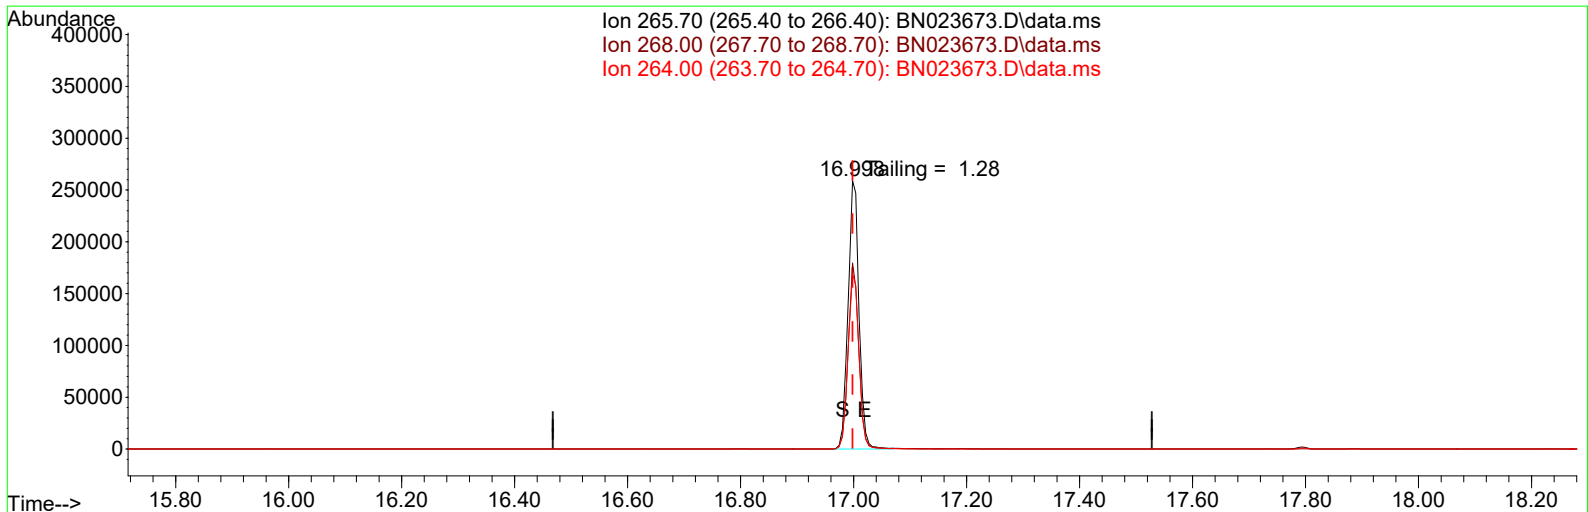

TIC: BN023673.D\data.ms

(70) Pentachlorophenol (C)

16.998min (0.000) 8414.73 ng




response 350721

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.37
264.00	61.60	65.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
Data File : BN023673.D
Acq On : 17 Jan 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 18 07:10:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 07:10:10 2023
Response via : Initial Calibration

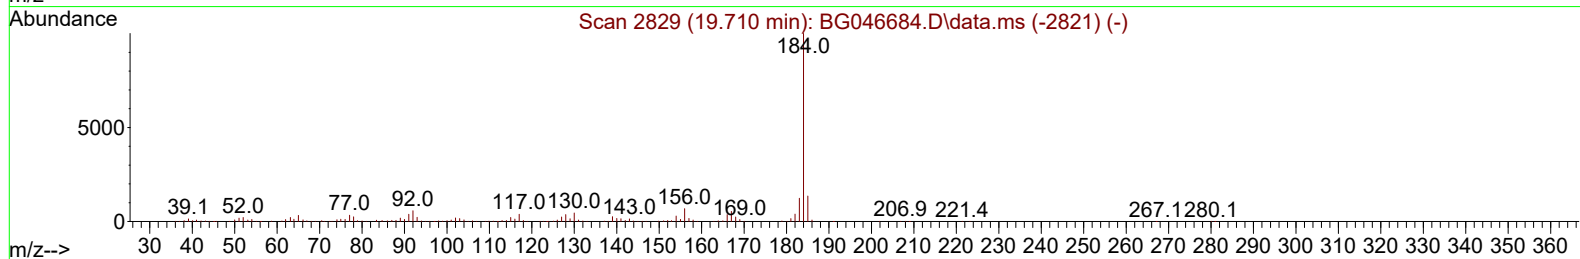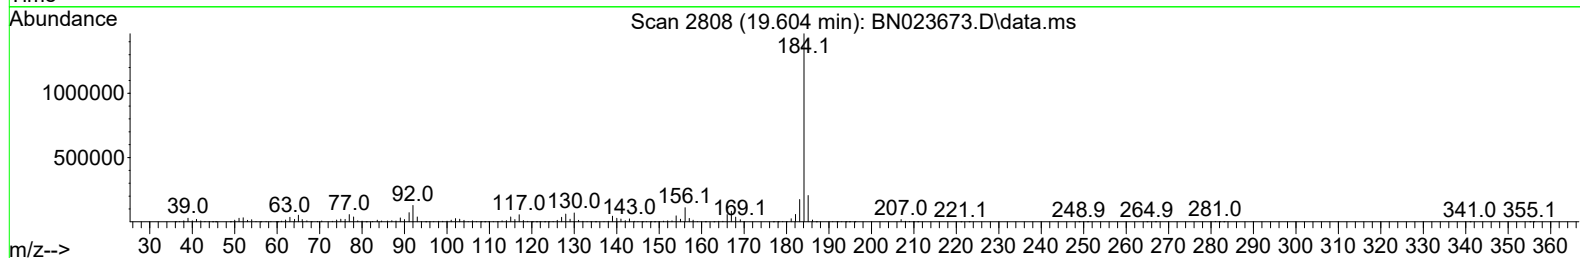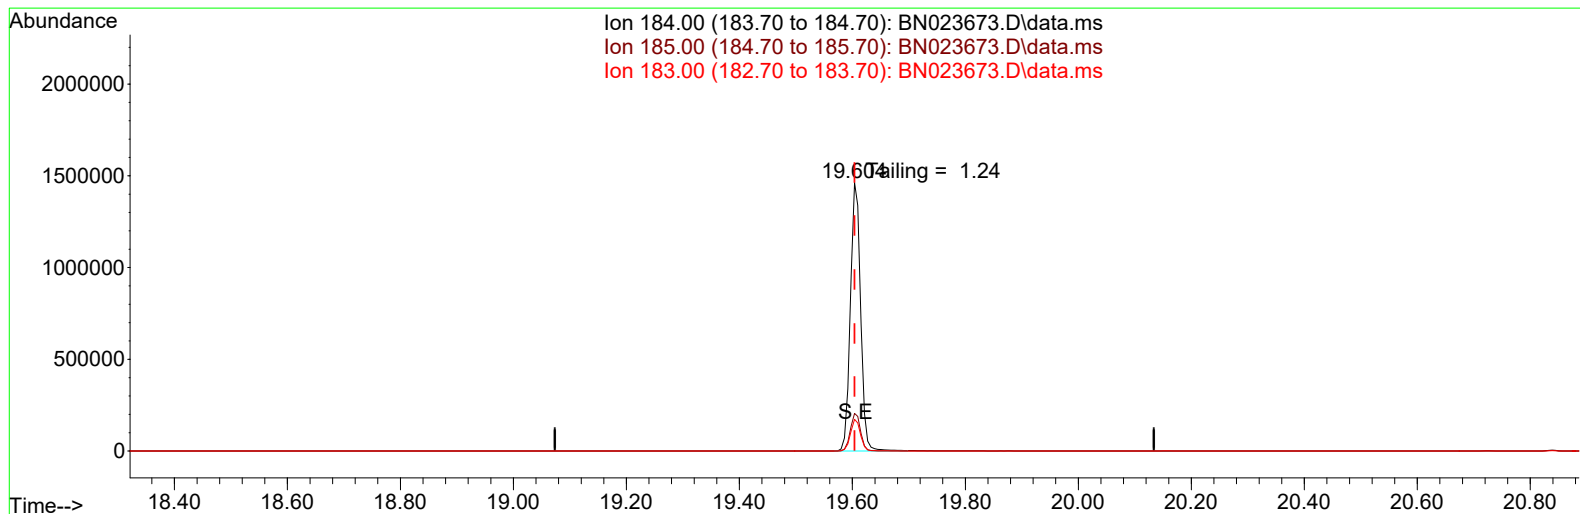

TIC: BN023673.D\data.ms

(77) Benzidine

19.604min (0.000) 0.00 ng

response 1851414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2023	BNA_N	<u>BN023673.D</u>
Compound Name	Response	Retention Time
DDT	1044547	20.839
DDD	36640	20.398
DDE	1744	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38384	1082931	3.54

Instrument :
BNA_N
ClientSampleId :
DFTPP