
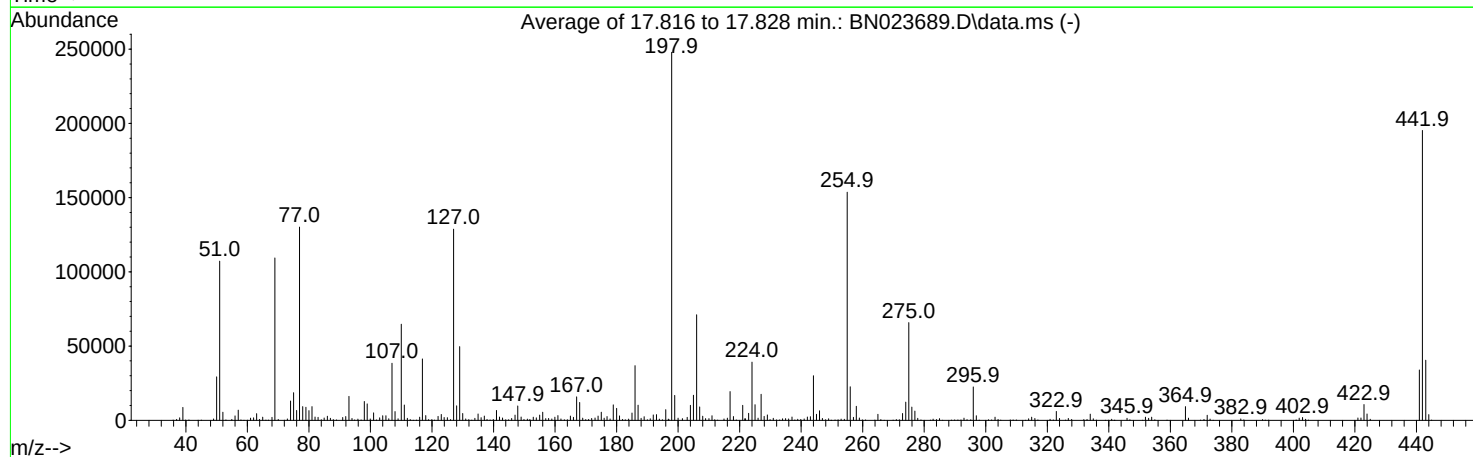


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
 Data File : BN023689.D
 Acq On : 17 Jan 2023 19:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 18 05:42:43 2023

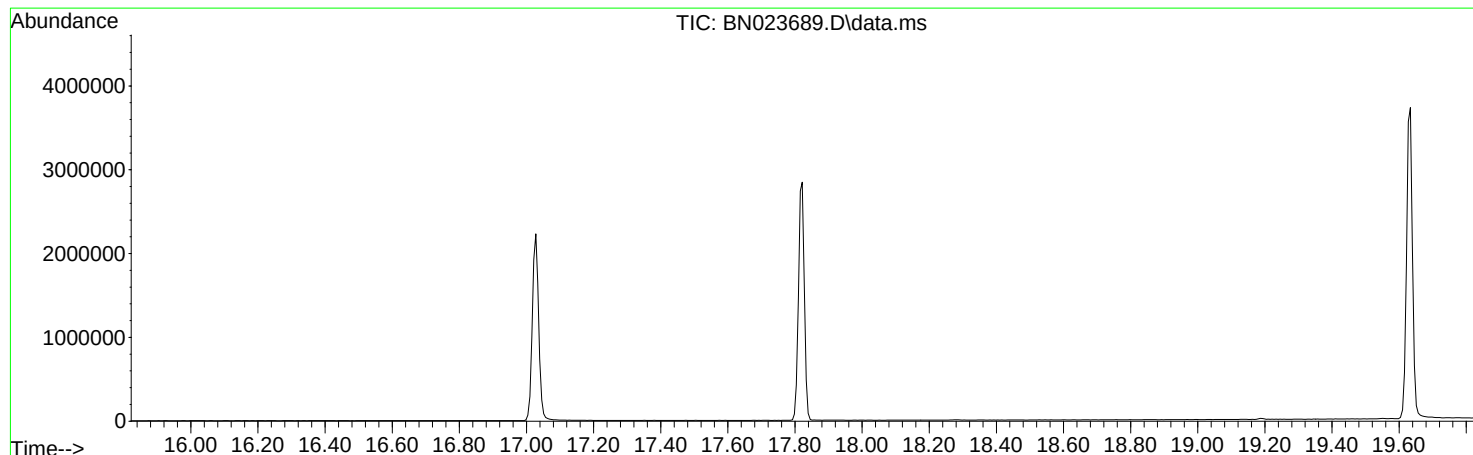




AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	107189	PASS
68	69	0.00	2	1.8	2001	PASS
69	198	0.00	100	44.1	109405	PASS
70	69	0.00	2	0.6	620	PASS
127	198	10	80	52.0	128787	PASS
197	198	0.00	2	0.3	762	PASS
198	198	100	100	100.0	247808	PASS
199	198	5	9	6.8	16815	PASS
275	198	10	60	26.5	65771	PASS
365	198	1	100	3.7	9262	PASS
441	198	0.01	100	13.7	33848	PASS
442	442	50	100	100.0	195264	PASS
443	442	15	24	20.7	40483	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
 Data File : BN023689.D
 Acq On : 17 Jan 2023 19:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 18 07:11:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 18 07:11:53 2023
 Response via : Initial Calibration

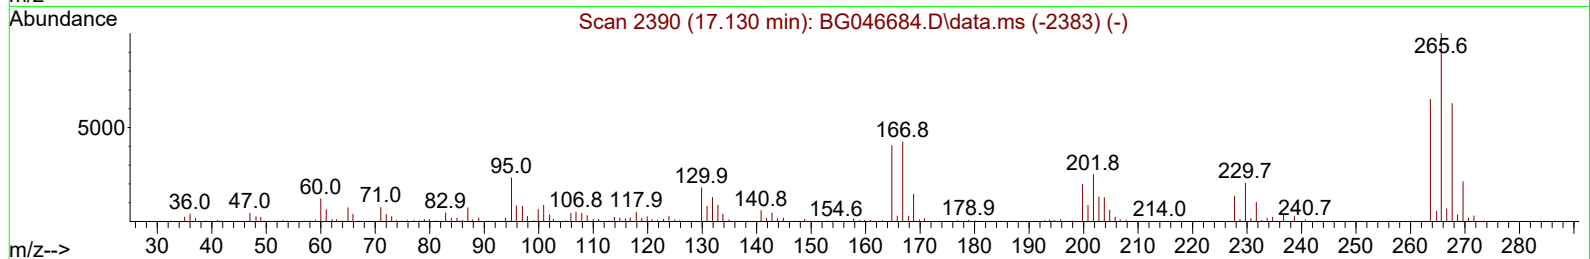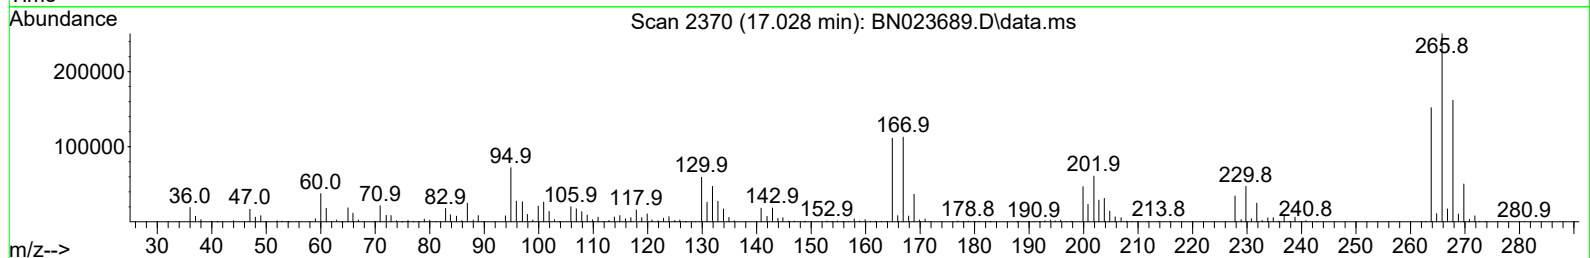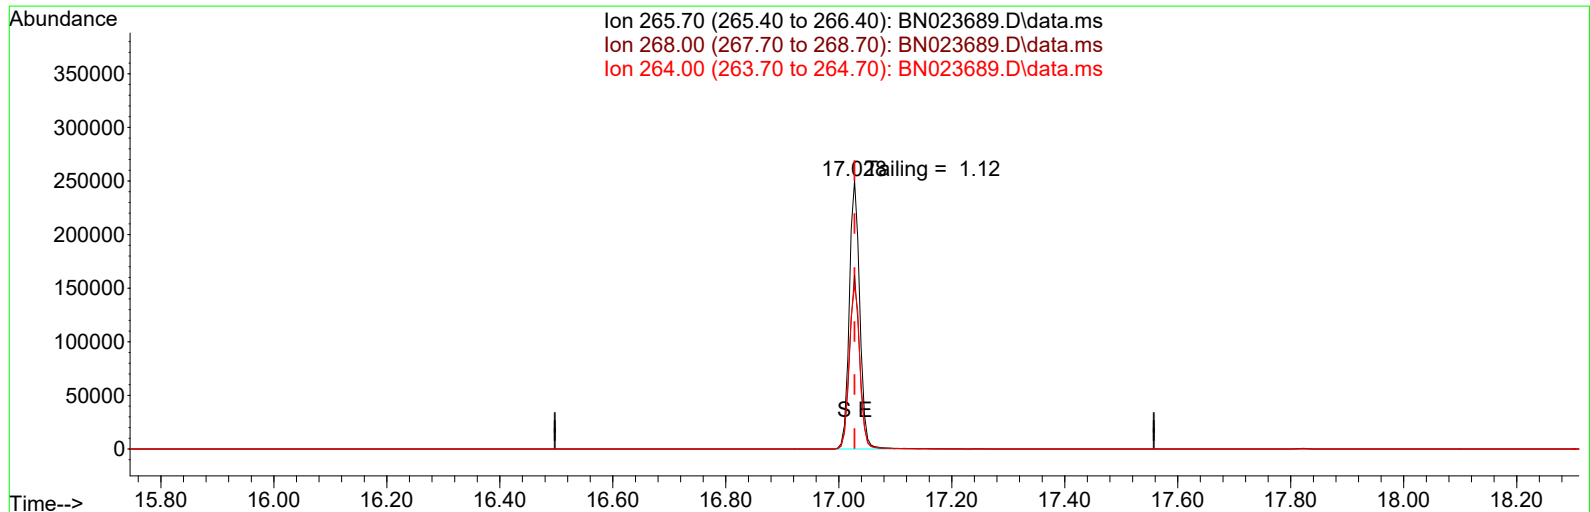

TIC: BN023689.D\data.ms

(70) Pentachlorophenol (C)

17.028min (0.000) 20868.15 ng




response 323278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.62
264.00	61.60	60.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011723\
Data File : BN023689.D
Acq On : 17 Jan 2023 19:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 18 07:11:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 07:11:53 2023
Response via : Initial Calibration

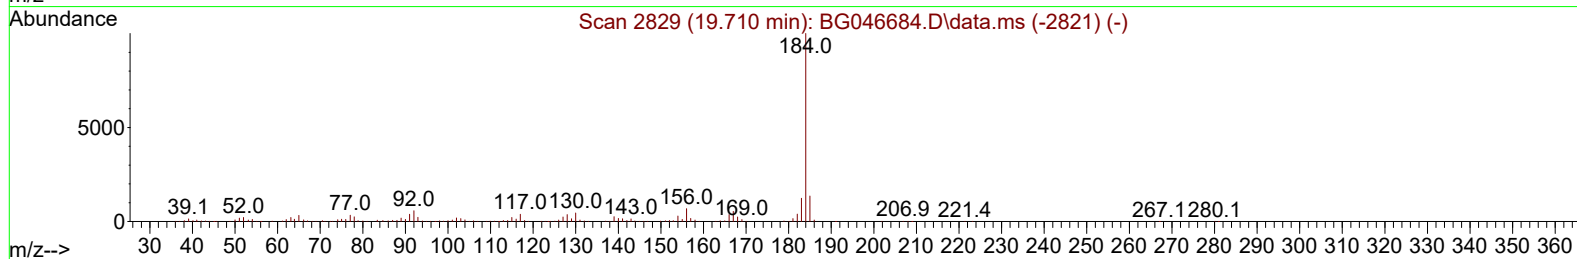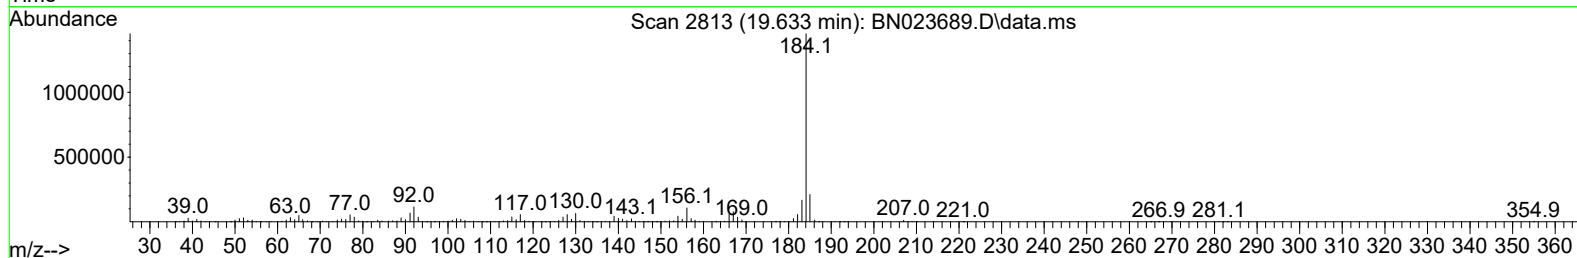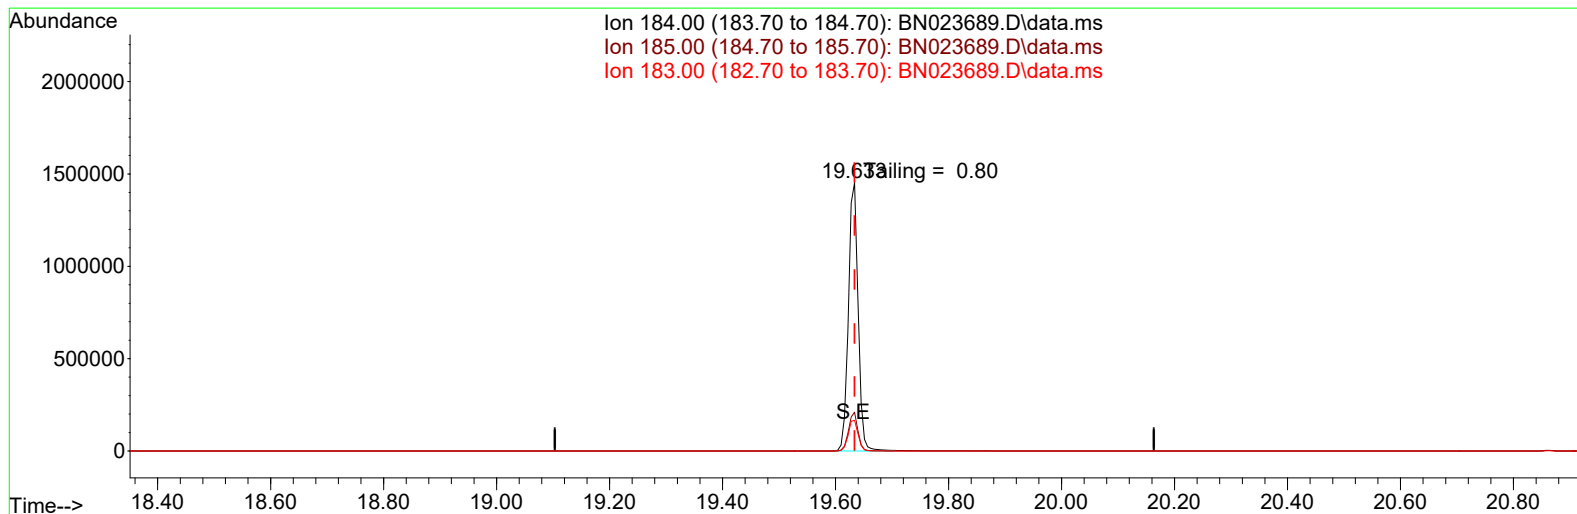

TIC: BN023689.D\data.ms

(77) Benzidine

19.633min (0.000) 0.00 ng

response 1746594

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	11.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2023	BNA_N	<u>BN023689.D</u>
Compound Name	Response	Retention Time
DDT	864676	20.863
DDD	22226	20.422
DDE	1195	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23421	888097	2.64

Instrument :
BNA_N
ClientSampleId :
DFTPP