

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
 Data File : BN029280.D
 Acq On : 17 Jan 2024 20:01
 Operator : MA/JU
 Sample : PB158468BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK368

Quant Time: Jan 18 00:28:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 16 03:57:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	101776	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	458714	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	315061	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.327	188	709478	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	668311	20.000	ng/ul	0.00
88) Perylene-d12	23.945	264	785142	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	16781	6.809	ng/uL	0.00
4) Pyridine-d5	3.781	84	246000	32.364	ng/ul	0.00
7) Phenol-d5	7.099	99	289306	29.627	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	200920	32.622	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	225048	32.580	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	239934	30.475	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	118597	35.638	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	99034	35.884	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	215448	31.362	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	380420	30.597	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	886461	34.181	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	937972	32.115	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	120233	26.638	ng/ul	0.00
60) Fluorene-d10	15.575	176	733940	33.206	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	73335	24.579	ng/ul	0.00
73) Anthracene-d10	17.427	188	1185898	33.250	ng/ul	0.00
81) Pyrene-d10	19.727	212	1422572	38.307	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.792	264	1418197	35.047	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.646	70	7057	1.005 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029280.D
Acq On : 17 Jan 2024 20:01
Operator : MA/JU
Sample : PB158468BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK368


Quant Time: Jan 18 00:28:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 16 03:57:40 2024
Response via : Initial Calibration

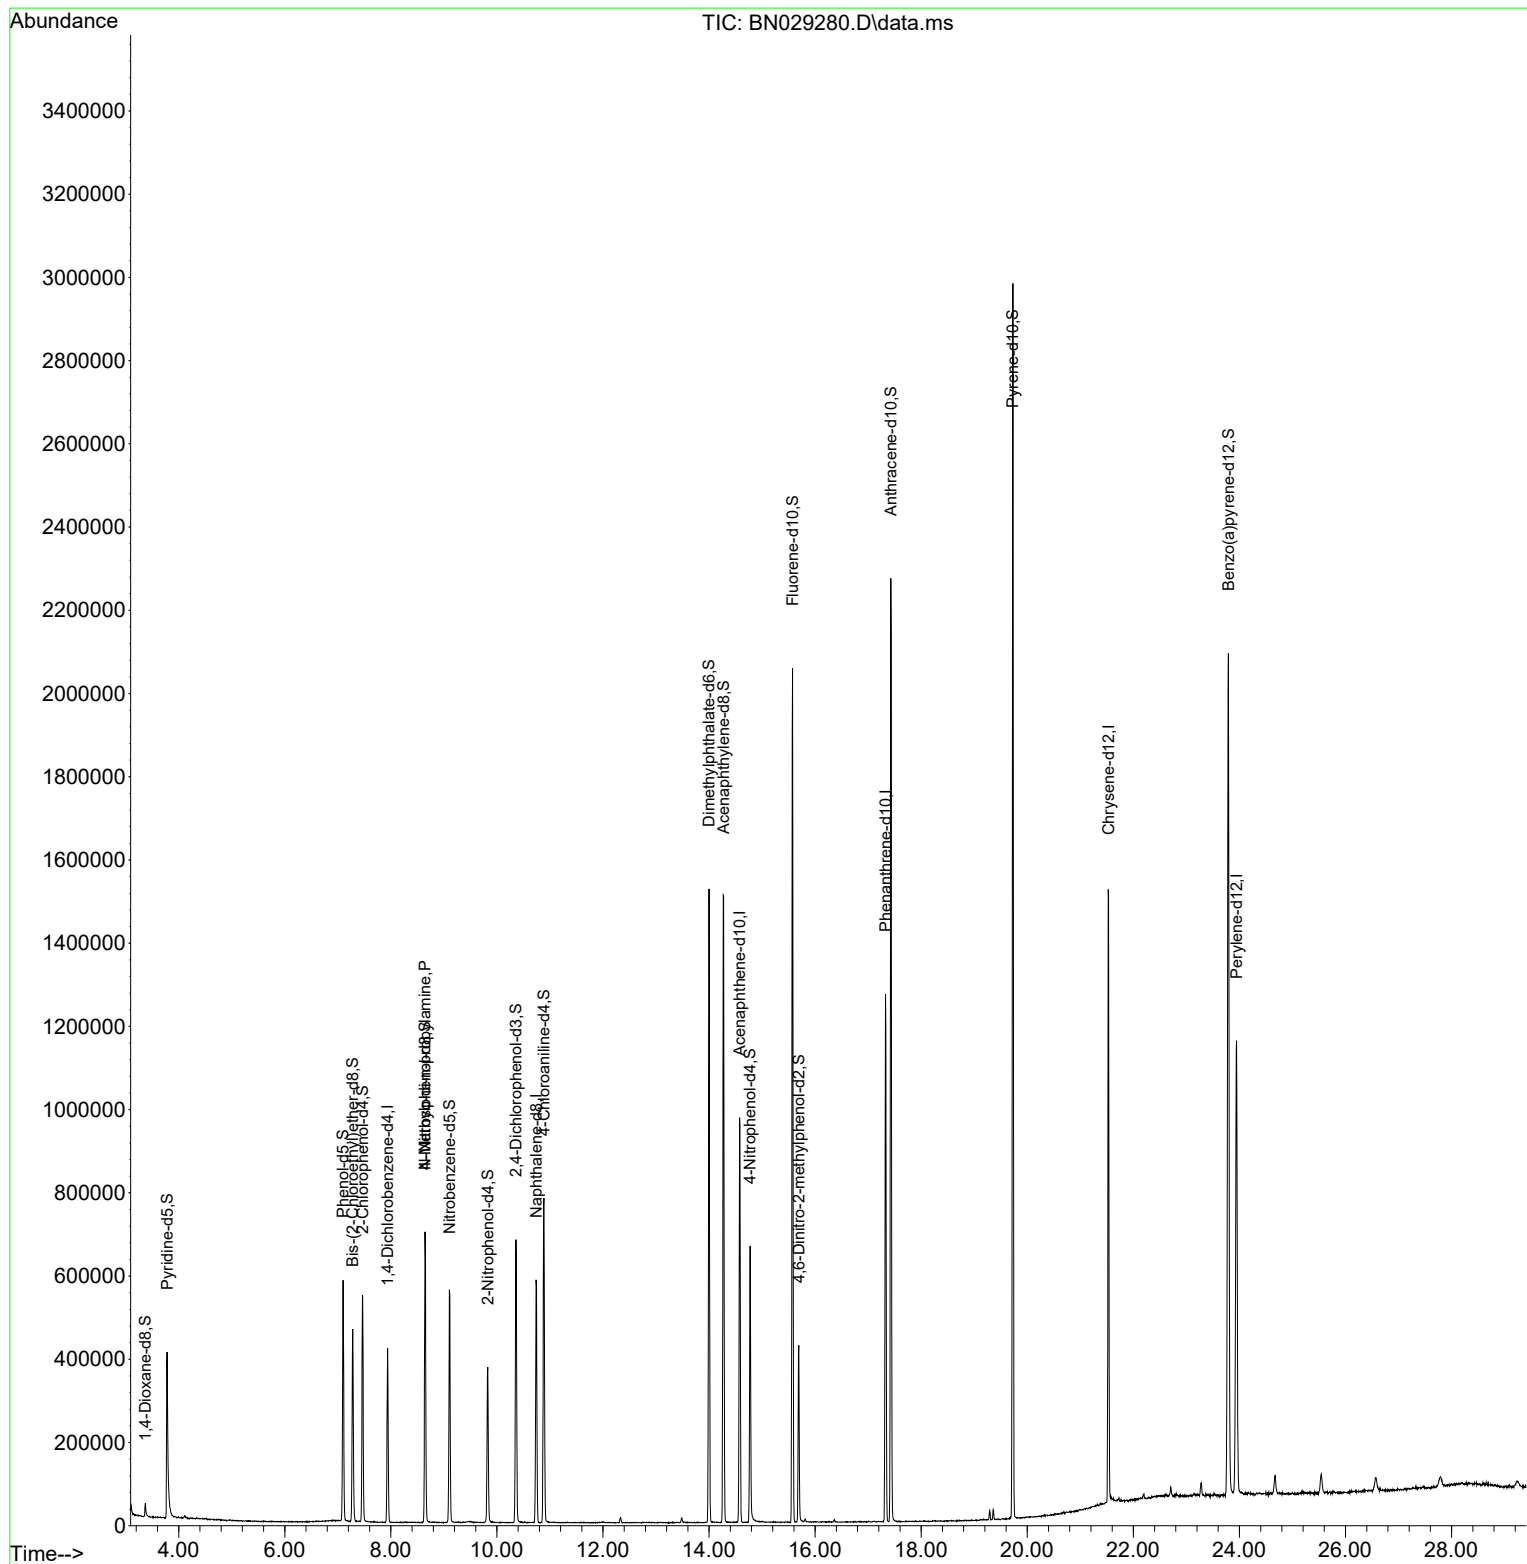

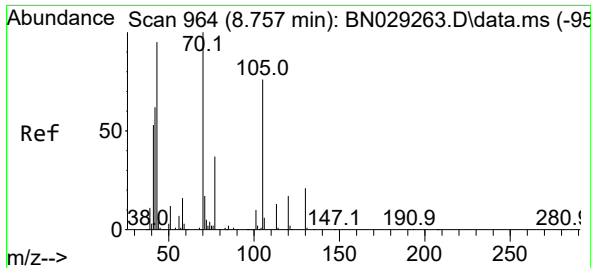

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.005 ng/ul
 RT: 8.646 min Scan# 945
 Delta R.T. -0.112 min
 Lab File: BN029280.D
 Acq: 17 Jan 2024 20:01

Instrument :
 BNA_N
 ClientSampleId :
 SBLK368

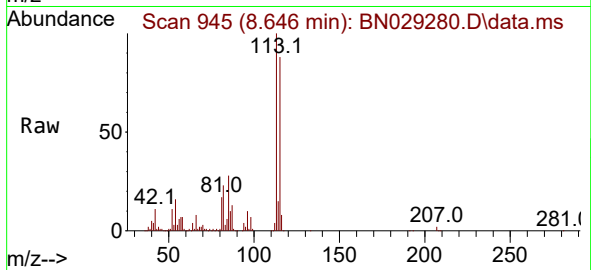

Tgt Ion:	70	Resp:	7057
Ion	Ratio	Lower	Upper
70	100		
42	399.8	48.3	72.5#
101	0.0	7.1	10.7#
130	0.0	15.4	23.2#

