

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
 Data File : BN029282.D
 Acq On : 17 Jan 2024 21:13
 Operator : MA/JU
 Sample : PB158470BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK370

Quant Time: Jan 18 00:29:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 16 03:57:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	114384	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	521116	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	346800	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	806101	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	745646	20.000	ng/ul	0.00
88) Perylene-d12	23.945	264	858525	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	17747	6.408	ng/uL	0.00
4) Pyridine-d5	3.781	84	262886	30.773	ng/ul	0.00
7) Phenol-d5	7.099	99	298315	27.182	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	208840	30.170	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	234644	30.225	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	245038	27.692	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	123634	32.703	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	103160	32.903	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	219971	28.186	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131	394354	27.920	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	908242	31.816	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	989494	30.778	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	124078	24.974	ng/ul	0.00
60) Fluorene-d10	15.575	176	773276	31.784	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	75844	22.373	ng/ul	0.00
73) Anthracene-d10	17.428	188	1235542	30.490	ng/ul	0.00
81) Pyrene-d10	19.727	212	1412940	34.101	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.792	264	1437204	32.480	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	14.004	165	5847	1.244	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029282.D
Acq On : 17 Jan 2024 21:13
Operator : MA/JU
Sample : PB158470BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370


Quant Time: Jan 18 00:29:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 16 03:57:40 2024
Response via : Initial Calibration

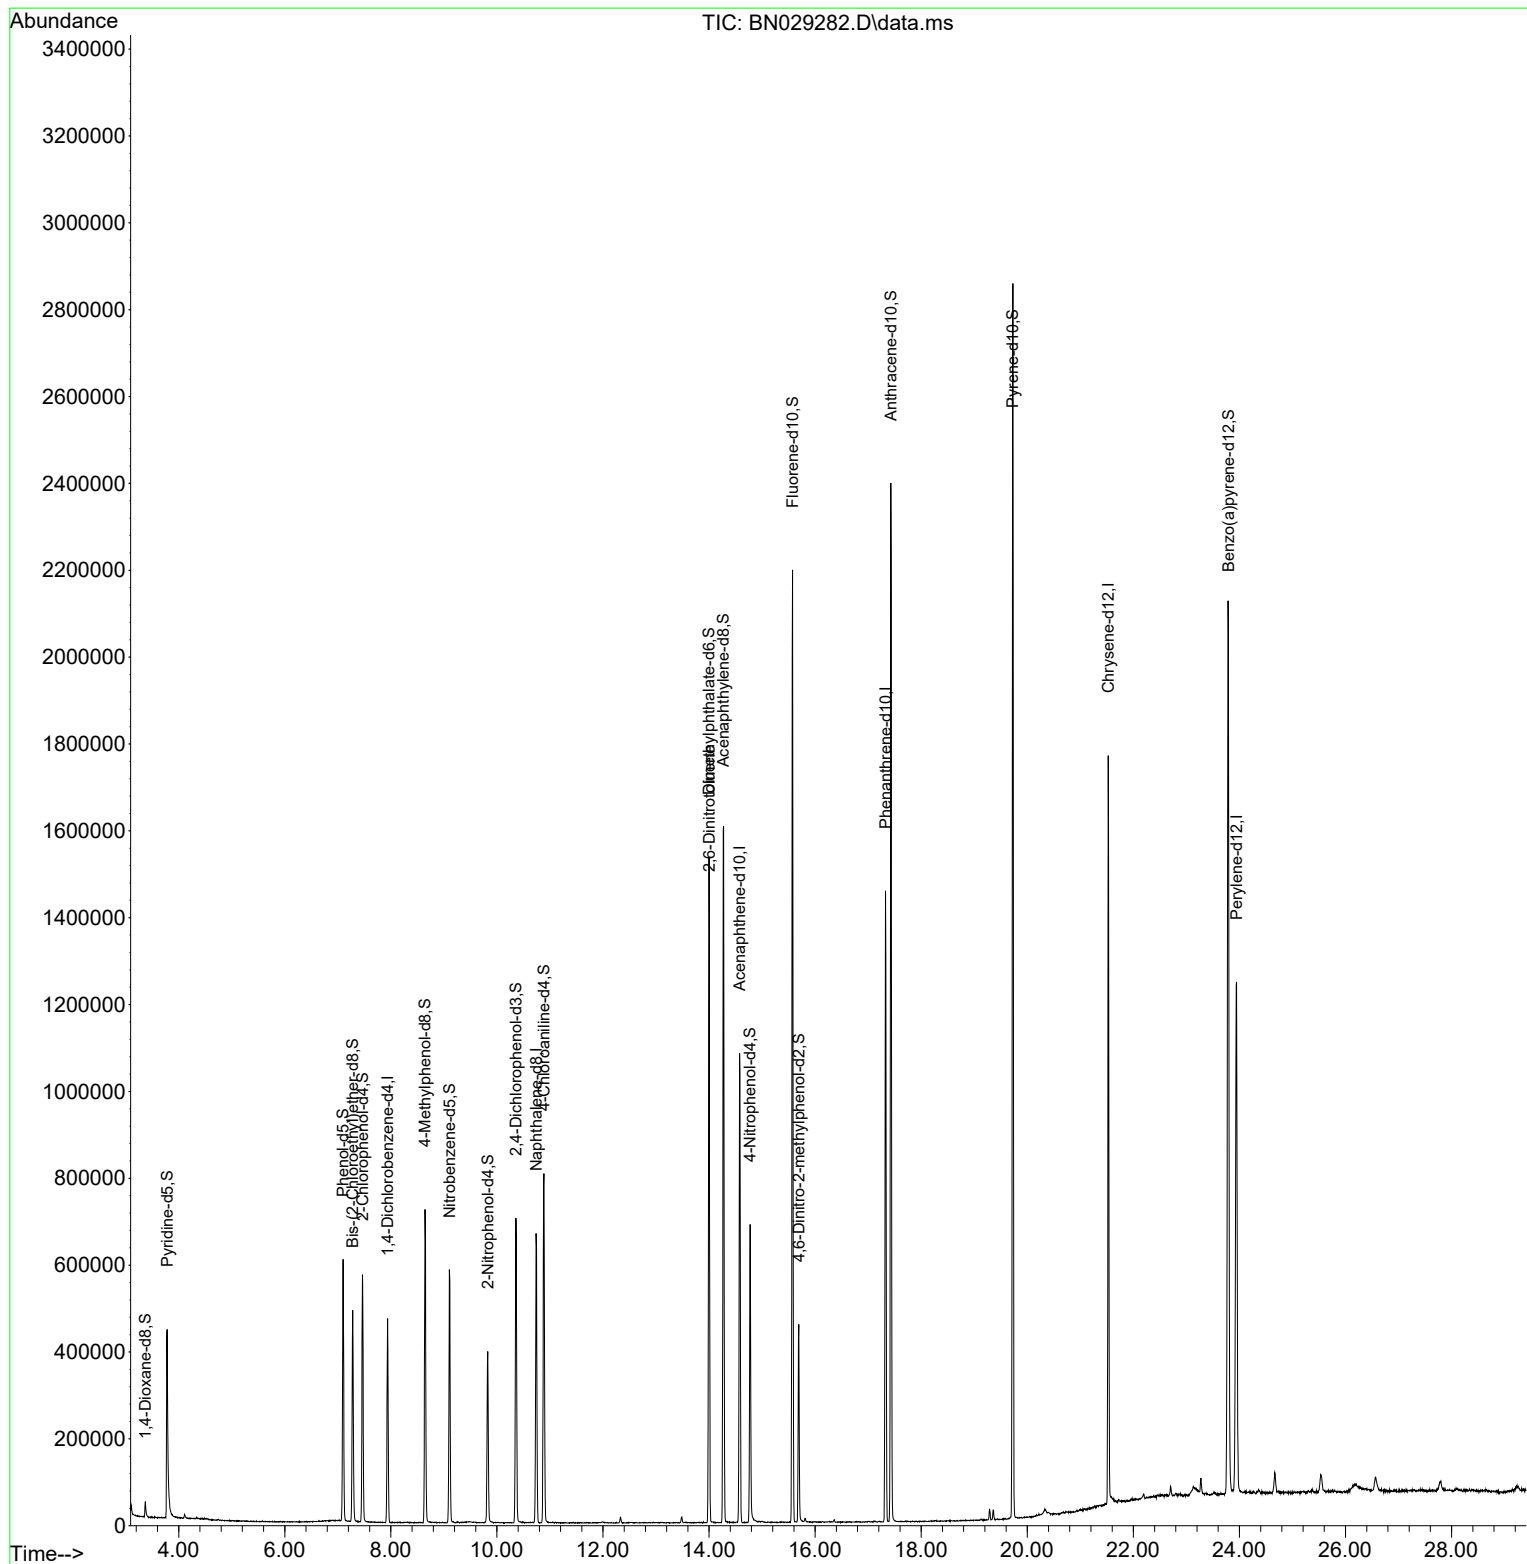

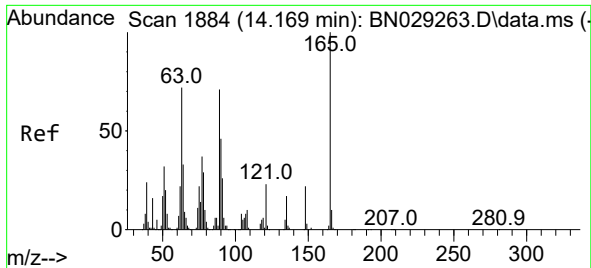

#48
 2,6-Dinitrotoluene
 Concen: 1.244 ng/ul
 RT: 14.004 min Scan# 1856
 Delta R.T. -0.164 min
 Lab File: BN029282.D
 Acq: 17 Jan 2024 21:13

Instrument :
 BNA_N
 ClientSampleId :
 SBLK370

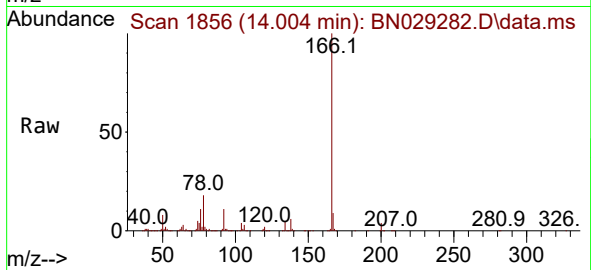

Tgt Ion:	165	Resp:	5847
Ion	Ratio	Lower	Upper
165	100		
89	0.0	58.6	87.8#
121	22.3	20.6	30.8

