

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
 Data File : BN029264.D
 Acq On : 17 Jan 2024 10:23
 Operator : MA/JU
 Sample : PB158323BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK323

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	59	rVB	39187	61826	1.15%	0.120%
2	3.781	115	118	138	rBV	533886	948133	17.57%	1.846%
3	4.117	172	175	177	rBV2	6141	5742	0.11%	0.011%
4	7.105	675	683	693	rVB	719319	1182376	21.91%	2.302%
5	7.281	703	713	722	rBV	601295	962426	17.83%	1.874%
6	7.469	737	745	754	rBV	734475	1167786	21.64%	2.274%
7	7.940	819	825	833	rVB	588783	953559	17.67%	1.857%
8	8.646	938	945	955	rBV	878608	1460753	27.06%	2.844%
9	9.110	1014	1024	1037	rBV	735098	1208405	22.39%	2.353%
10	9.828	1133	1146	1156	rBV	500551	819758	15.19%	1.596%
11	10.363	1229	1237	1251	rBV	870309	1468382	27.21%	2.859%
12	10.746	1293	1302	1312	rVB	849511	1452900	26.92%	2.829%
13	10.887	1317	1326	1337	rBV	1046586	1732688	32.10%	3.374%
14	12.334	1566	1572	1578	rVB	18018	26731	0.50%	0.052%
15	13.487	1763	1768	1775	rBV4	10712	18726	0.35%	0.036%
16	14.004	1849	1856	1865	rBV	1931092	2727862	50.54%	5.311%
17	14.275	1895	1902	1909	rBV	2082344	3048777	56.49%	5.936%
18	14.581	1946	1954	1962	rBV	1434986	2116627	39.22%	4.121%
19	14.775	1981	1987	2002	rBV	828197	1225947	22.71%	2.387%
20	15.004	2023	2026	2031	rVB7	3572	5504	0.10%	0.011%
21	15.575	2116	2123	2132	rBV	2815609	3882349	71.93%	7.559%
22	15.692	2135	2143	2155	rBV	594093	799674	14.82%	1.557%
23	15.810	2160	2163	2169	rVB2	11114	17001	0.31%	0.033%
24	16.363	2252	2257	2261	rBV5	8501	11696	0.22%	0.023%
25	17.333	2415	2422	2429	rBV	1811194	2657694	49.24%	5.175%
26	17.433	2432	2439	2454	rVB	3078267	4332694	80.27%	8.436%
27	19.292	2750	2755	2762	rBV3	33291	44724	0.83%	0.087%
28	19.363	2762	2767	2771	rBV2	30864	41457	0.77%	0.081%
29	19.727	2823	2829	2839	rVB	3716874	4991401	92.48%	9.718%
30	21.533	3130	3136	3144	rBV	2349721	2974823	55.12%	5.792%
31	22.710	3333	3336	3340	rBV3	29362	38733	0.72%	0.075%
32	23.280	3429	3433	3443	rVB3	47232	86156	1.60%	0.168%
33	23.792	3511	3520	3536	rBV	2669423	5397353	100.00%	10.509%
34	23.945	3538	3546	3564	rVB2	1588170	3361950	62.29%	6.546%
35	24.680	3666	3671	3680	rVB3	60028	128096	2.37%	0.249%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029264.D
Acq On : 17 Jan 2024 10:23
Operator : MA/JU
Sample : PB158323BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK323

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 51360709

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029264.D
Acq On : 17 Jan 2024 10:23
Operator : MA/JU
Sample : PB158323BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

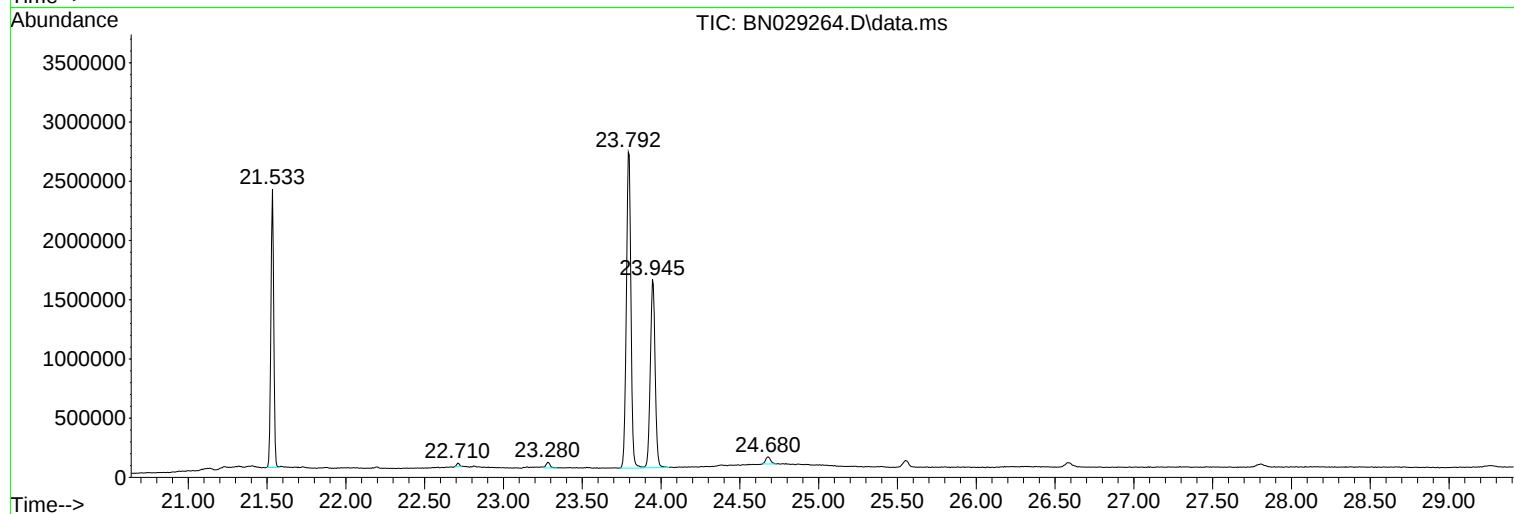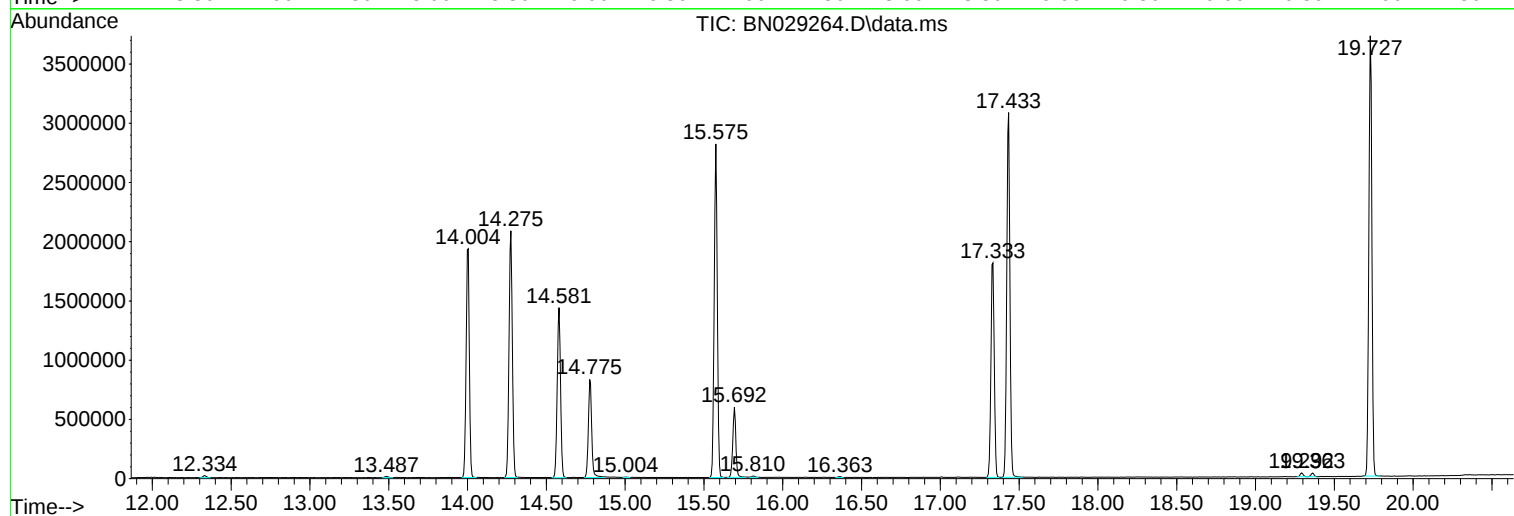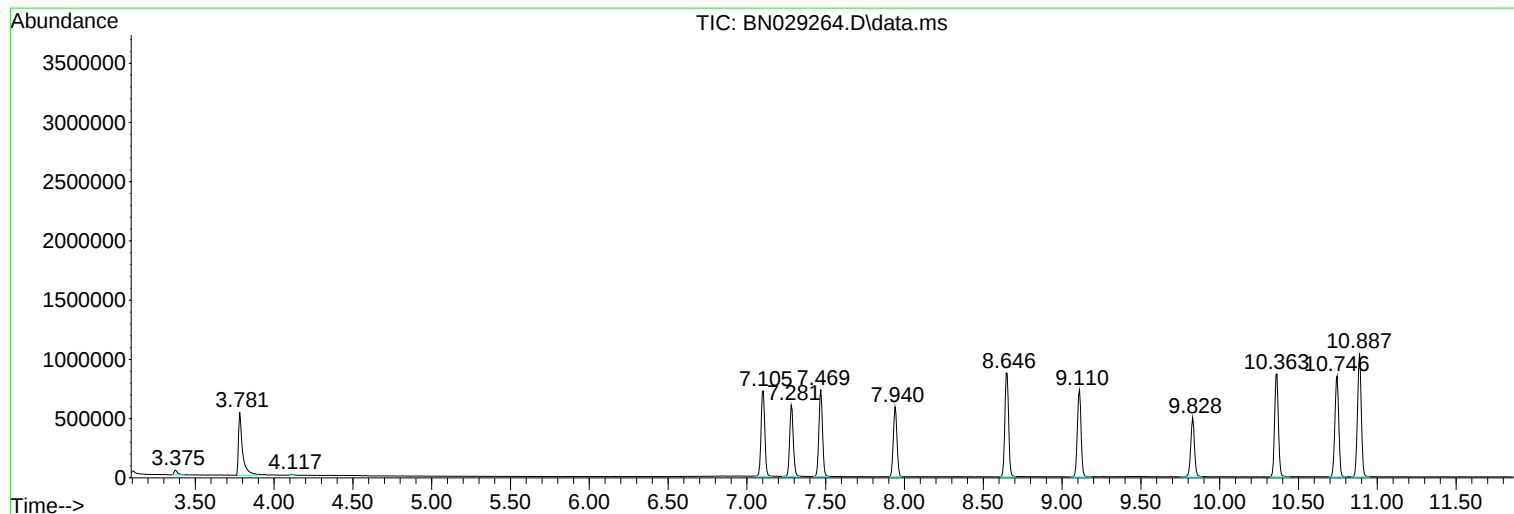

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029264.D
Acq On : 17 Jan 2024 10:23
Operator : MA/JU
Sample : PB158323BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029264.D
Acq On : 17 Jan 2024 10:23
Operator : MA/JU
Sample : PB158323BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK323

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------