

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
 Data File : BN029277.D
 Acq On : 17 Jan 2024 18:13
 Operator : MA/JU
 Sample : PB158436BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK436

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	55	rBV	28613	40707	1.08%	0.113%
2	3.781	114	118	132	rBV	365735	642066	17.02%	1.785%
3	4.116	170	175	180	rBV2	7129	10244	0.27%	0.028%
4	7.099	676	682	692	rVB	530096	832221	22.06%	2.314%
5	7.281	707	713	721	rVV	422000	660718	17.52%	1.837%
6	7.469	737	745	752	rBV	498573	819149	21.72%	2.278%
7	7.940	819	825	832	rBV	430465	671776	17.81%	1.868%
8	8.646	938	945	956	rBV	647000	1031820	27.36%	2.869%
9	9.104	1015	1023	1034	rBV	504234	854077	22.64%	2.375%
10	9.510	1091	1092	1104	rVB8	3000	5001	0.13%	0.014%
11	9.828	1139	1146	1156	rBV	337471	567594	15.05%	1.578%
12	10.357	1229	1236	1247	rBV	624426	1029330	27.29%	2.862%
13	10.740	1293	1301	1310	rVB	605431	1023278	27.13%	2.845%
14	10.887	1318	1326	1339	rBV	709186	1221067	32.37%	3.395%
15	12.334	1567	1572	1576	rVB2	11216	18273	0.48%	0.051%
16	13.487	1763	1768	1772	rBV5	7634	11510	0.31%	0.032%
17	13.998	1847	1855	1862	rBV	1344746	1831579	48.56%	5.093%
18	14.275	1894	1902	1909	rBV	1400952	2093227	55.50%	5.820%
19	14.575	1946	1953	1962	rVB	942943	1454831	38.57%	4.045%
20	14.775	1979	1987	1998	rBV	591228	845489	22.42%	2.351%
21	15.575	2116	2123	2130	rBV	1848920	2648389	70.21%	7.364%
22	15.692	2136	2143	2154	rBV	368416	525515	13.93%	1.461%
23	15.810	2159	2163	2168	rVB5	8461	11276	0.30%	0.031%
24	16.363	2253	2257	2260	rVB4	5098	6607	0.18%	0.018%
25	17.110	2380	2384	2389	rBV5	4038	5830	0.15%	0.016%
26	17.328	2415	2421	2430	rVB	1279866	1857234	49.24%	5.164%
27	17.428	2430	2438	2448	rBV2	2069666	2961933	78.53%	8.236%
28	19.127	2724	2727	2729	rBV3	2596	3867	0.10%	0.011%
29	19.180	2734	2736	2743	rVB4	2870	5205	0.14%	0.014%
30	19.292	2750	2755	2761	rBV2	24773	34727	0.92%	0.097%
31	19.357	2762	2766	2772	rVV	22120	29172	0.77%	0.081%
32	19.686	2818	2822	2823	rBV4	3610	4104	0.11%	0.011%
33	19.727	2823	2829	2838	rVV	2677954	3515977	93.21%	9.777%
34	20.316	2926	2929	2930	rBV3	3960	4673	0.12%	0.013%
35	21.527	3129	3135	3141	rBV	1694353	2143956	56.84%	5.962%
36	22.704	3332	3335	3341	rVB5	25500	36591	0.97%	0.102%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029277.D
Acq On : 17 Jan 2024 18:13
Operator : MA/JU
Sample : PB158436BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK436

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION

37	23.268	3428	3431	3438	rVB3	36219	64934	1.72%	0.181%
38	23.786	3511	3519	3532	rBV	1946819	3771918	100.00%	10.488%
39	23.939	3536	3545	3559	rVB	1166913	2444878	64.82%	6.798%
40	24.668	3663	3669	3676	rVB2	53653	109748	2.91%	0.305%
41	25.539	3812	3817	3826	rVB3	47157	112795	2.99%	0.314%




Sum of corrected areas: 35963286

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029277.D
Acq On : 17 Jan 2024 18:13
Operator : MA/JU
Sample : PB158436BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

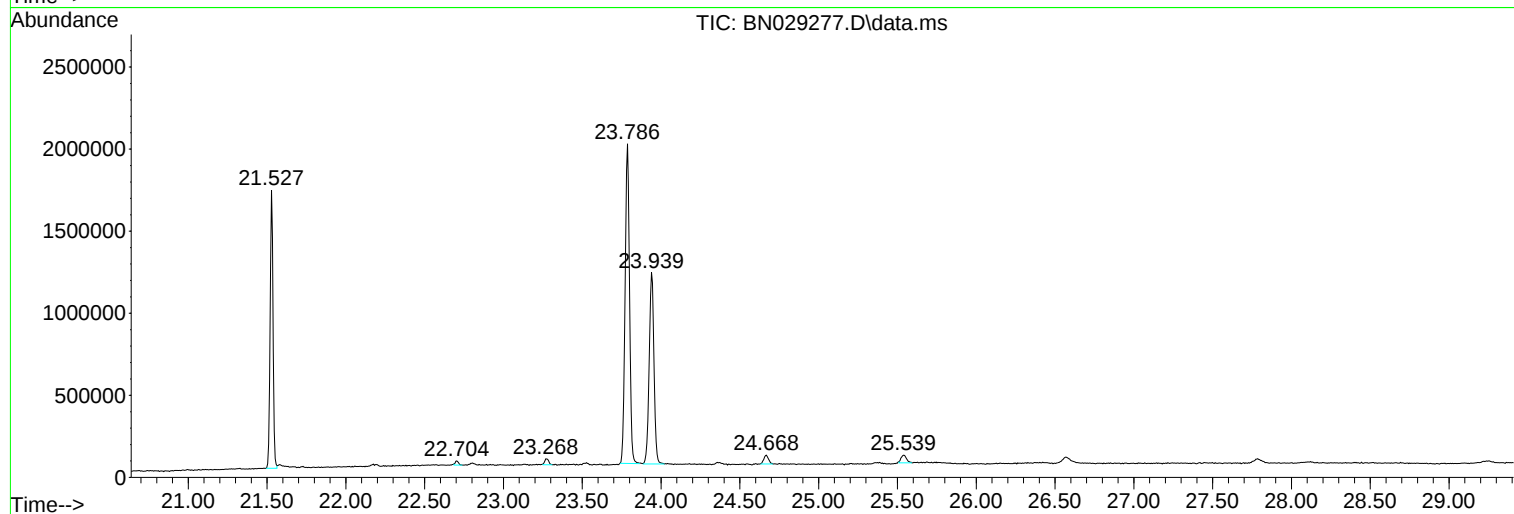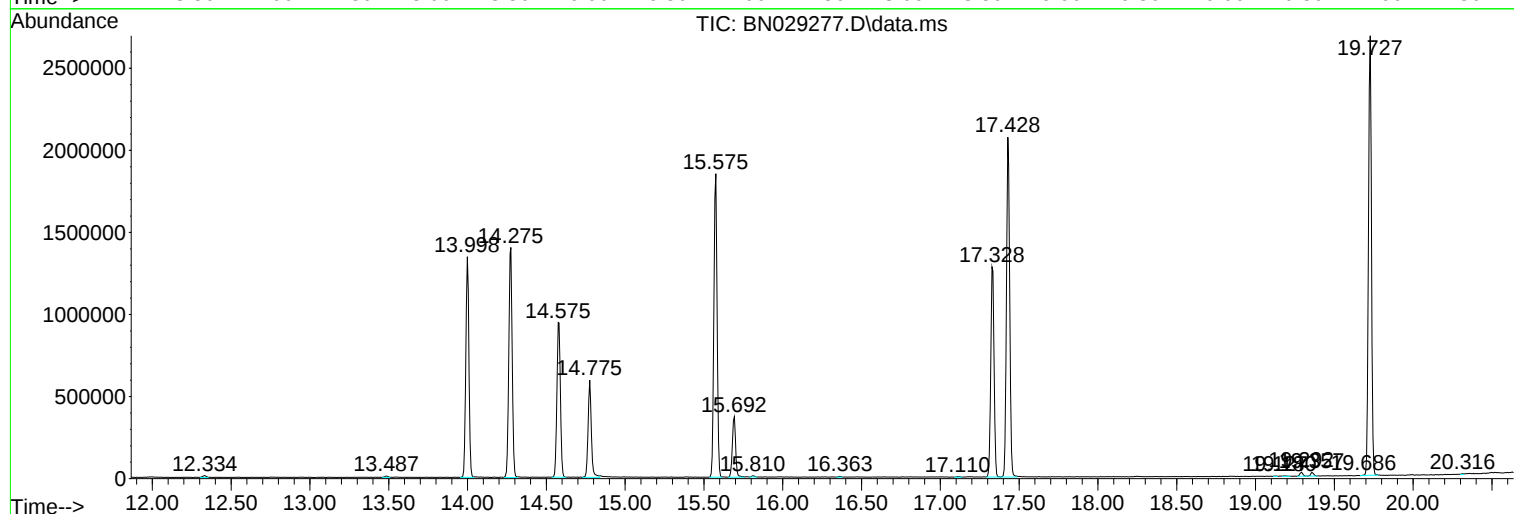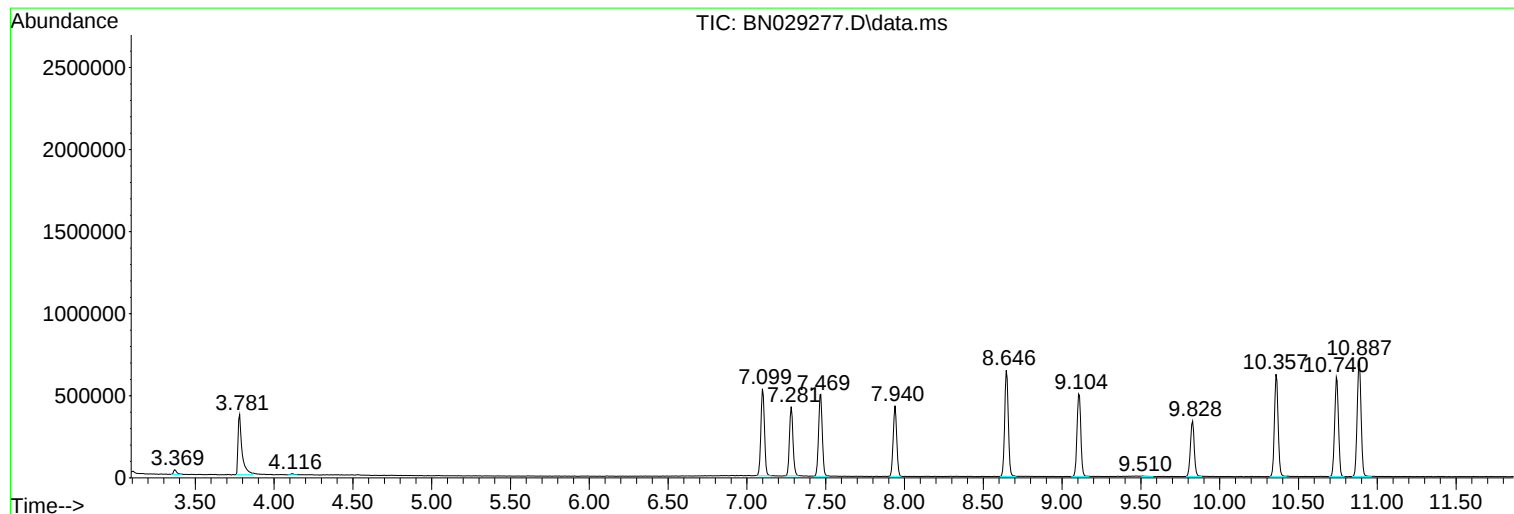

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029277.D
Acq On : 17 Jan 2024 18:13
Operator : MA/JU
Sample : PB158436BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029277.D
Acq On : 17 Jan 2024 18:13
Operator : MA/JU
Sample : PB158436BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc