

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
 Data File : BN029278.D
 Acq On : 17 Jan 2024 18:49
 Operator : MA/JU
 Sample : PB158437BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK437

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	45	48	55	rVB	32007	43498	1.13%	0.114%
2	3.781	114	118	138	rBV	407951	730884	18.98%	1.912%
3	4.117	171	175	181	rVB3	7021	11752	0.31%	0.031%
4	4.752	281	283	293	rVB8	3166	6259	0.16%	0.016%
5	7.099	675	682	691	rBV	602263	917242	23.82%	2.399%
6	7.281	707	713	723	rVB	463447	729946	18.96%	1.909%
7	7.463	738	744	754	rBV	561031	897004	23.29%	2.346%
8	7.940	817	825	834	rBV	468386	741923	19.27%	1.941%
9	8.646	938	945	957	rBV	711163	1136543	29.51%	2.973%
10	9.105	1016	1023	1031	rBV	568858	940194	24.42%	2.459%
11	9.828	1139	1146	1158	rBV	374302	621107	16.13%	1.625%
12	10.357	1228	1236	1245	rBV	690890	1131150	29.37%	2.959%
13	10.740	1294	1301	1309	rVB	666017	1118382	29.04%	2.926%
14	10.887	1318	1326	1334	rBV	788582	1327904	34.48%	3.474%
15	12.328	1566	1571	1576	rVB2	12242	17825	0.46%	0.047%
16	13.481	1761	1767	1774	rVB3	12444	21705	0.56%	0.057%
17	13.998	1848	1855	1862	rBV	1495342	2023329	52.54%	5.293%
18	14.275	1894	1902	1910	rBV	1515036	2292110	59.52%	5.996%
19	14.581	1946	1954	1965	rVB	1047917	1593374	41.38%	4.168%
20	14.775	1980	1987	2004	rBV	628253	919016	23.87%	2.404%
21	15.575	2116	2123	2131	rBV	1989909	2878760	74.76%	7.531%
22	15.692	2137	2143	2153	rBV	399787	579545	15.05%	1.516%
23	15.810	2160	2163	2169	rBV5	8143	8604	0.22%	0.023%
24	16.357	2253	2256	2260	rVB2	6431	7707	0.20%	0.020%
25	17.116	2379	2385	2389	rBV5	3024	5689	0.15%	0.015%
26	17.328	2415	2421	2428	rBV	1392968	2000115	51.94%	5.232%
27	17.428	2431	2438	2452	rBV	2275004	3185575	82.73%	8.333%
28	19.292	2750	2755	2760	rVB2	25120	32641	0.85%	0.085%
29	19.357	2762	2766	2773	rVB	22058	28856	0.75%	0.075%
30	19.686	2818	2822	2823	rBV4	3538	4907	0.13%	0.013%
31	19.728	2823	2829	2841	rVB	2922328	3733145	96.95%	9.766%
32	19.980	2869	2872	2875	rBV5	3117	4866	0.13%	0.013%
33	21.527	3129	3135	3143	rBV	1678864	2196742	57.05%	5.746%
34	23.274	3429	3432	3437	rVB5	29954	44641	1.16%	0.117%
35	23.786	3511	3519	3532	rVB2	1957210	3850782	100.00%	10.073%
36	23.939	3537	3545	3557	rVB	1184845	2443802	63.46%	6.393%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029278.D
Acq On : 17 Jan 2024 18:49
Operator : MA/JU
Sample : PB158437BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK437

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 38227524

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029278.D
Acq On : 17 Jan 2024 18:49
Operator : MA/JU
Sample : PB158437BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK437

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

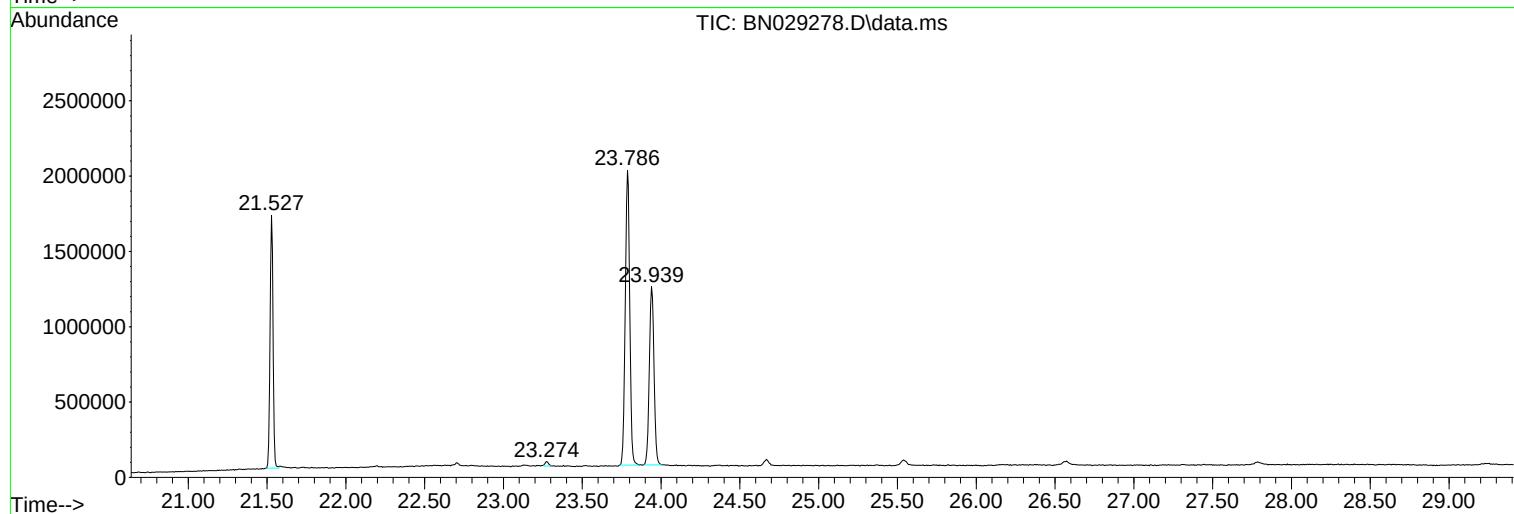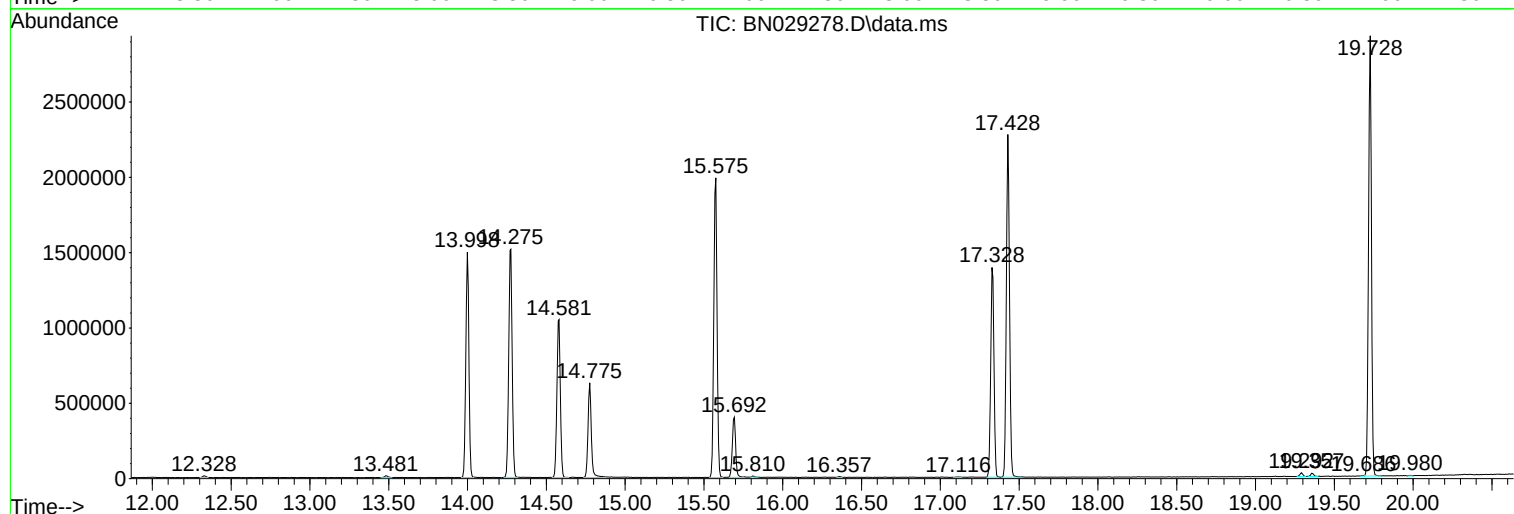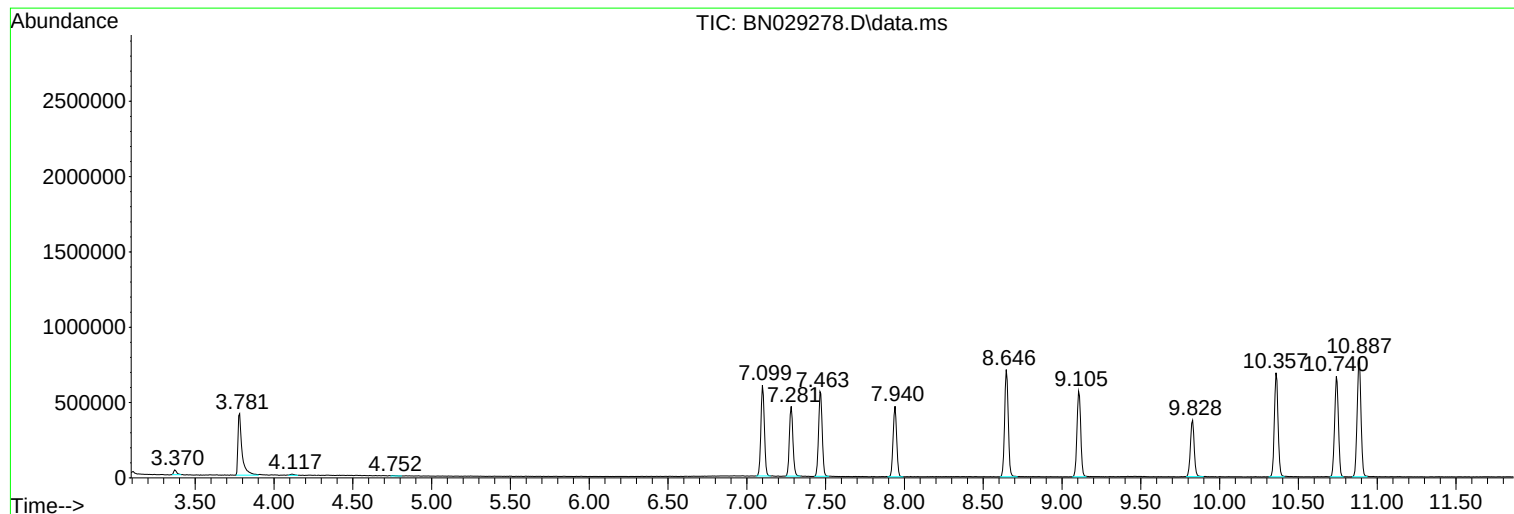

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029278.D
Acq On : 17 Jan 2024 18:49
Operator : MA/JU
Sample : PB158437BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK437

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029278.D
Acq On : 17 Jan 2024 18:49
Operator : MA/JU
Sample : PB158437BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK437

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------