

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
 Data File : BN029280.D
 Acq On : 17 Jan 2024 20:01
 Operator : MA/JU
 Sample : PB158368BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK368

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029280.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	59	rVB	32143	48912	1.24%	0.130%
2	3.781	114	118	140	rBV	397986	705695	17.83%	1.870%
3	4.116	171	175	181	rVB2	5982	9797	0.25%	0.026%
4	4.334	210	212	217	rBV5	2854	4206	0.11%	0.011%
5	7.099	675	682	694	rVB	578215	901355	22.77%	2.389%
6	7.281	706	713	724	rVB	462479	724828	18.31%	1.921%
7	7.463	737	744	755	rBV	544771	881140	22.26%	2.335%
8	7.940	817	825	835	rBV	419066	664021	16.78%	1.760%
9	8.646	938	945	956	rBV	698262	1113113	28.12%	2.950%
10	9.104	1015	1023	1033	rBV	559284	929234	23.48%	2.462%
11	9.451	1073	1082	1083	rBV7	2351	6502	0.16%	0.017%
12	9.828	1135	1146	1156	rBV	373310	616042	15.56%	1.632%
13	10.357	1228	1236	1248	rBV	680429	1121288	28.33%	2.971%
14	10.740	1294	1301	1309	rBV	583668	1001579	25.31%	2.654%
15	10.887	1318	1326	1335	rBV	779540	1326446	33.51%	3.515%
16	12.328	1567	1571	1578	rVB2	12712	21940	0.55%	0.058%
17	13.487	1763	1768	1772	rVB2	10940	16878	0.43%	0.045%
18	13.998	1847	1855	1864	rBV	1522774	2042721	51.61%	5.413%
19	14.269	1893	1901	1911	rBV	1507813	2302306	58.17%	6.101%
20	14.575	1947	1953	1964	rVB	972536	1446569	36.55%	3.833%
21	14.775	1980	1987	1999	rBV	664313	935464	23.64%	2.479%
22	15.575	2116	2123	2132	rBV	2051873	2918657	73.74%	7.734%
23	15.692	2137	2143	2153	rBV	424410	604529	15.27%	1.602%
24	15.816	2160	2164	2168	rVB5	6862	9972	0.25%	0.026%
25	16.363	2252	2257	2261	rVB4	5716	7727	0.20%	0.020%
26	17.116	2378	2385	2390	rVB7	2518	6087	0.15%	0.016%
27	17.327	2414	2421	2428	rBV	1267954	1819682	45.98%	4.822%
28	17.427	2431	2438	2447	rBV	2266889	3220400	81.37%	8.534%
29	18.257	2573	2579	2582	rVB6	2499	4271	0.11%	0.011%
30	19.292	2750	2755	2759	rVB2	23144	31942	0.81%	0.085%
31	19.357	2762	2766	2771	rVV	23561	28943	0.73%	0.077%
32	19.727	2823	2829	2836	rVV	2966267	3793785	95.85%	10.053%
33	20.280	2920	2923	2924	rBV2	3285	4007	0.10%	0.011%
34	21.527	3130	3135	3142	rBV	1472849	1997249	50.46%	5.293%
35	23.280	3429	3433	3438	rVB5	29595	46864	1.18%	0.124%
36	23.792	3511	3520	3533	rBV2	2021473	3957883	100.00%	10.488%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029280.D
Acq On : 17 Jan 2024 20:01
Operator : MA/JU
Sample : PB158368BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK368

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION

37	23.945	3537	3546	3558	rVB	1085351	2261331	57.13%	5.992%
38	24.674	3665	3670	3677	rVB2	43601	96031	2.43%	0.254%
39	25.545	3813	3818	3828	rVB4	45837	107068	2.71%	0.284%




Sum of corrected areas: 37736464

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029280.D
Acq On : 17 Jan 2024 20:01
Operator : MA/JU
Sample : PB158368BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK368

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

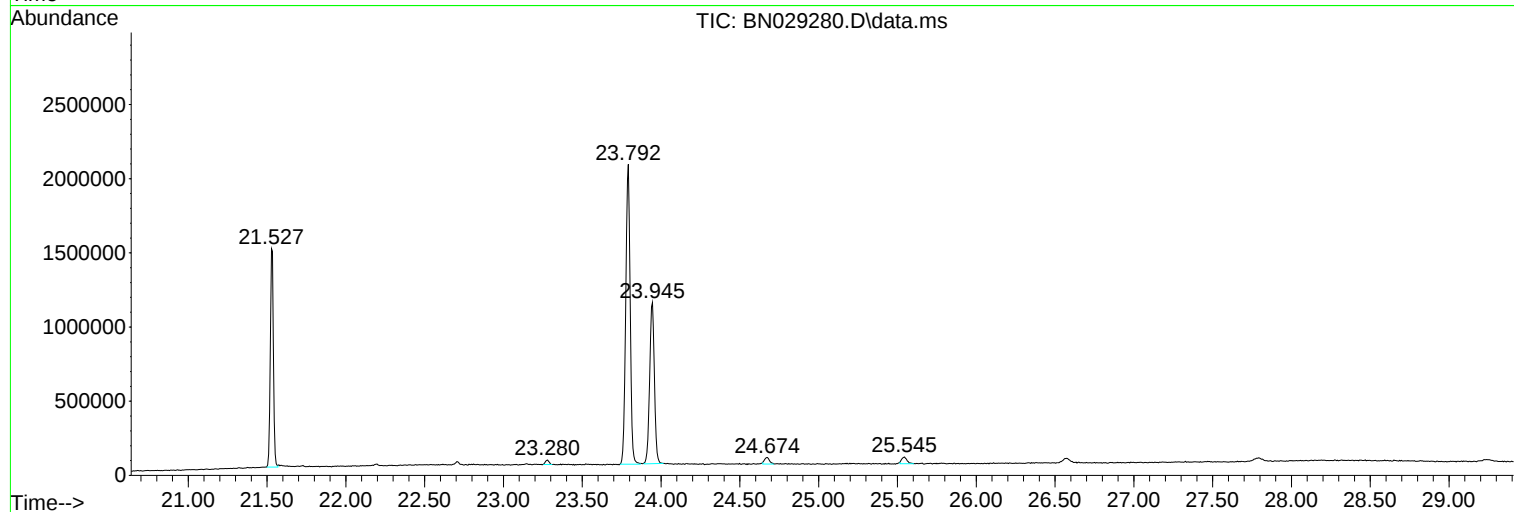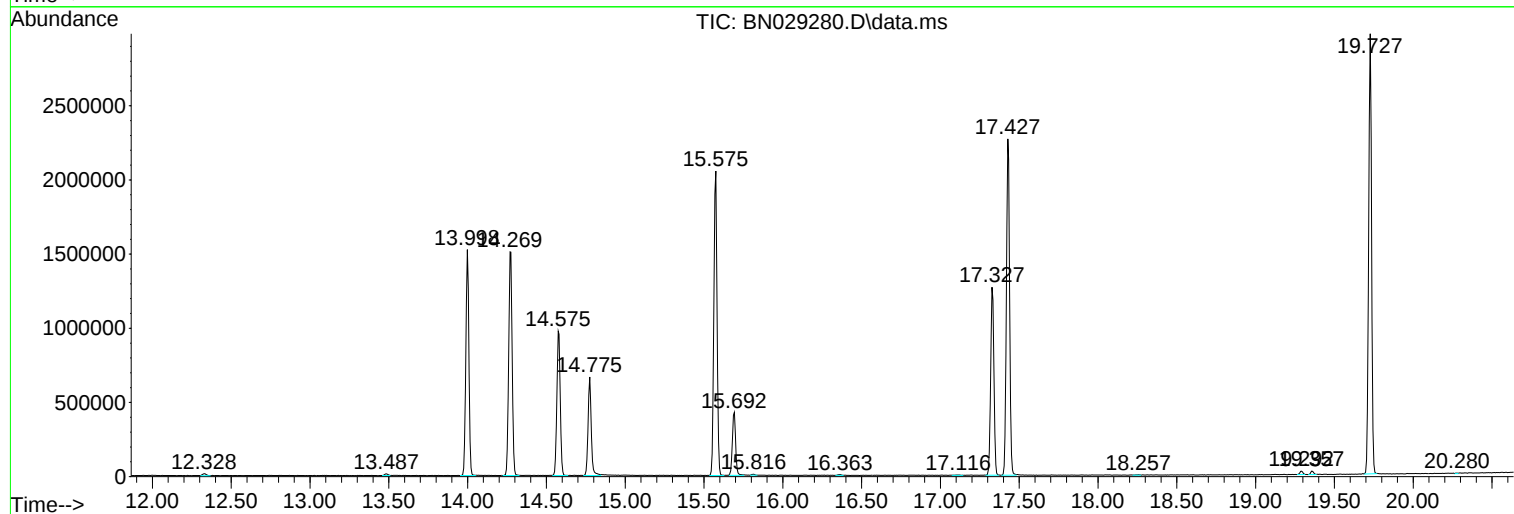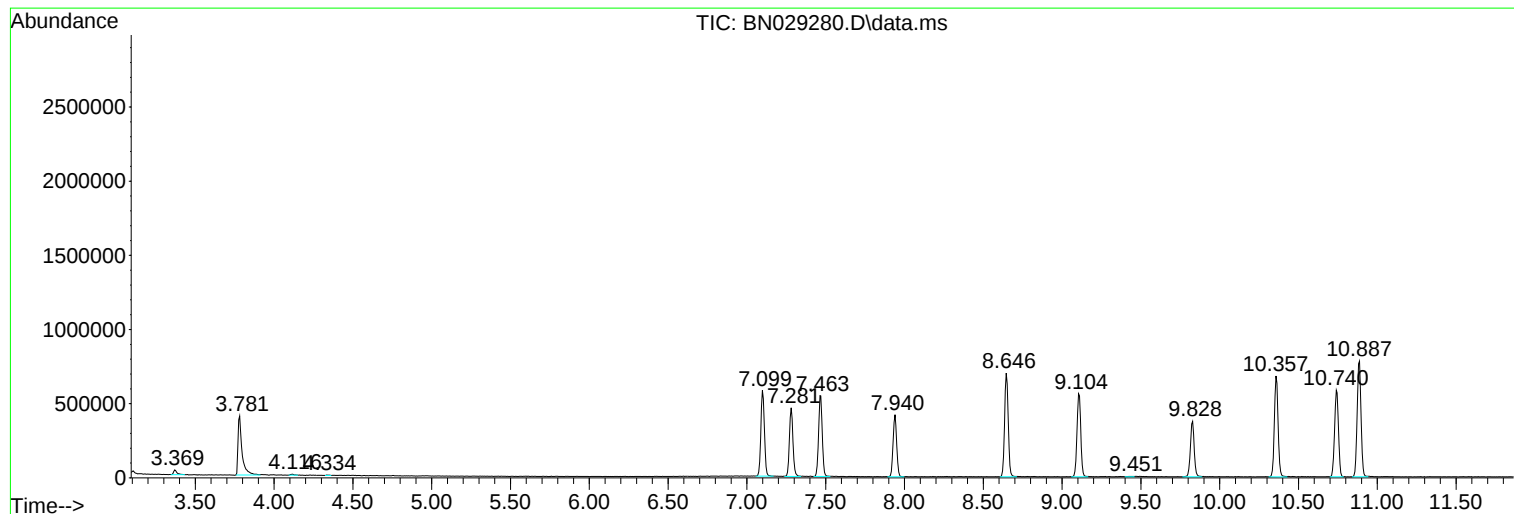

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029280.D
Acq On : 17 Jan 2024 20:01
Operator : MA/JU
Sample : PB158368BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK368

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029280.D
Acq On : 17 Jan 2024 20:01
Operator : MA/JU
Sample : PB158368BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK368

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc