

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
 Data File : BN029282.D
 Acq On : 17 Jan 2024 21:13
 Operator : MA/JU
 Sample : PB158370BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK370

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	59	rVB	37532	60466	1.52%	0.153%
2	3.781	114	118	134	rBV	433623	741038	18.62%	1.872%
3	4.111	171	174	181	rVB2	8795	12441	0.31%	0.031%
4	7.099	675	682	690	rVB	601553	926454	23.28%	2.341%
5	7.281	705	713	726	rBV	486317	755665	18.99%	1.909%
6	7.463	737	744	757	rBV	569517	917424	23.05%	2.318%
7	7.940	818	825	832	rBV	469861	742233	18.65%	1.875%
8	8.646	938	945	956	rBV	721913	1155896	29.04%	2.920%
9	9.105	1015	1023	1034	rBV	583098	968620	24.34%	2.447%
10	9.828	1133	1146	1156	rBV	394630	650437	16.34%	1.643%
11	10.357	1227	1236	1251	rBV	701819	1160860	29.17%	2.933%
12	10.740	1293	1301	1310	rVB	666435	1133795	28.49%	2.865%
13	10.887	1318	1326	1339	rBV	803728	1383131	34.75%	3.494%
14	12.328	1566	1571	1578	rVB3	13578	21136	0.53%	0.053%
15	13.487	1761	1768	1774	rBV3	14235	22845	0.57%	0.058%
16	13.998	1848	1855	1865	rBV	1532474	2119870	53.26%	5.356%
17	14.275	1895	1902	1909	rBV	1603382	2396631	60.22%	6.055%
18	14.575	1946	1953	1964	rVB2	1080889	1617382	40.64%	4.086%
19	14.775	1980	1987	2003	rBV	686231	973482	24.46%	2.460%
20	14.998	2020	2025	2031	rVB9	2492	6056	0.15%	0.015%
21	15.575	2115	2123	2130	rBV	2193149	3047692	76.58%	7.700%
22	15.692	2136	2143	2154	rBV	455281	628211	15.78%	1.587%
23	15.810	2159	2163	2168	rVB4	8019	11872	0.30%	0.030%
24	16.363	2252	2257	2262	rVB5	6268	8587	0.22%	0.022%
25	17.110	2381	2384	2387	rBV3	3432	4620	0.12%	0.012%
26	17.328	2414	2421	2428	rBV	1453019	2045033	51.38%	5.167%
27	17.428	2432	2438	2451	rVV	2391083	3338932	83.90%	8.436%
28	18.551	2628	2629	2636	rBV6	2952	5309	0.13%	0.013%
29	19.175	2734	2735	2740	rBV5	2807	4250	0.11%	0.011%
30	19.286	2750	2754	2759	rVB2	23706	35287	0.89%	0.089%
31	19.357	2762	2766	2772	rVB	22616	32395	0.81%	0.082%
32	19.727	2823	2829	2838	rVB	2842444	3846264	96.64%	9.718%
33	20.333	2930	2932	2936	rBV4	4888	4360	0.11%	0.011%
34	21.527	3130	3135	3143	rBV	1720909	2212332	55.59%	5.589%
35	23.274	3429	3432	3443	rVB4	38768	65024	1.63%	0.164%
36	23.786	3511	3519	3530	rBV2	2052631	3979881	100.00%	10.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029282.D
Acq On : 17 Jan 2024 21:13
Operator : MA/JU
Sample : PB158370BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Title : SVOA CALIBRATION

37	23.945	3537	3546	3557	rVB	1172751	2458226	61.77%	6.211%
38	24.668	3665	3669	3675	rVB4	44047	86216	2.17%	0.218%




Sum of corrected areas: 39580353

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029282.D
Acq On : 17 Jan 2024 21:13
Operator : MA/JU
Sample : PB158370BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

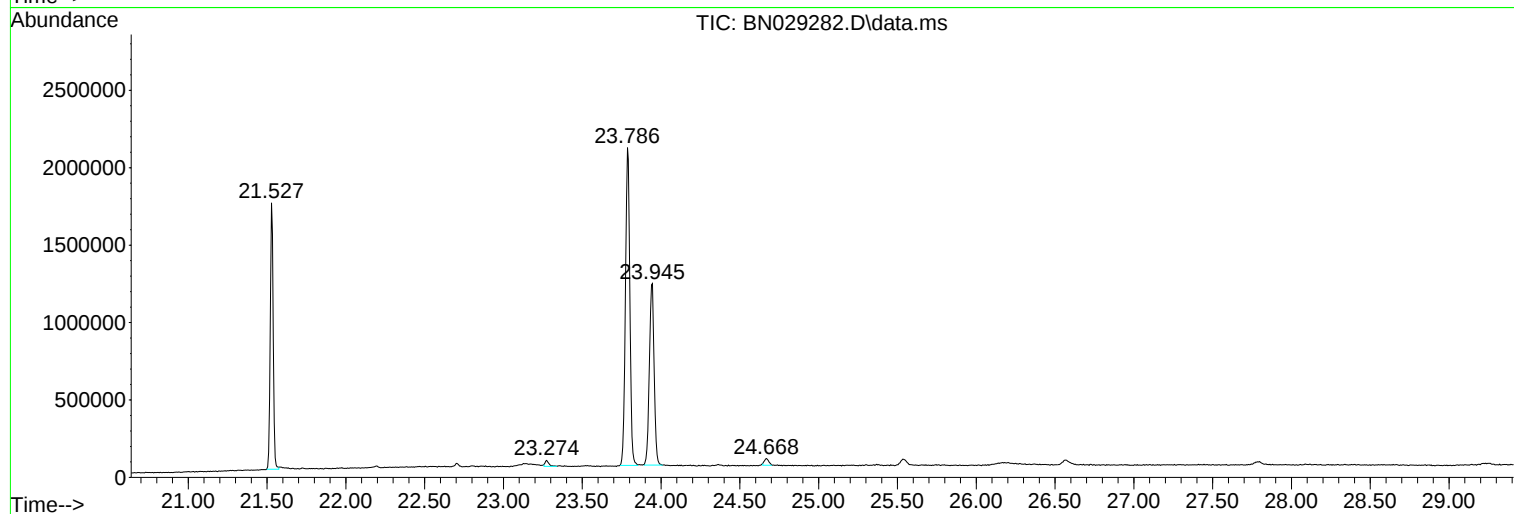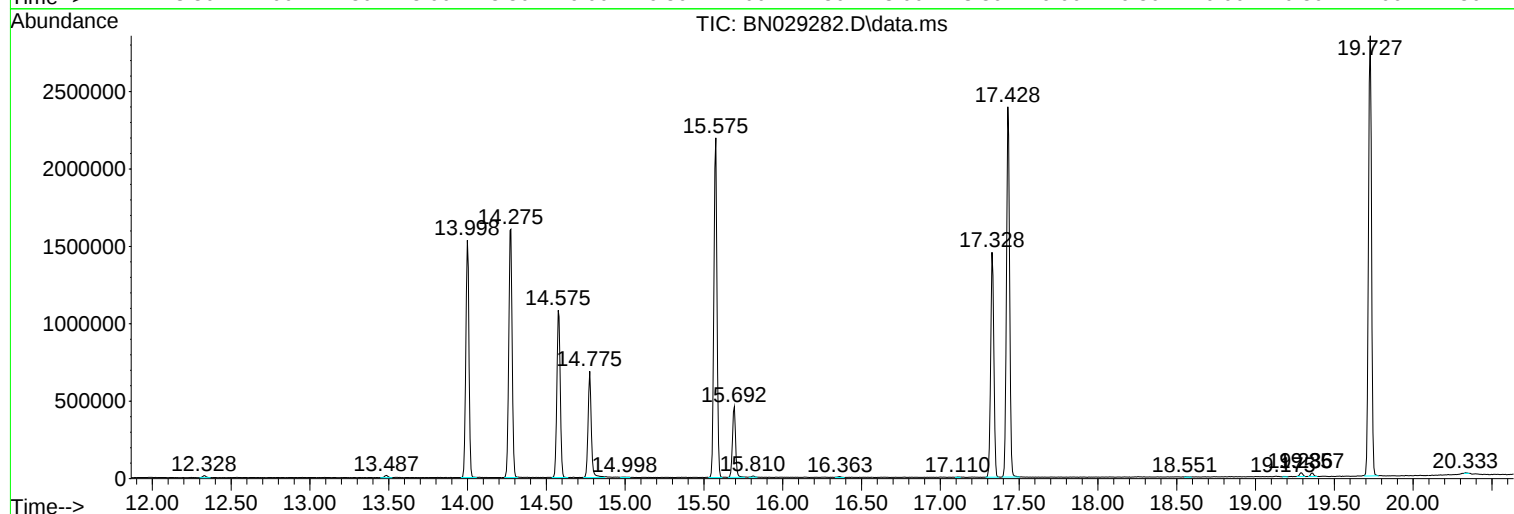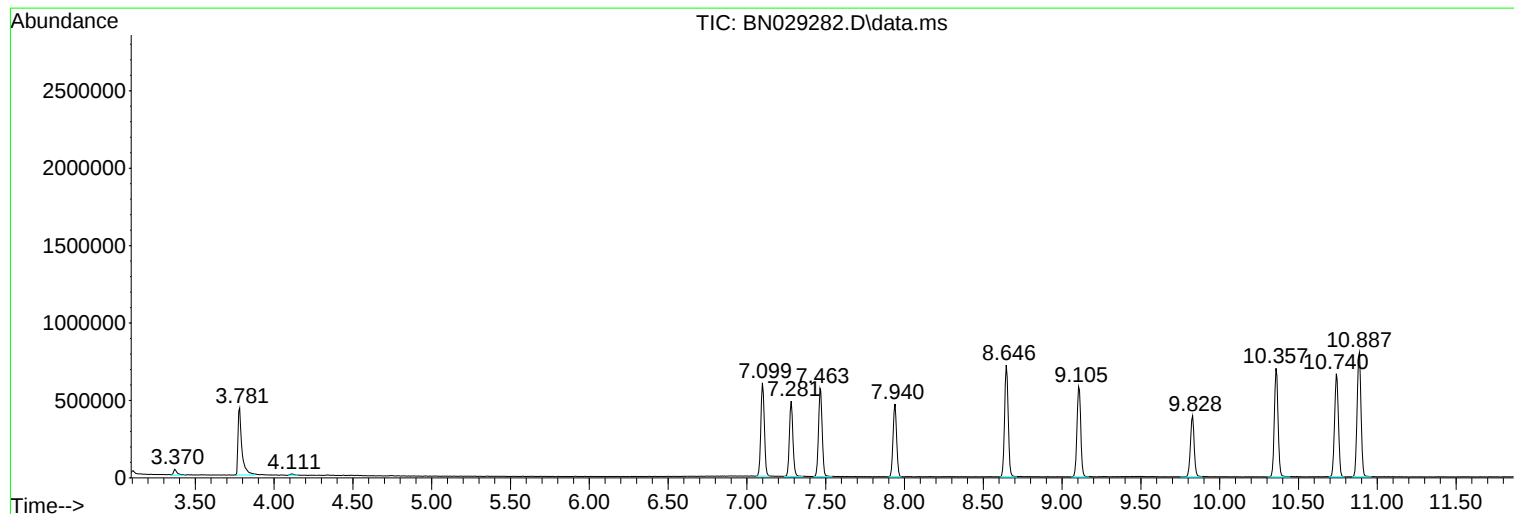

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029282.D
Acq On : 17 Jan 2024 21:13
Operator : MA/JU
Sample : PB158370BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011724\
Data File : BN029282.D
Acq On : 17 Jan 2024 21:13
Operator : MA/JU
Sample : PB158370BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN011524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc