

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
 Data File : BN035976.D
 Acq On : 18 Jan 2025 06:39
 Operator : RC/JU
 Sample : PB166121BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK121

Quant Time: Jan 19 23:52:52 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 10:40:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	1897	0.400	ng/ul	0.00
4) Naphthalene-d8	10.615	136	3883	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.454	164	2157	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.372	240	3638	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.68
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	14312	7.483	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.204	152	1818	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.220	212	3835	0.398	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.449	166	705	0.093	ng/ul#	18
20) Pyrene	19.587	202	662	0.050	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
Data File : BN035976.D
Acq On : 18 Jan 2025 06:39
Operator : RC/JU
Sample : PB166121BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK121

Quant Time: Jan 19 23:52:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 10:40:45 2025
Response via : Initial Calibration




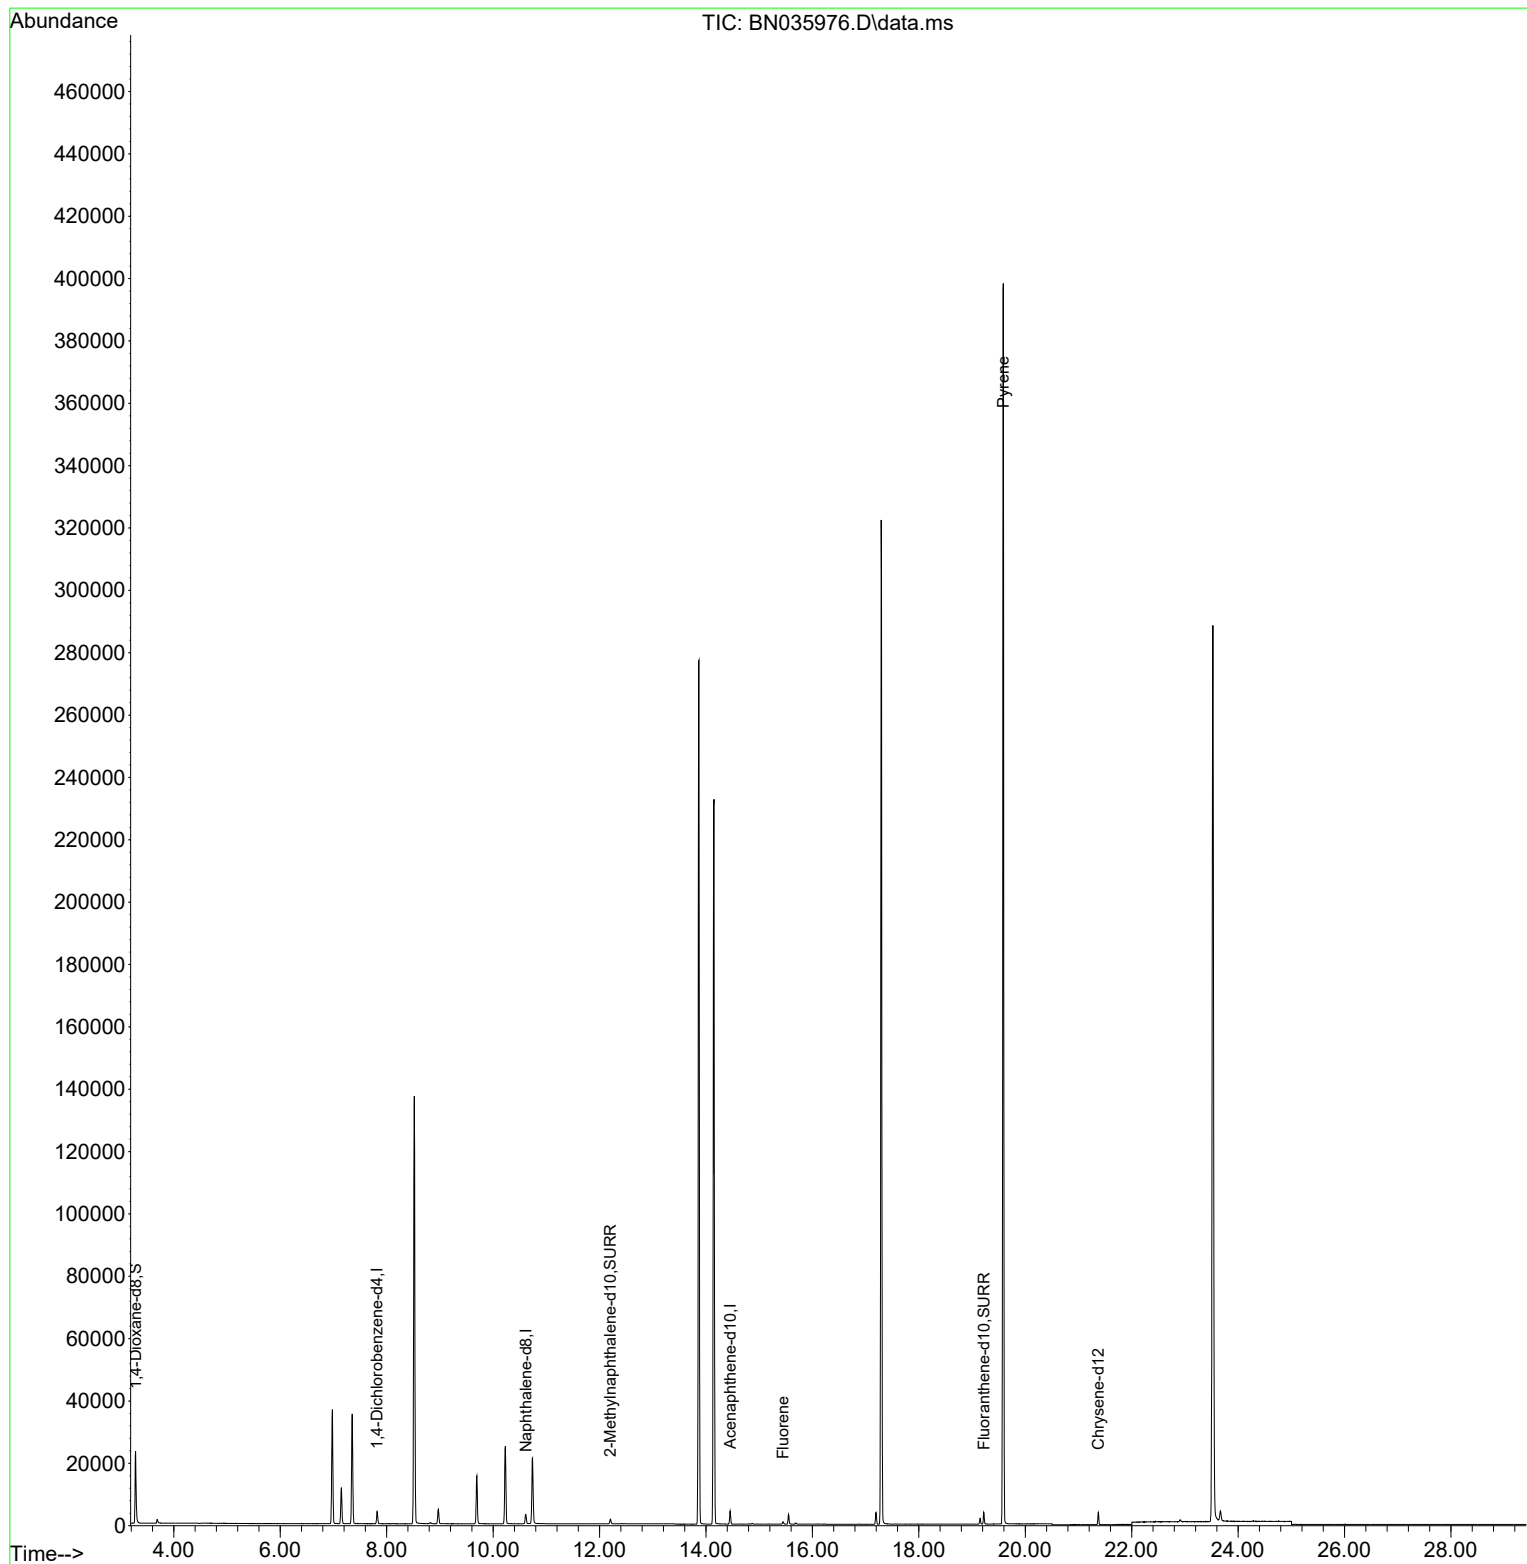


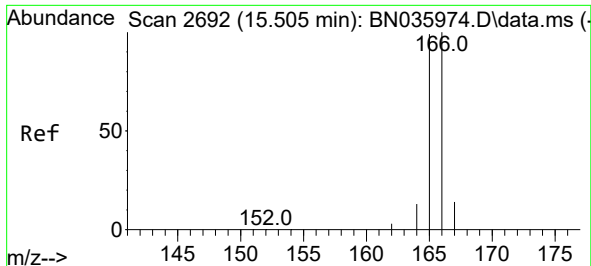

#12
Fluorene
Concen: 0.093 ng/ul
RT: 15.449 min Scan# 2680
Delta R.T. -0.061 min
Lab File: BN035976.D
Acq: 18 Jan 2025 06:39

Instrument :
BNA_N
ClientSampleId :
SBLK121

Tgt Ion:166 Resp: 705
Ion Ratio Lower Upper
166 100
165 14.5 79.0 118.6#
167 41.3 12.2 18.4#

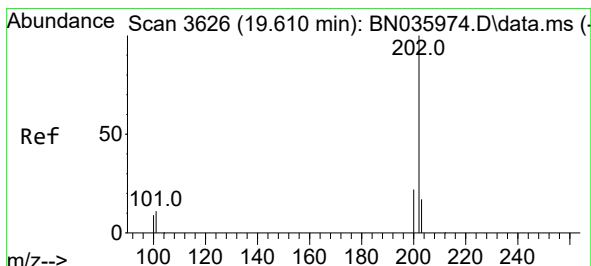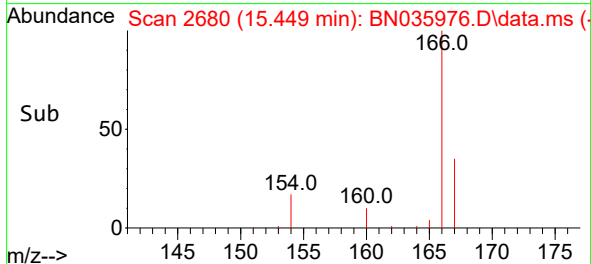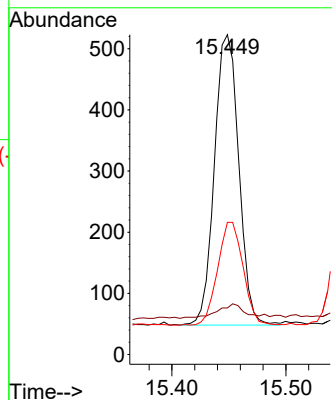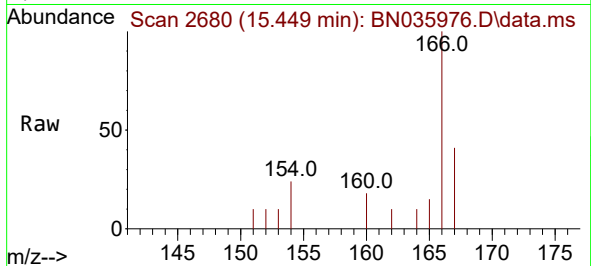

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.587 min Scan# 3621
Delta R.T. -0.032 min
Lab File: BN035976.D
Acq: 18 Jan 2025 06:39

Tgt Ion:202 Resp: 662
Ion Ratio Lower Upper
202 100
101 208.8 9.8 14.6#
100 1545.7 8.2 12.2#

