

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
 Data File : BN035980.D
 Acq On : 18 Jan 2025 09:03
 Operator : RC/JU
 Sample : Q1088-10
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B09

Quant Time: Jan 19 23:53:30 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 10:40:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	2805	0.400	ng/ul	0.00
4) Naphthalene-d8	10.611	136	6063	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.454	164	3422	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.371	240	6438	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.68
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	15321	5.418	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.205	152	3138	0.398	ng/ul	0.00
18) Fluoranthene-d10	19.219	212	8287	0.486	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	85	0.028	ng/ul#	54
20) Pyrene	19.587	202	1544	0.066	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
Data File : BN035980.D
Acq On : 18 Jan 2025 09:03
Operator : RC/JU
Sample : Q1088-10
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B09

Quant Time: Jan 19 23:53:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 10:40:45 2025
Response via : Initial Calibration




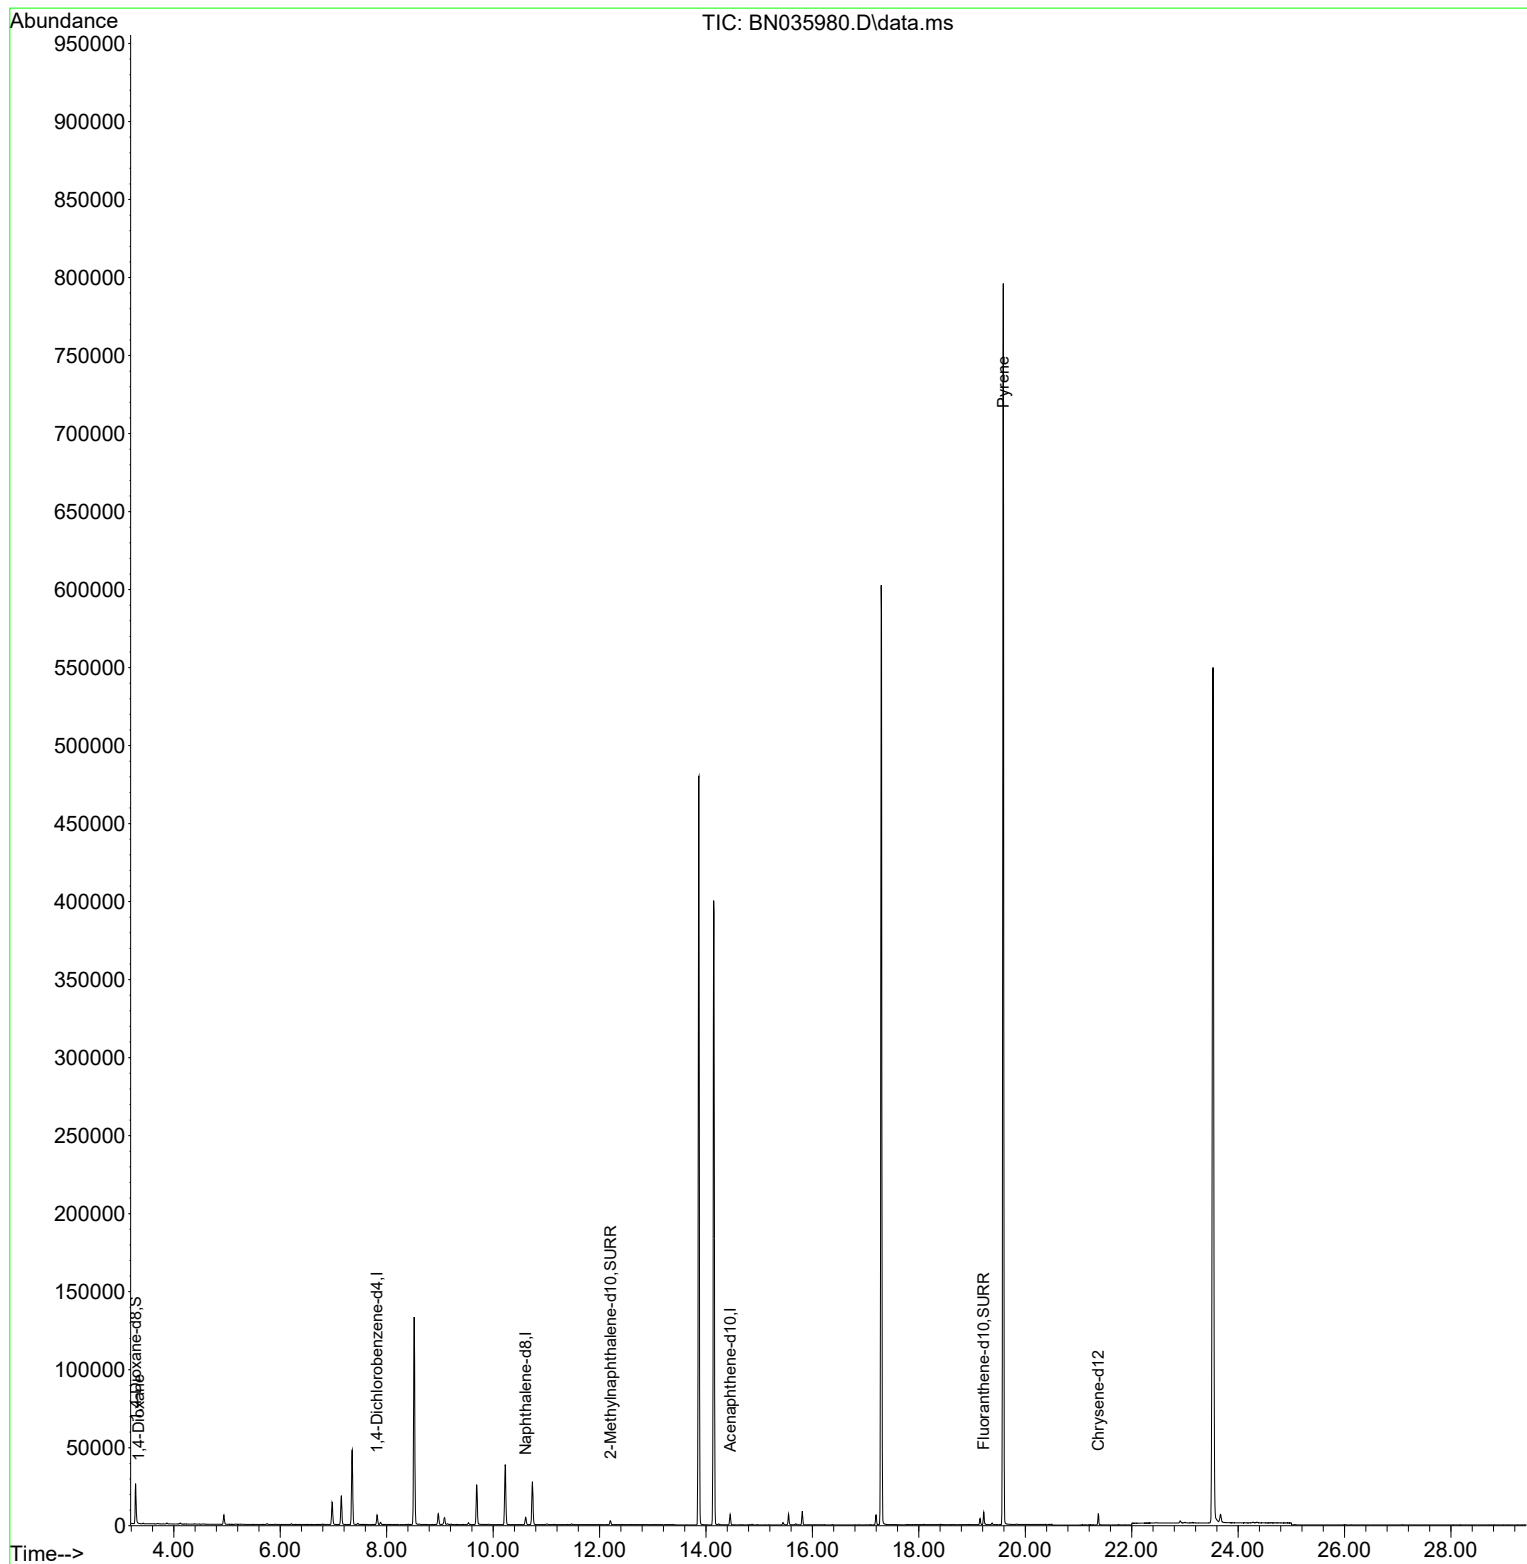


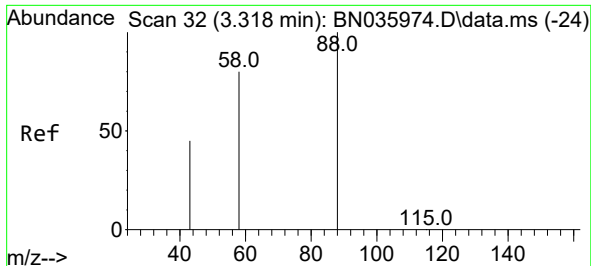

#2
1,4-Dioxane
Concen: 0.028 ng/ul
RT: 3.339 min Scan# 31
Delta R.T. 0.021 min
Lab File: BN035980.D
Acq: 18 Jan 2025 09:03

Instrument :
BNA_N
ClientSampleId :
C0B09

Tgt Ion: 88 Resp: 85
Ion Ratio Lower Upper
88 100
43 112.3 57.8 86.8#
58 38.2 60.0 90.0#

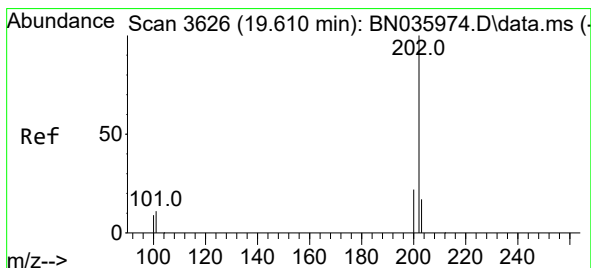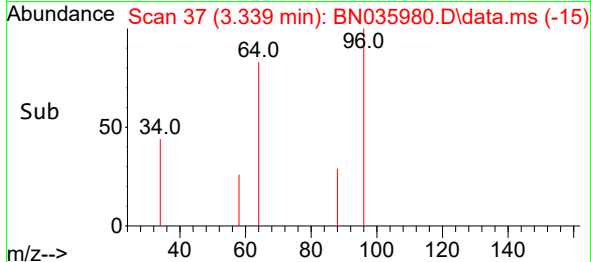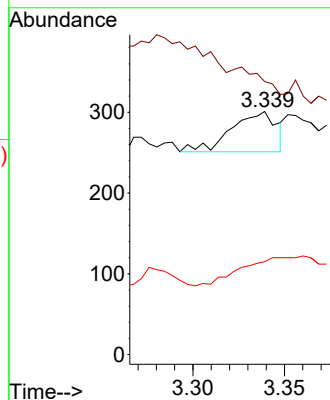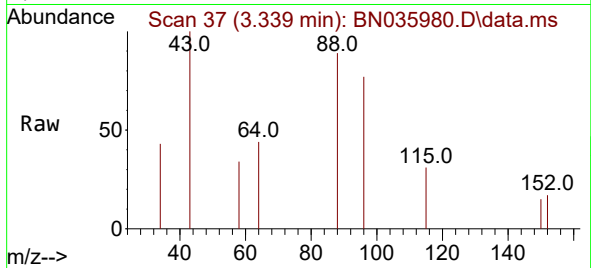

#20
Pyrene
Concen: 0.066 ng/ul
RT: 19.587 min Scan# 3621
Delta R.T. -0.033 min
Lab File: BN035980.D
Acq: 18 Jan 2025 09:03

Tgt Ion: 202 Resp: 1544
Ion Ratio Lower Upper
202 100
101 199.0 9.8 14.6#
100 1454.6 8.2 12.2#

