

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
 Data File : BN035981.D
 Acq On : 18 Jan 2025 09:39
 Operator : RC/JU
 Sample : Q1088-11
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B10

Quant Time: Jan 19 23:53:37 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 10:40:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	2759	0.400	ng/ul	0.00
4) Naphthalene-d8	10.611	136	5830	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.454	164	3302	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.371	240	6029	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.68
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	14702	5.285	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.205	152	3037	0.401	ng/ul	0.00
18) Fluoranthene-d10	19.219	212	7249	0.454	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.364	88	281	0.093	ng/ul#	78
20) Pyrene	19.582	202	1229	0.056	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
Data File : BN035981.D
Acq On : 18 Jan 2025 09:39
Operator : RC/JU
Sample : Q1088-11
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Quant Time: Jan 19 23:53:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 10:40:45 2025
Response via : Initial Calibration




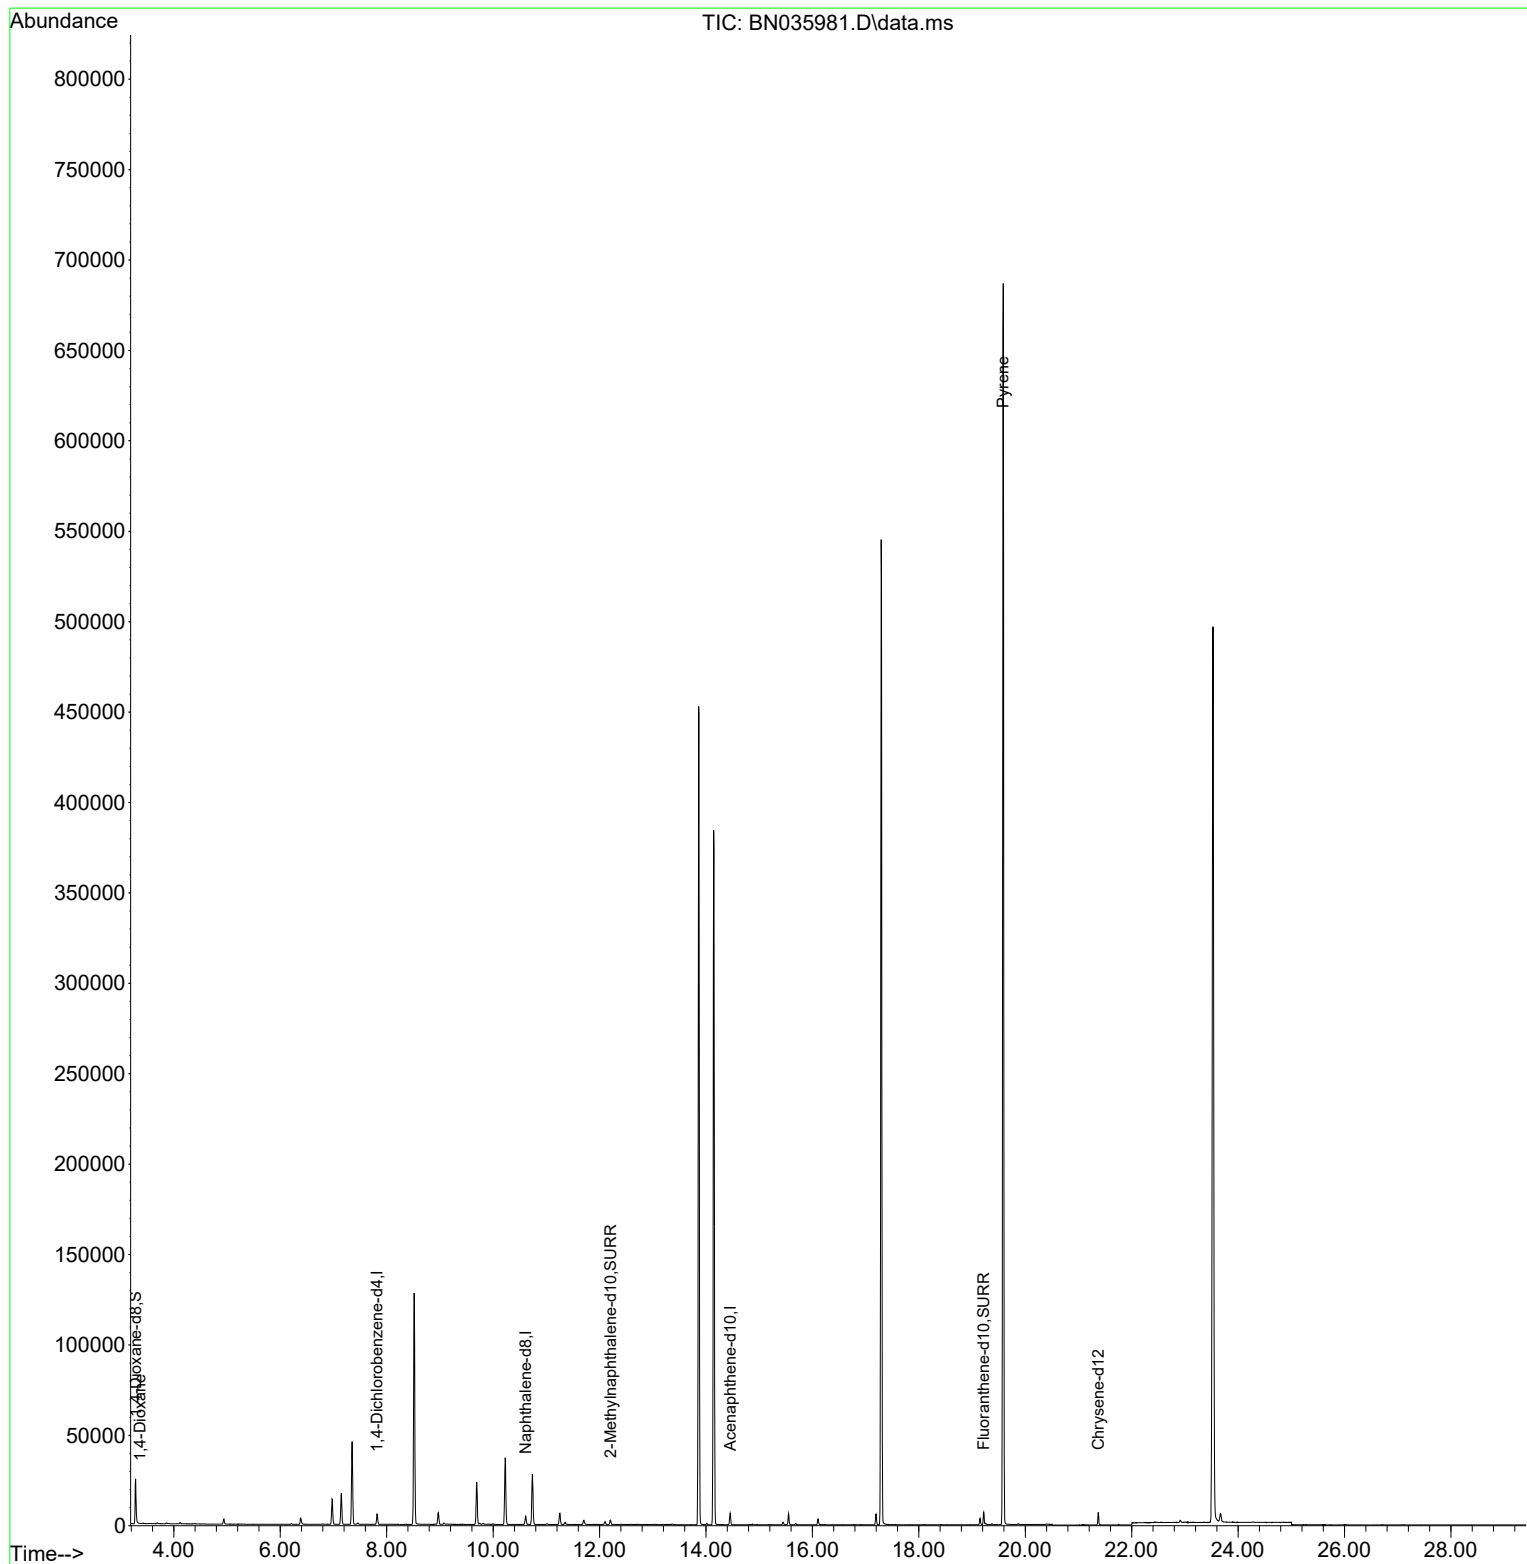


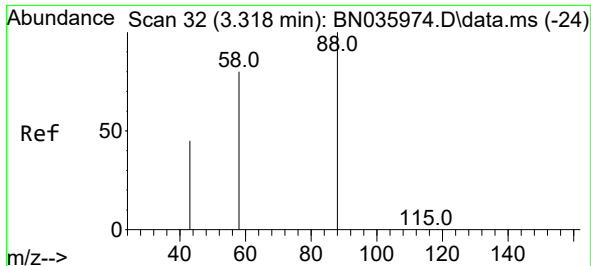

#2
1,4-Dioxane
Concen: 0.093 ng/ul
RT: 3.364 min Scan# 41
Delta R.T. 0.046 min
Lab File: BN035981.D
Acq: 18 Jan 2025 09:39

Instrument :
BNA_N
ClientSampleId :
C0B10

Tgt Ion: 88 Resp: 281
Ion Ratio Lower Upper
88 100
43 93.9 57.8 86.8#
58 59.3 60.0 90.0#

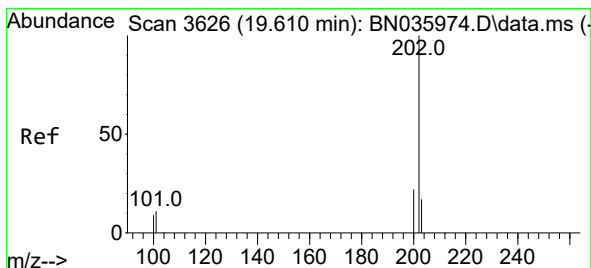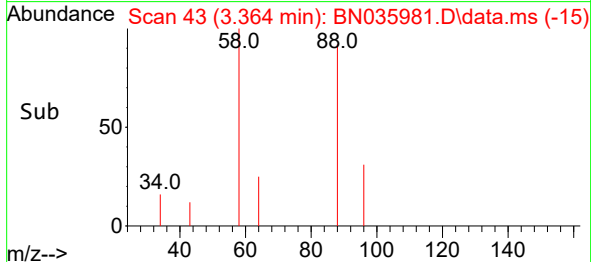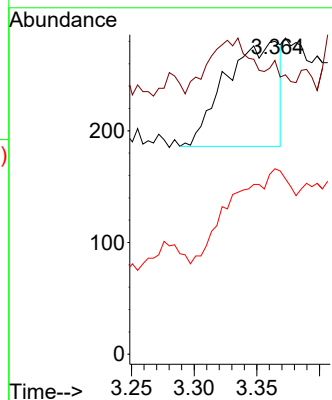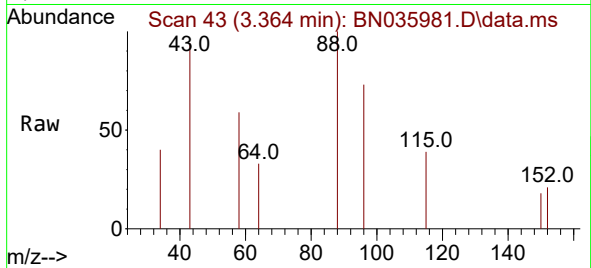

#20
Pyrene
Concen: 0.056 ng/ul
RT: 19.582 min Scan# 3620
Delta R.T. -0.037 min
Lab File: BN035981.D
Acq: 18 Jan 2025 09:39

Tgt Ion: 202 Resp: 1229
Ion Ratio Lower Upper
202 100
101 212.3 9.8 14.6#
100 1617.3 8.2 12.2#

