

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
 Data File : BN035987.D
 Acq On : 18 Jan 2025 13:15
 Operator : RC/JU
 Sample : PB166088BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK088

Quant Time: Jan 19 23:54:34 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 10:40:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	2497	0.400	ng/ul	0.00
4) Naphthalene-d8	10.611	136	5304	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.455	164	3133	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.372	240	5749	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.68
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	16013	6.361	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.200	152	2298	0.333	ng/ul	-0.01
18) Fluoranthene-d10	19.220	212	5468	0.359	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.449	166	950	0.087	ng/ul#	17
20) Pyrene	19.587	202	915	0.044	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
Data File : BN035987.D
Acq On : 18 Jan 2025 13:15
Operator : RC/JU
Sample : PB166088BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK088

Quant Time: Jan 19 23:54:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 10:40:45 2025
Response via : Initial Calibration




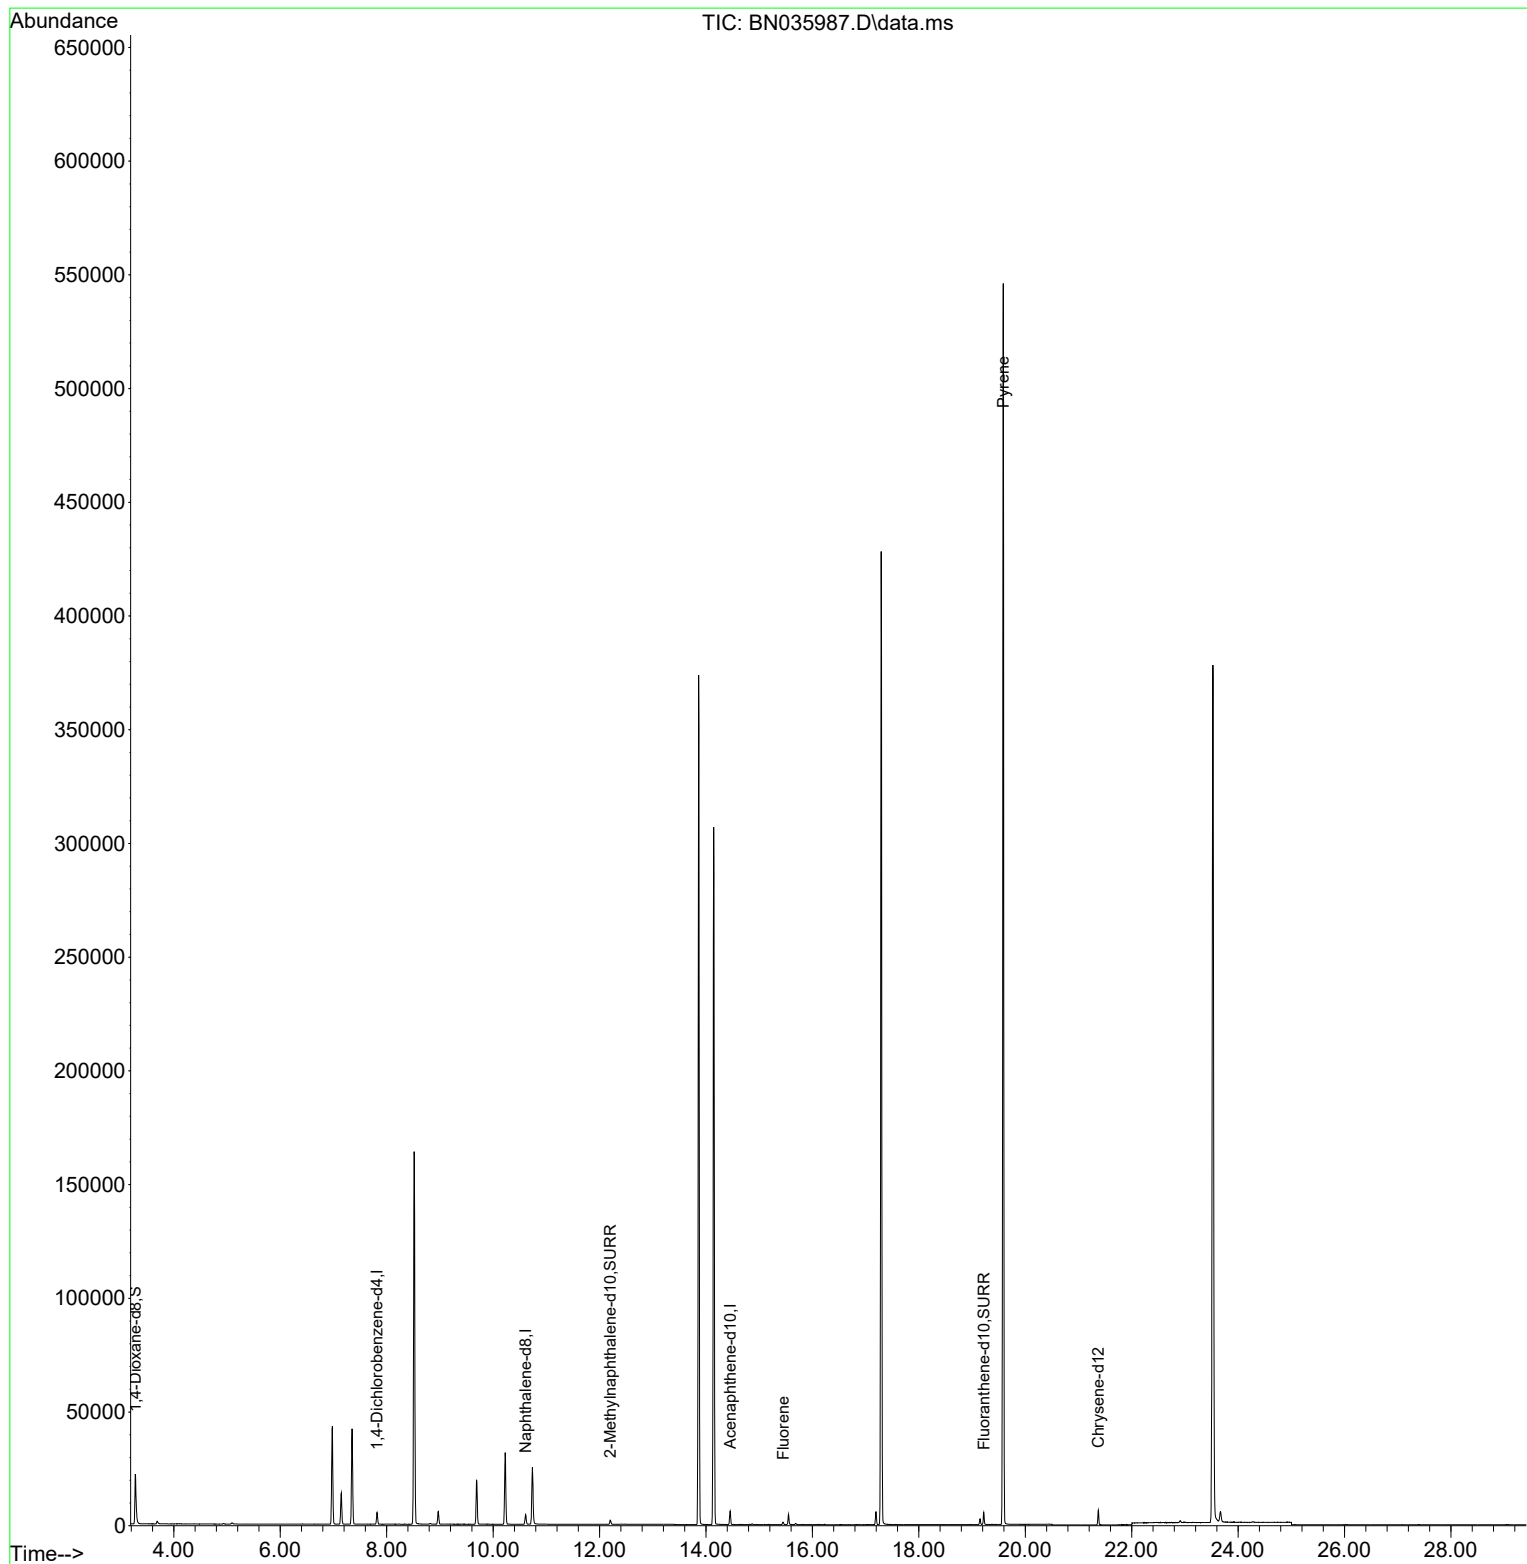


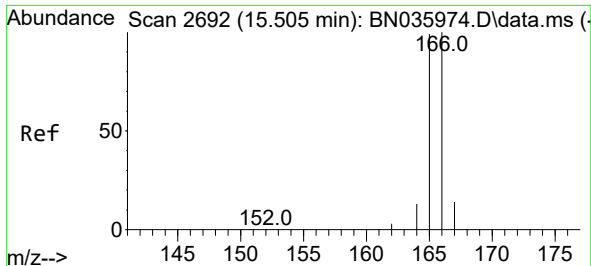

#12
Fluorene
Concen: 0.087 ng/ul
RT: 15.449 min Scan# 2680
Delta R.T. -0.060 min
Lab File: BN035987.D
Acq: 18 Jan 2025 13:15

Instrument :
BNA_N
ClientSampleId :
SBLK088

Tgt Ion:166 Resp: 950
Ion Ratio Lower Upper
166 100
165 12.4 79.0 118.6#
167 38.6 12.2 18.4#

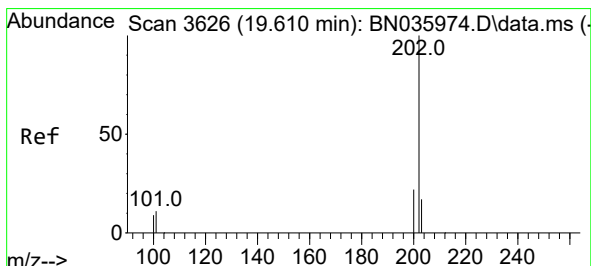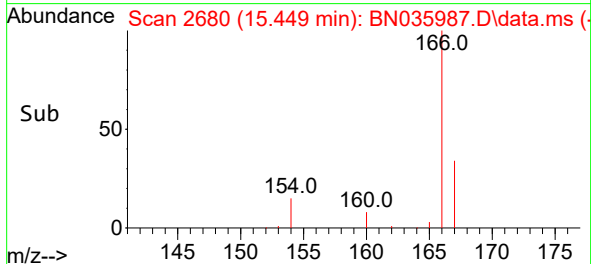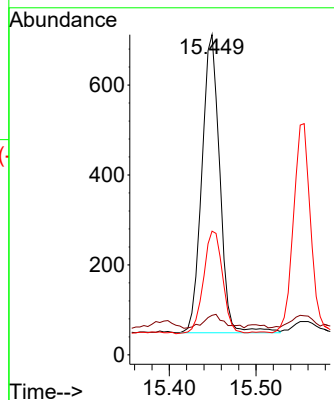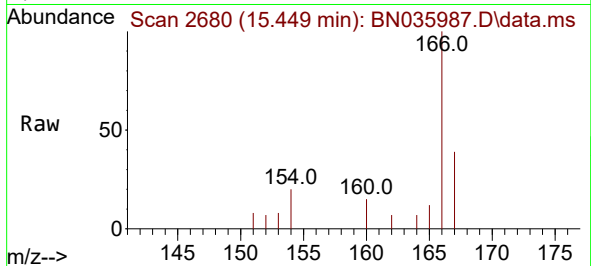

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.587 min Scan# 3621
Delta R.T. -0.032 min
Lab File: BN035987.D
Acq: 18 Jan 2025 13:15

Tgt Ion:202 Resp: 915
Ion Ratio Lower Upper
202 100
101 216.4 9.8 14.6#
100 1612.2 8.2 12.2#

