

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
 Data File : BN035952.D
 Acq On : 17 Jan 2025 15:02
 Operator : RC/JU
 Sample : Q1086-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/20/2025
 Supervised By :mohammad ahmed 01/20/2025

Quant Time: Jan 17 15:55:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 10:40:45 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.824	152	2290	0.400	ng/ul	0.00
4) Naphthalene-d8	10.616	136	4663	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.459	164	2565	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.195	188	5136m	0.400	ng/ul	0.00
17) Chrysene-d12	21.374	240	4097	0.400	ng/ul	0.00
23) Perylene-d12	23.671	264	3913m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	11109	4.812	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.205	152	2069	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.224	212	4647	0.428	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.318	88	4651	1.850	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011725\
Data File : BN035952.D
Acq On : 17 Jan 2025 15:02
Operator : RC/JU
Sample : Q1086-07
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AF8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/20/2025
Supervised By :mohammad ahmed 01/20/2025


Quant Time: Jan 17 15:55:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN123124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 10:40:45 2025
Response via : Initial Calibration

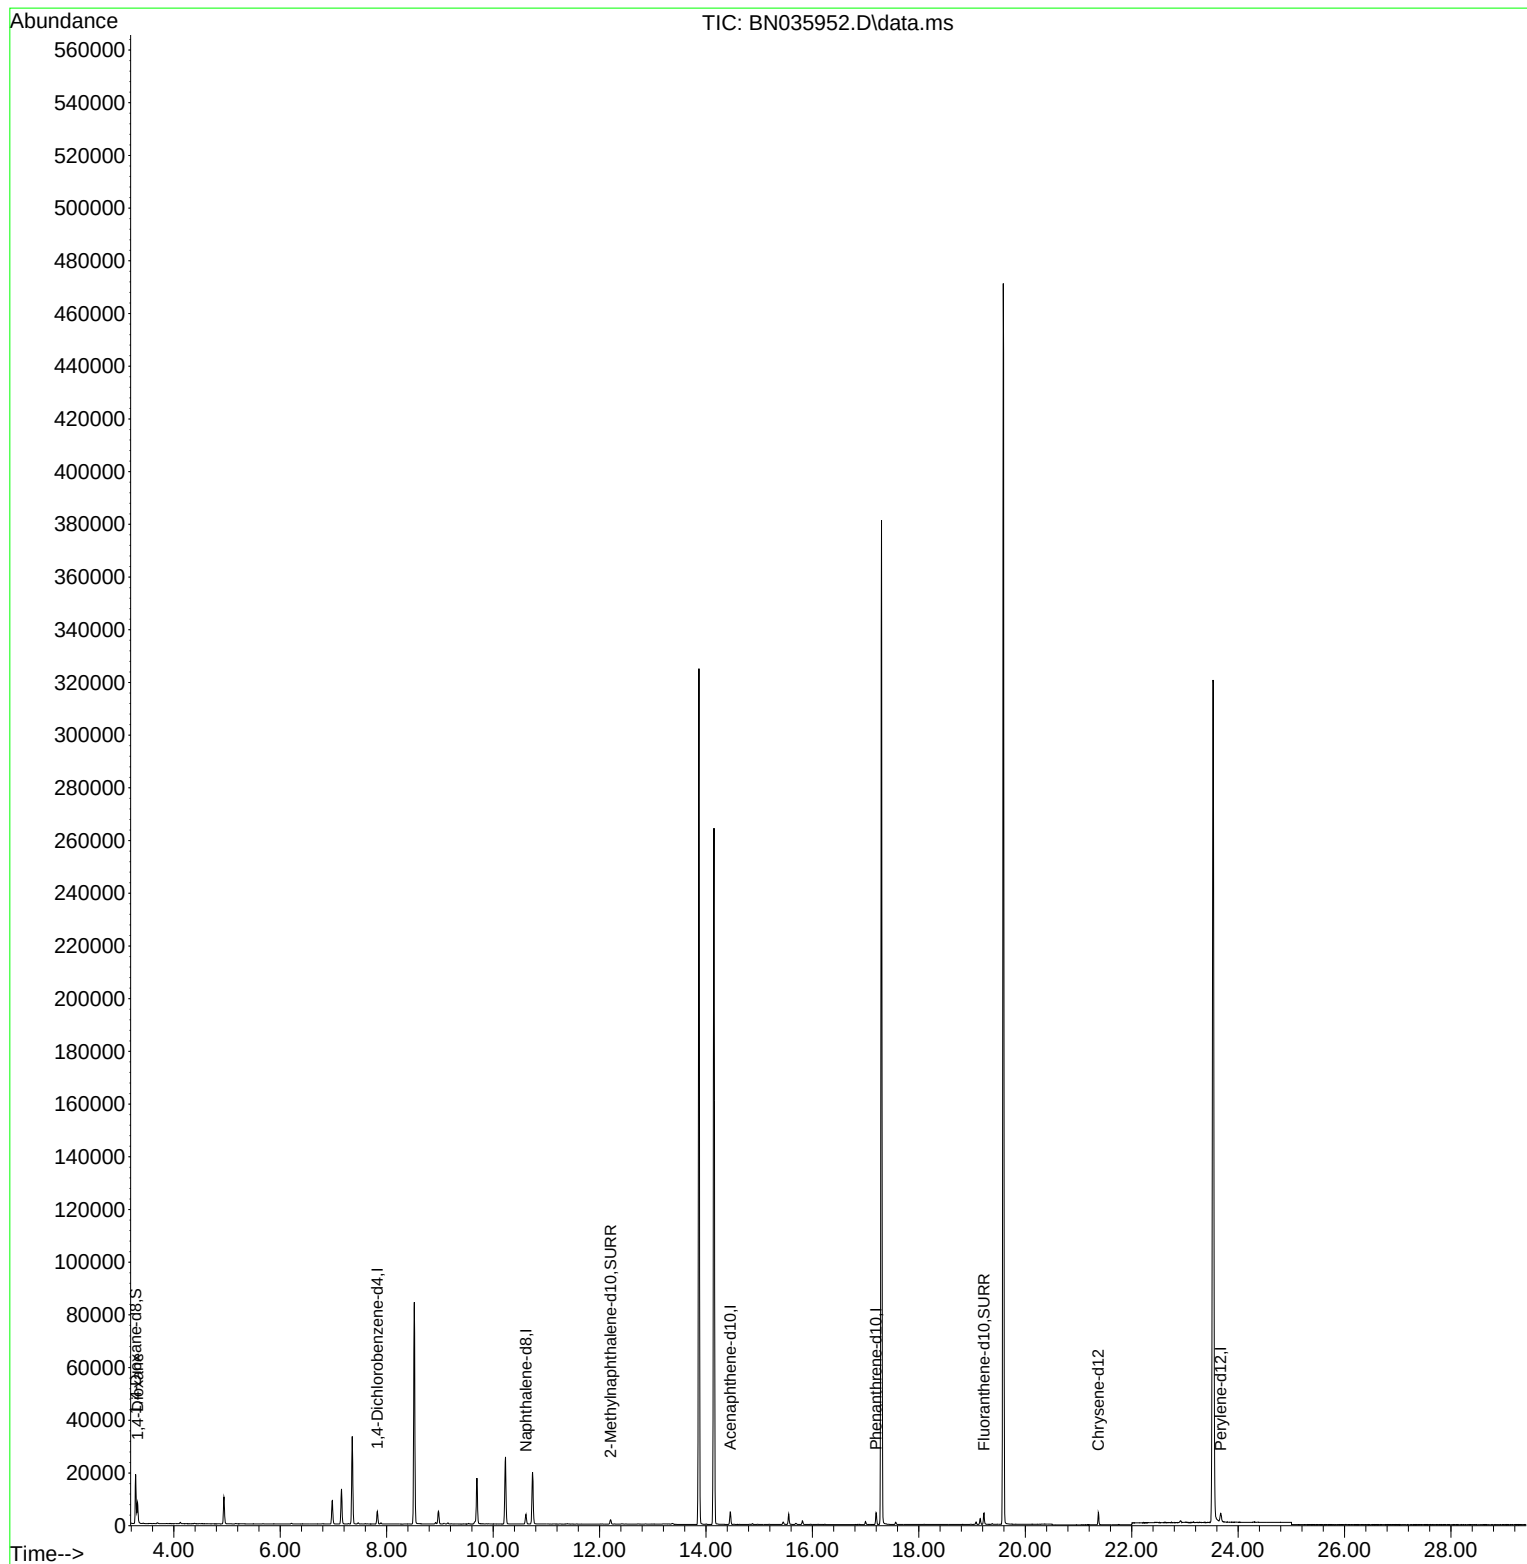

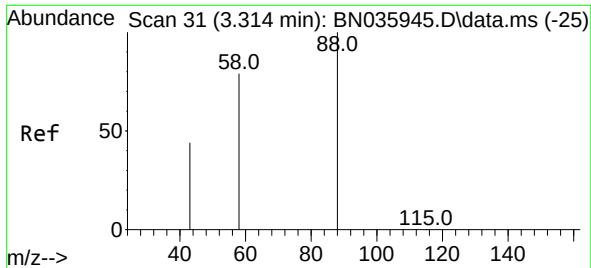

#2
 1,4-Dioxane
 Concen: 1.850 ng/ul
 RT: 3.318 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN035952.D
 Acq: 17 Jan 2025 15:02

Instrument :
 BNA_N
 ClientSampleId :
 C0AF8

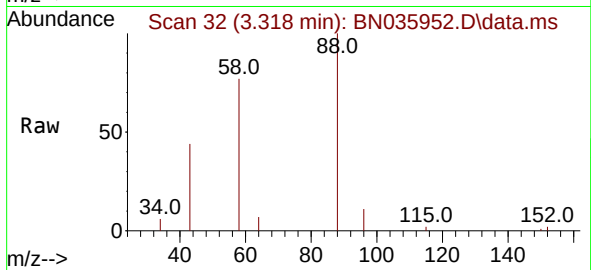

Tgt Ion: 88 Resp: 465
 Ion Ratio Lower Upper
 88 100
 43 44.2 57.8 86.8
 58 76.7 60.0 90.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/20/2025
 Supervised By :mohammad ahmed 01/20/2025

