
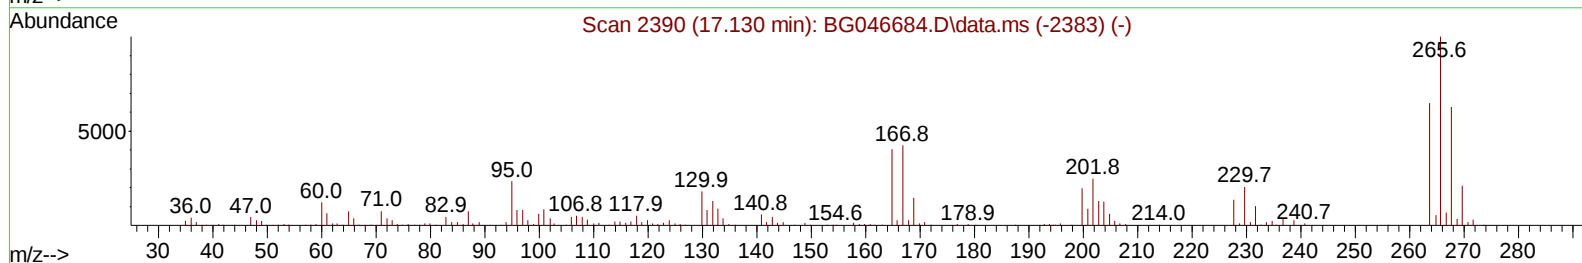
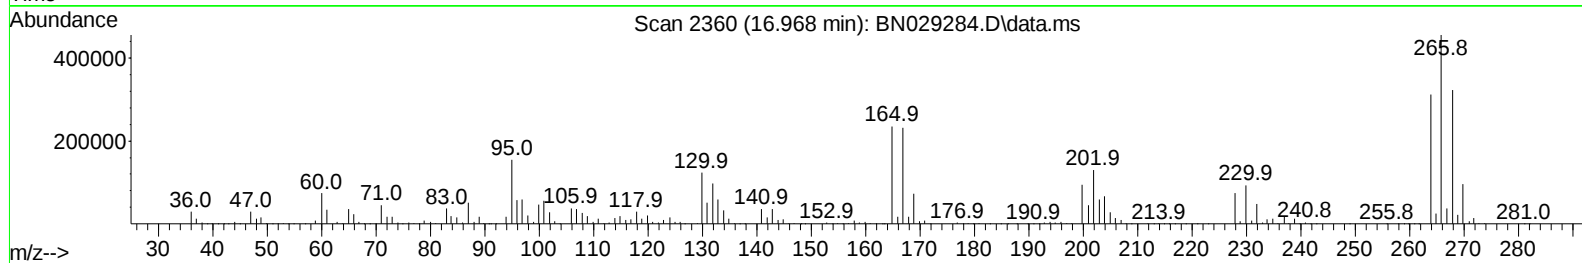


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011824\
Data File : BN029284.D
Acq On : 18 Jan 2024 10:13
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 01:39:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 01:39:16 2024
Response via : Initial Calibration

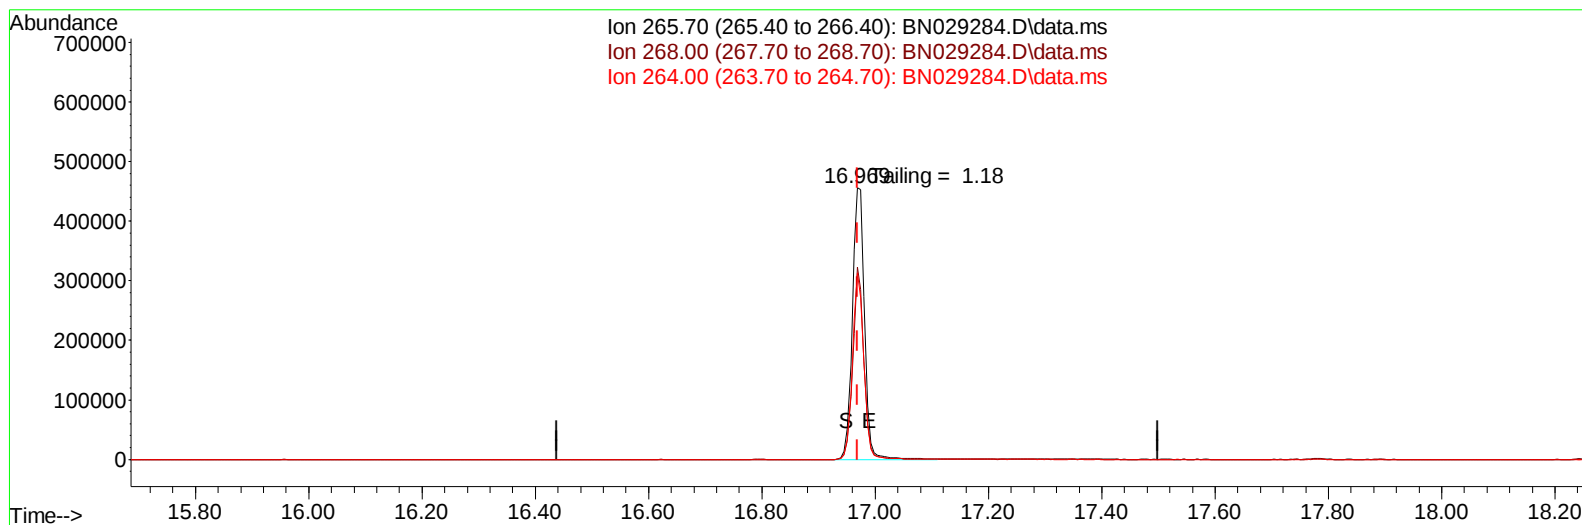




TIC: BN029284.D\data.ms

(70) Pentachloropheno1 (C)**16.968min (0.000) 183833.45 ng****response 682387**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.96
264.00	61.60	68.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011824\
Data File : BN029284.D
Acq On : 18 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 01:39:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 01:39:16 2024
Response via : Initial Calibration

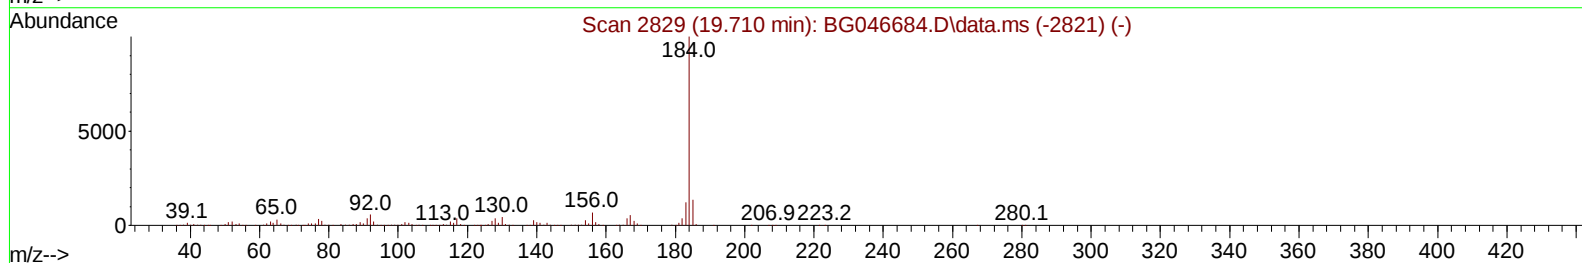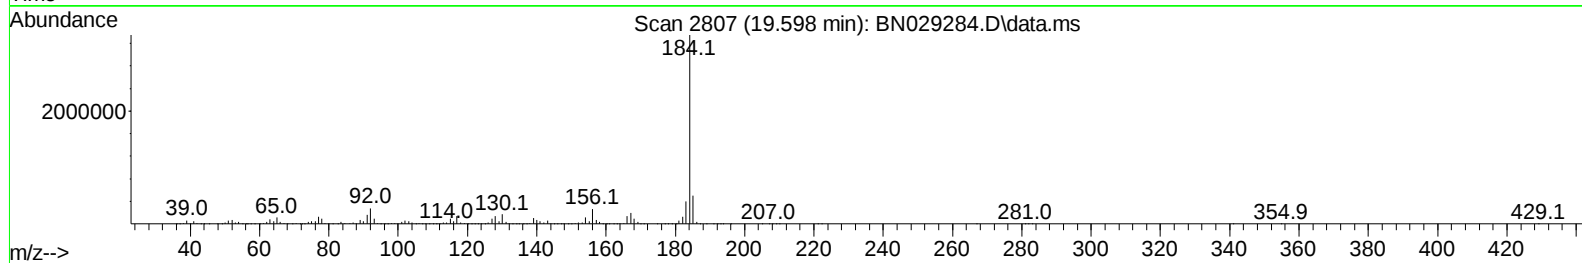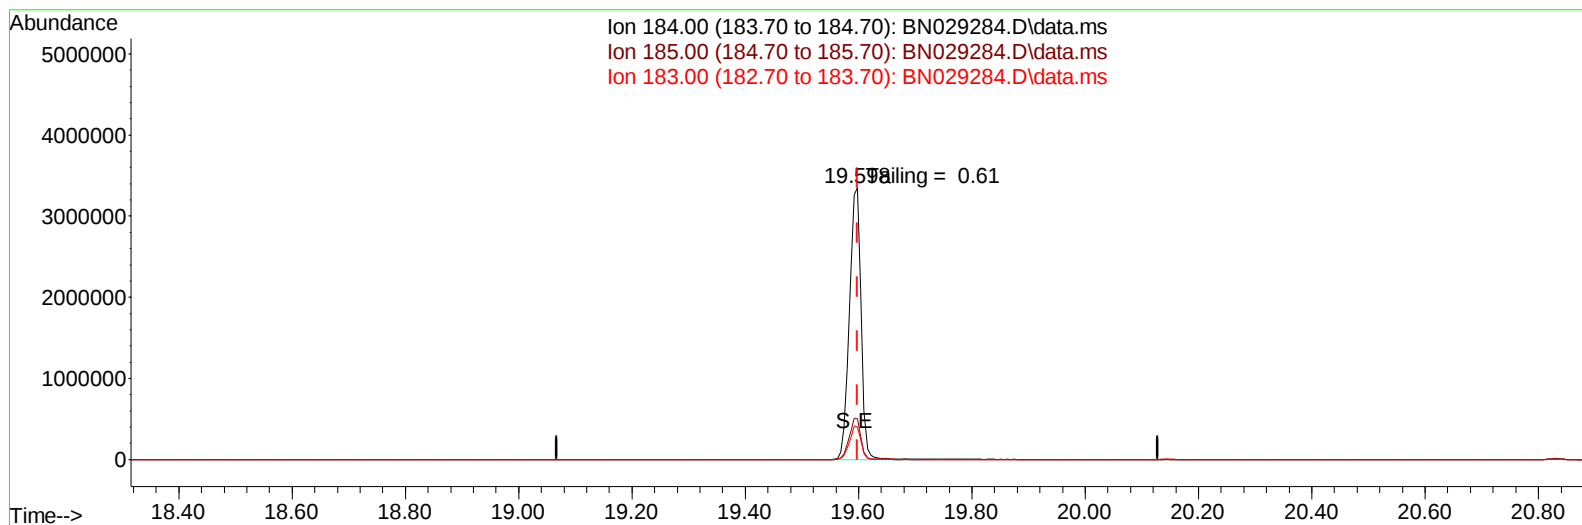

TIC: BN029284.D\data.ms

(77) Benzidine**19.598min (0.000) 21579.71 ng****response 4818728**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.09
183.00	13.20	12.00
0.00	0.00	0.00