
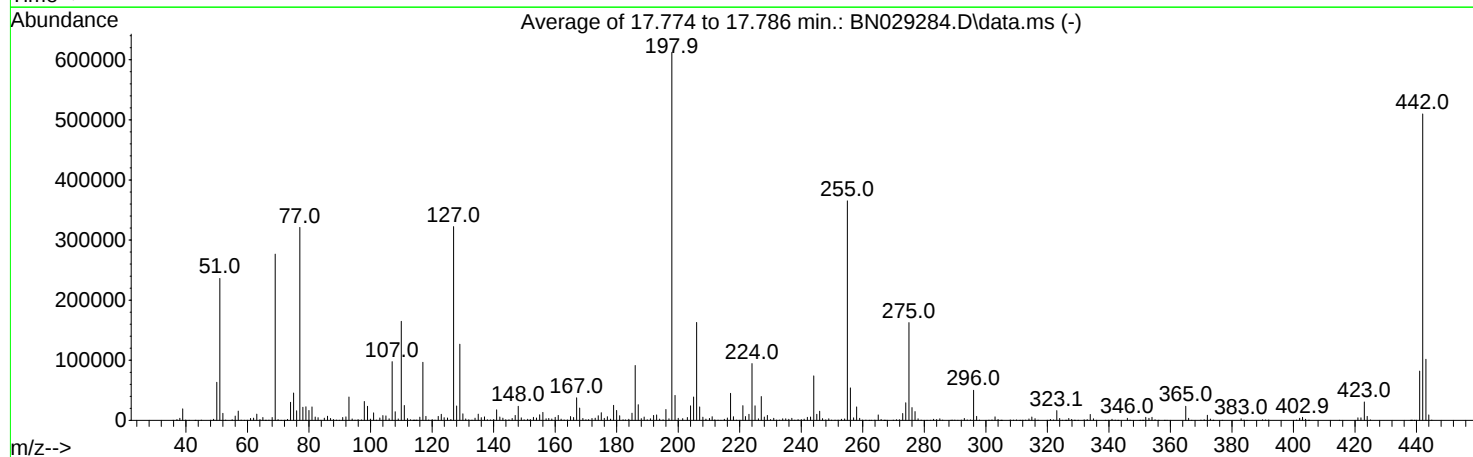


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011824\
Data File : BN029284.D
Acq On : 18 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 18 16:49:42 2024

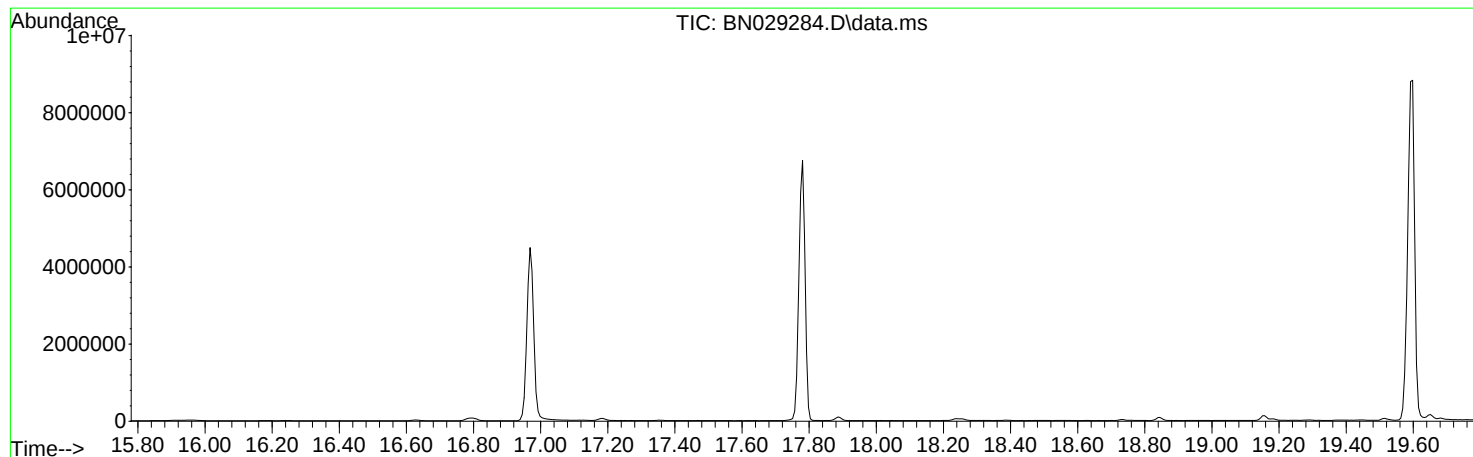




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	236160	PASS
68	69	0.00	2	1.8	4905	PASS
69	198	0.00	100	45.2	276672	PASS
70	69	0.00	2	0.5	1322	PASS
127	198	10	80	52.7	322432	PASS
197	198	0.00	2	0.4	2745	PASS
198	198	100	100	100.0	612096	PASS
199	198	5	9	6.8	41541	PASS
275	198	10	60	26.6	162624	PASS
365	198	1	100	3.8	23424	PASS
441	198	0.01	100	13.4	81936	PASS
442	442	50	100	100.0	509739	PASS
443	442	15	24	20.0	101741	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011824\
Data File : BN029284.D
Acq On : 18 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 19 01:39:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 01:39:16 2024
Response via : Initial Calibration

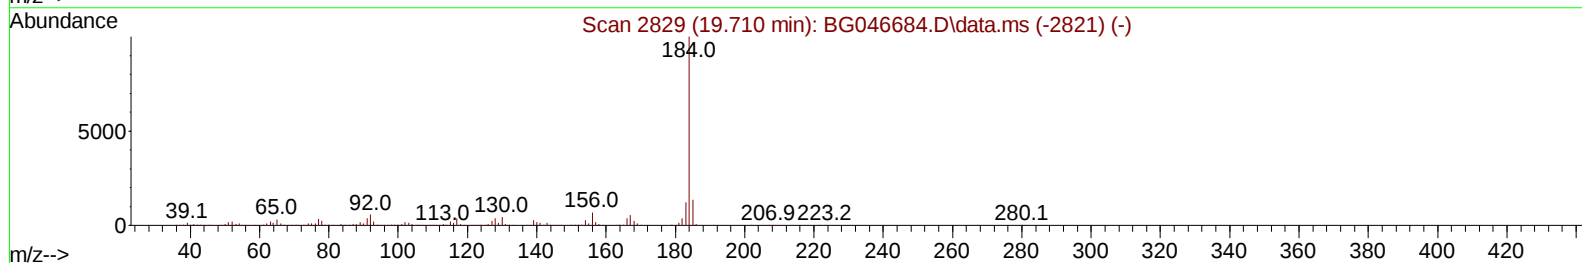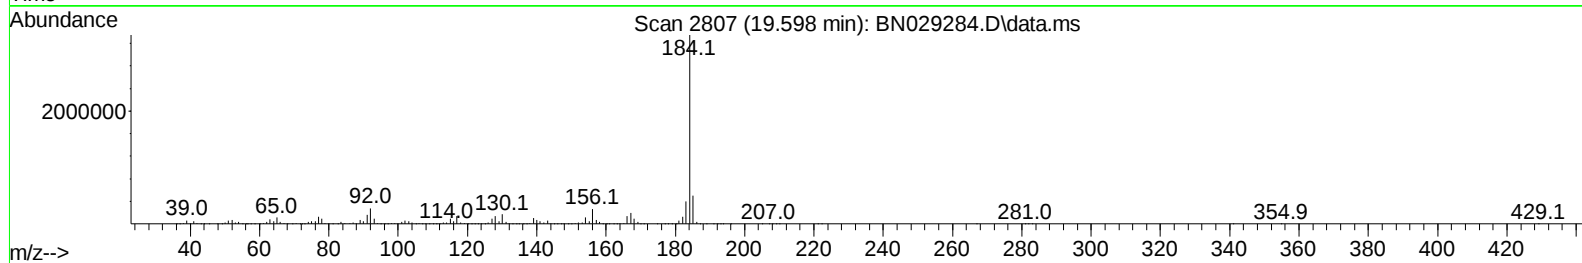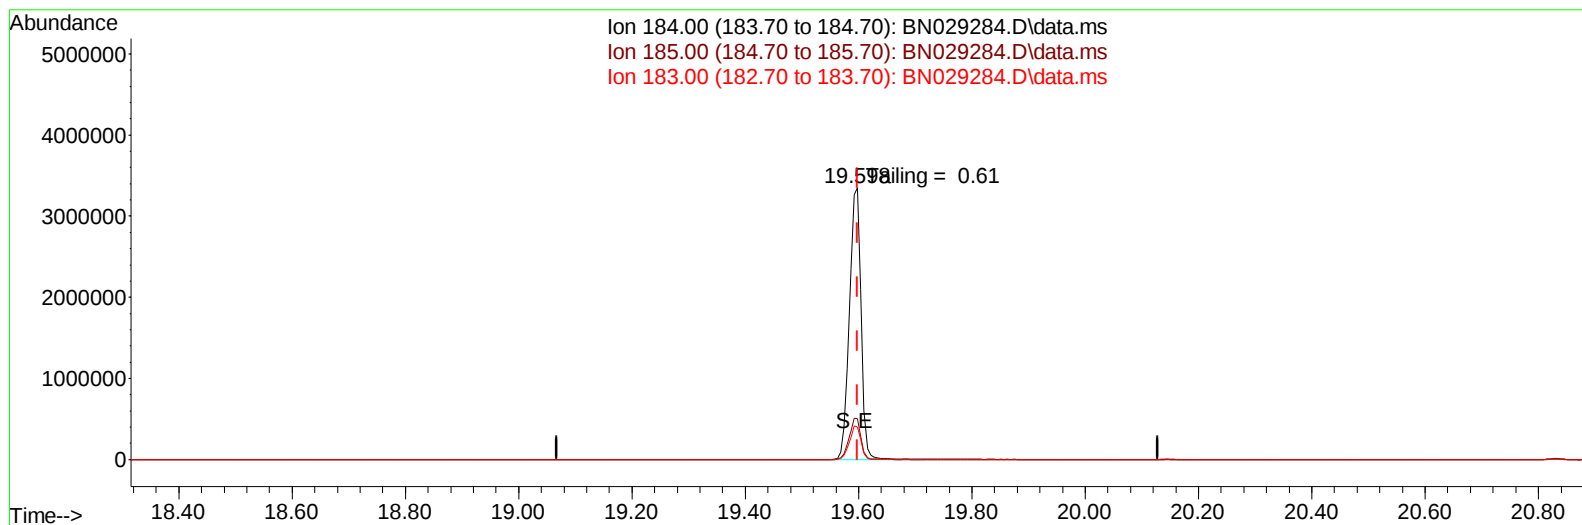

TIC: BN029284.D\data.ms

(77) Benzidine

19.598min (0.000) 21579.71 ng

response 4818728

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.09
183.00	13.20	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2024	BNA_N	<u>BN029284.D</u>
Compound Name	Response	Retention Time
DDT	2169300	20.833
DDD	39566	20.386
DDE	1500	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41066	2210366	1.86

Instrument :
BNA_N
ClientSampleId :
DFTPP