
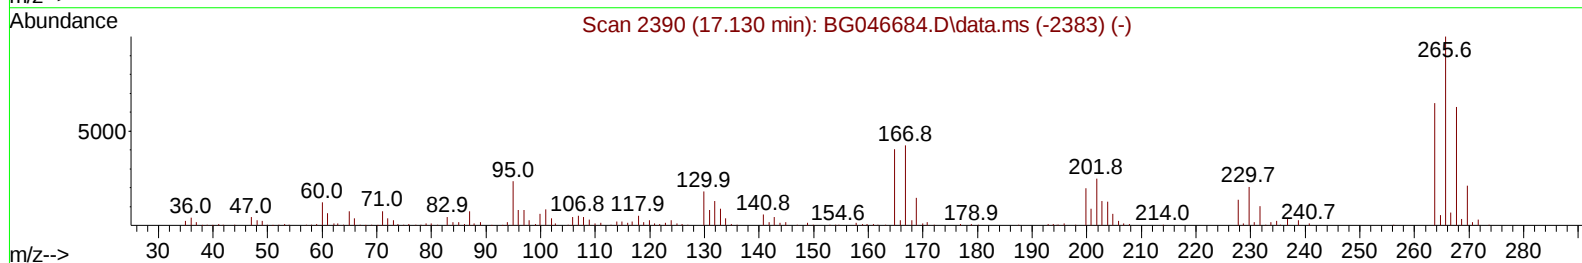
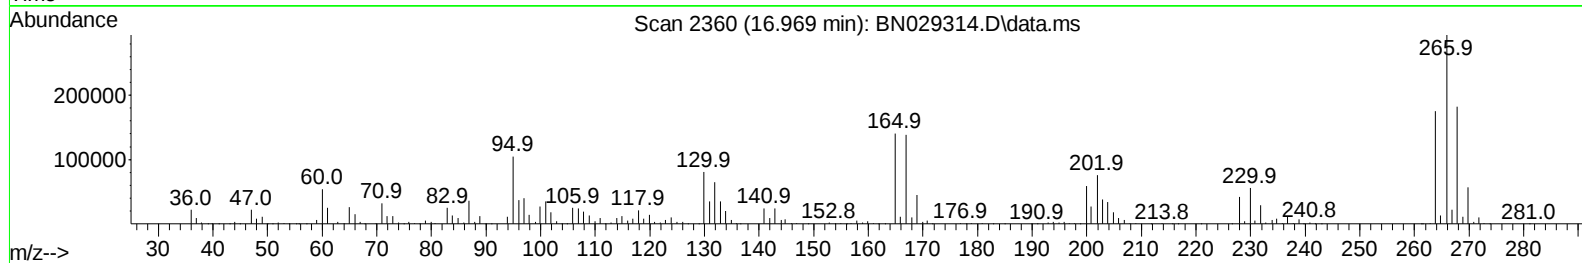


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029314.D
Acq On : 19 Jan 2024 21:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Jan 20 02:58:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 02:57:17 2024
Response via : Initial Calibration

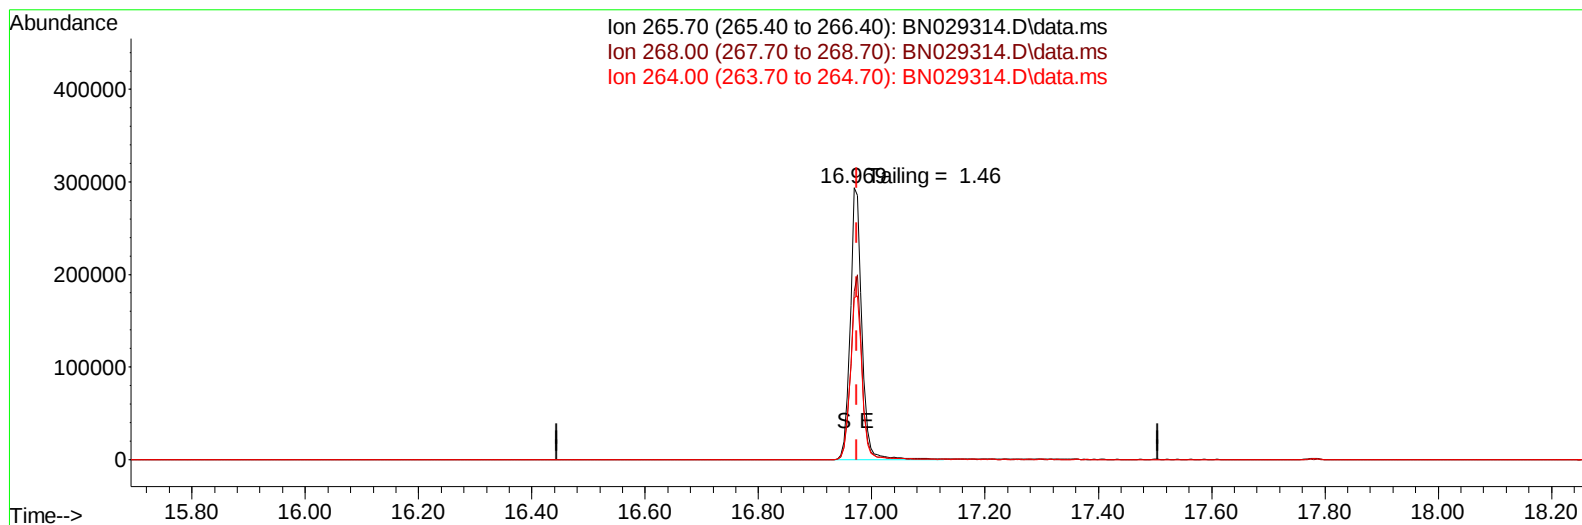




TIC: BN029314.D\data.ms

(70) Pentachlorophenol (C)**16.969min (-0.006) 17423.38 ng****response 419911**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.01
264.00	61.60	59.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029314.D
Acq On : 19 Jan 2024 21:19
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Jan 20 02:58:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 02:57:17 2024
Response via : Initial Calibration

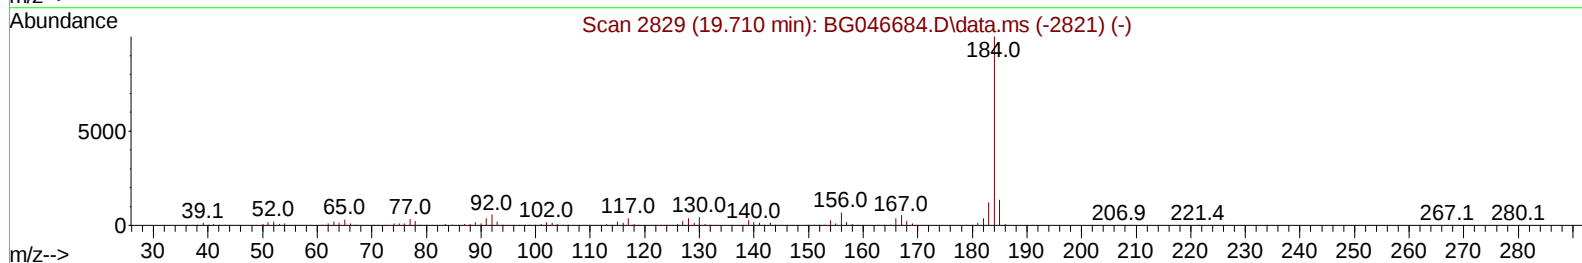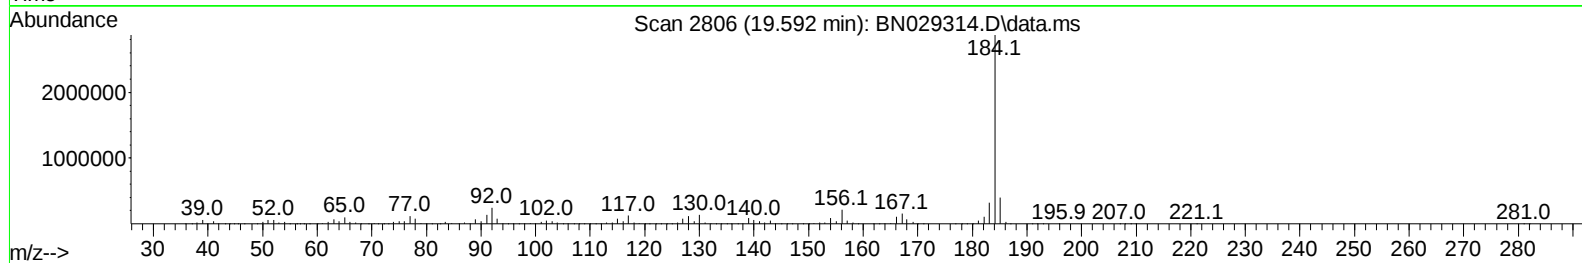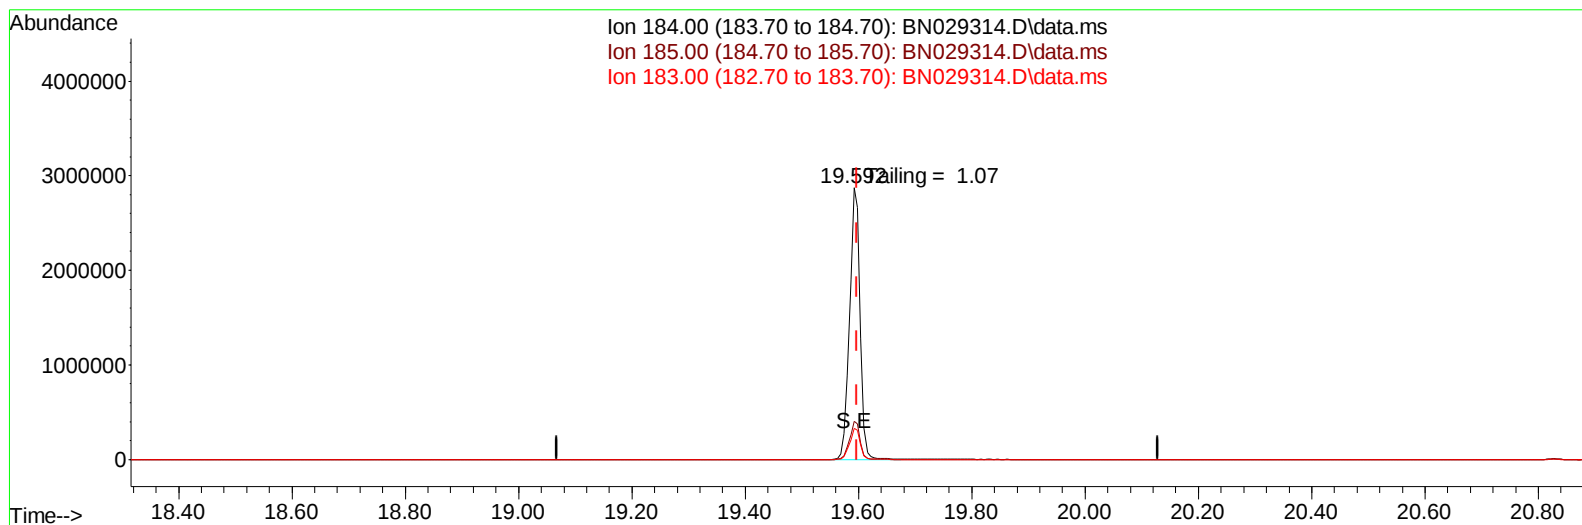

TIC: BN029314.D\data.ms

(77) Benzidine**19.592min (-0.006) 0.00 ng****response 3708933**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.36
0.00	0.00	0.00