

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
 Data File : BN029324.D
 Acq On : 20 Jan 2024 03:19
 Operator : MA/JU
 Sample : P1171-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-195-GW-320-322

Quant Time: Jan 20 03:46:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 18 16:49:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	3402	0.400	ng	0.00
7) Naphthalene-d8	10.744	136	9556	0.400	ng	0.00
13) Acenaphthene-d10	14.575	164	5421	0.400	ng	0.00
19) Phenanthrene-d10	17.330	188	13795	0.400	ng	0.00
29) Chrysene-d12	21.528	240	11945	0.400	ng	# 0.00
35) Perylene-d12	23.932	264	12078	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.507	112	1330	0.158	ng	0.00
5) Phenol-d6	7.103	99	1148	0.103	ng	0.00
8) Nitrobenzene-d5	9.099	82	2238	0.253	ng	0.00
11) 2-Methylnaphthalene-d10	12.329	152	3851	0.236	ng	0.00
14) 2,4,6-Tribromophenol	16.064	330	722	0.434	ng	0.00
15) 2-Fluorobiphenyl	13.207	172	6561	0.260	ng	0.00
27) Fluoranthene-d10	19.359	212	11763	0.281	ng	0.00
31) Terphenyl-d14	19.968	244	12364	0.413	ng	0.00
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phtha...	21.456	149	6240	0.300	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029324.D
Acq On : 20 Jan 2024 03:19
Operator : MA/JU
Sample : P1171-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-320-322


Quant Time: Jan 20 03:46:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 16:49:42 2024
Response via : Initial Calibration

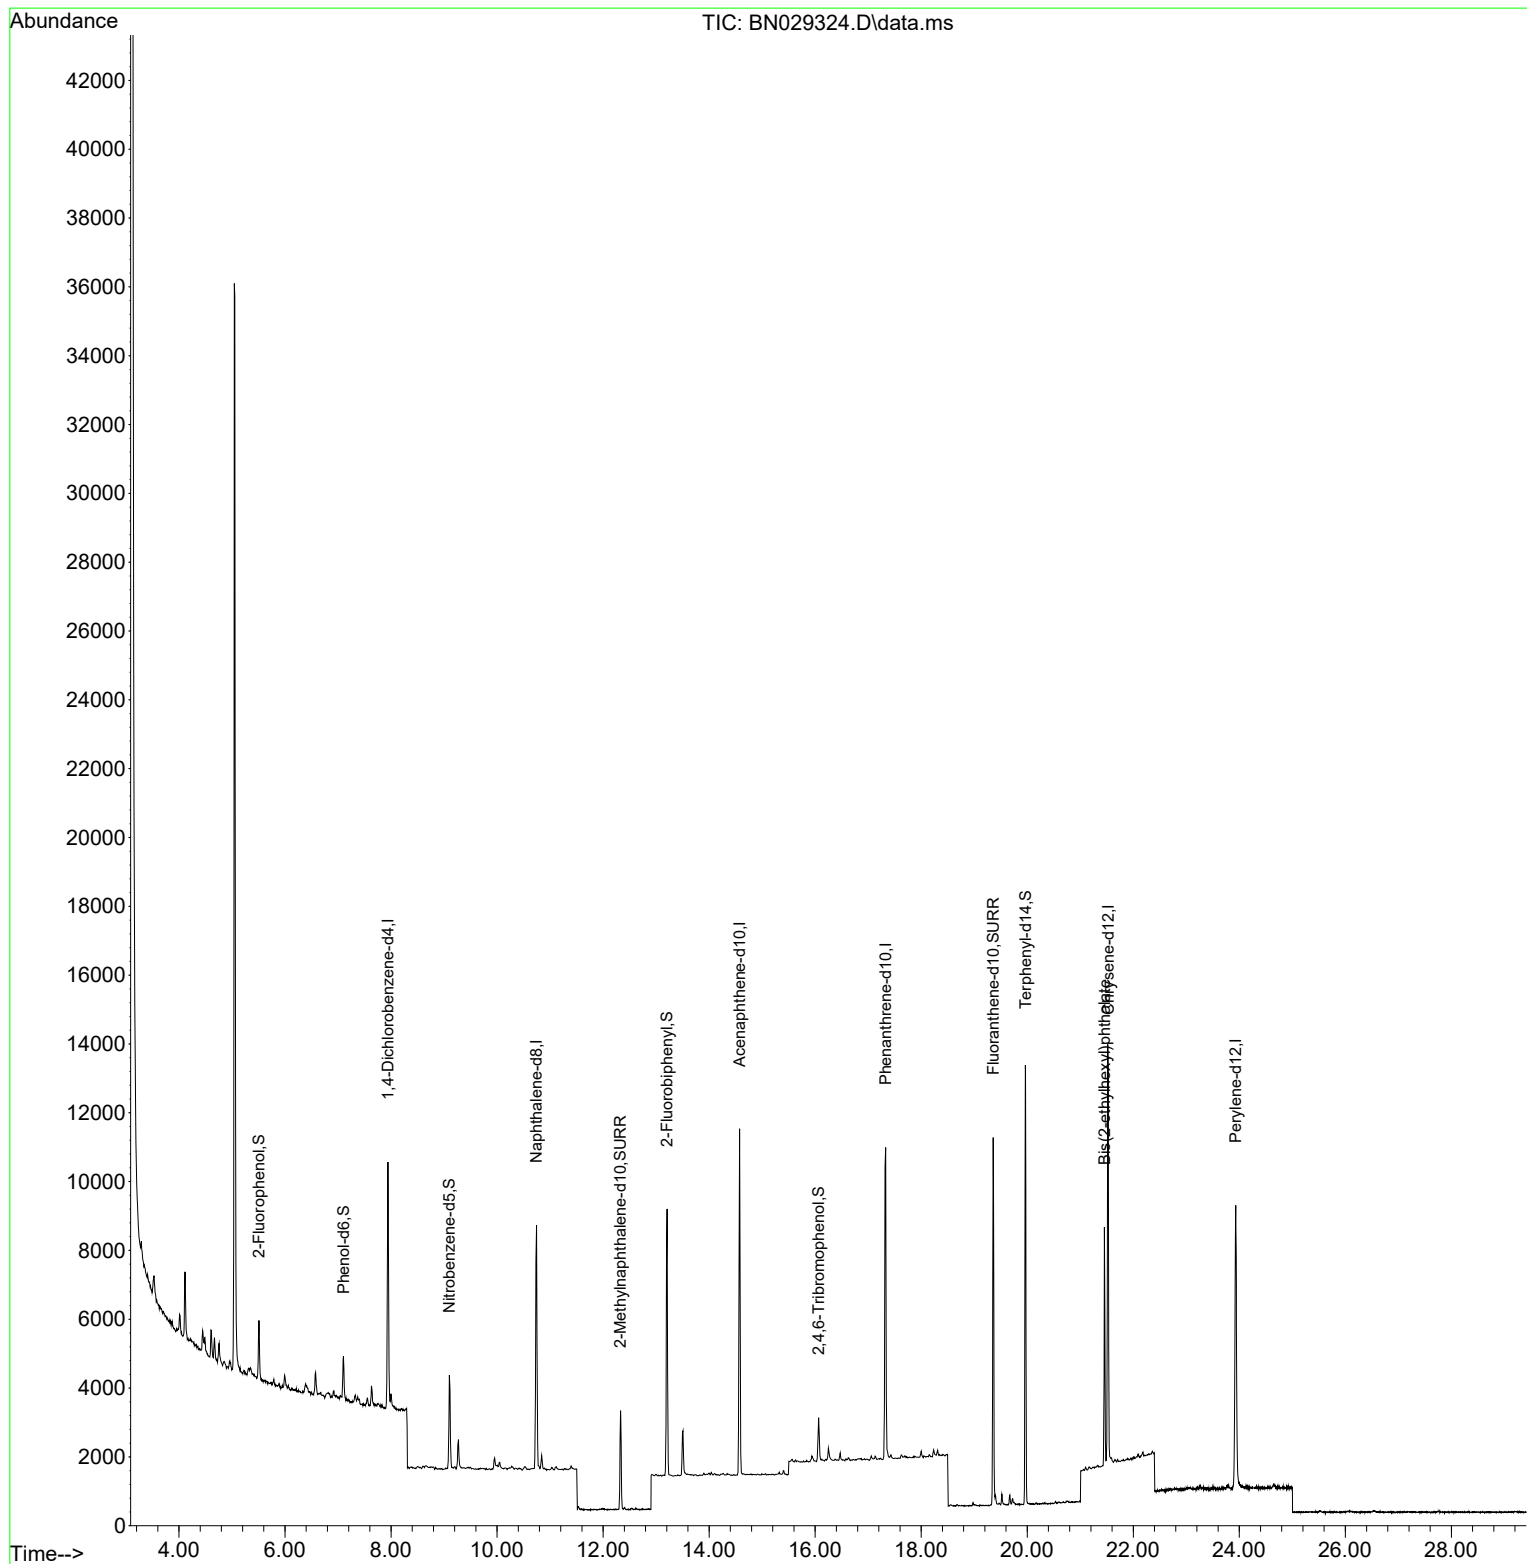

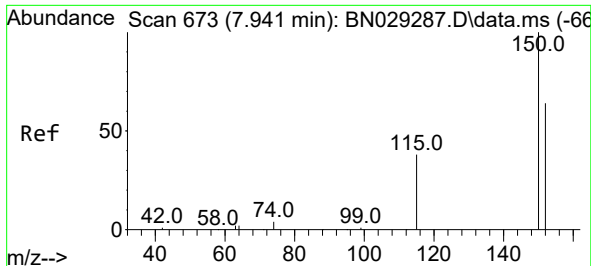




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.941 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN029324.D
 Acq: 20 Jan 2024 03:19

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-195-GW-320-322

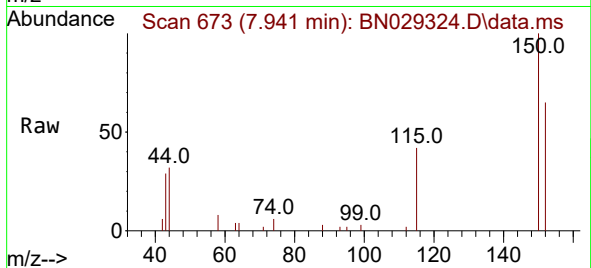

Tgt Ion:152 Resp: 3402




Ion	Ratio	Lower	Upper
152	100		
150	154.4	124.6	186.8
115	65.0	50.6	76.0

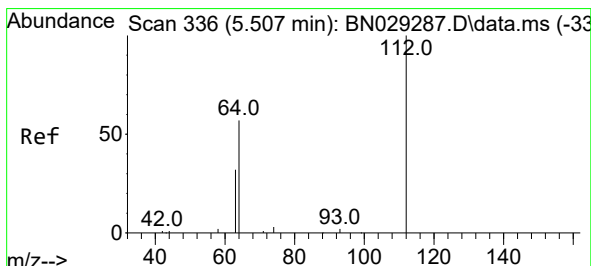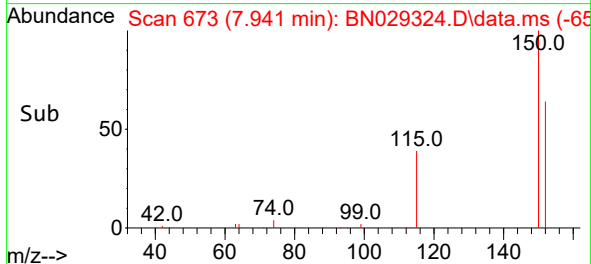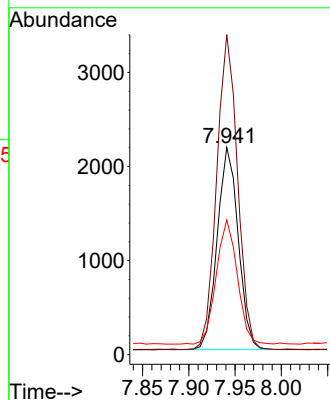


#4
 2-Fluorophenol
 Concen: 0.158 ng
 RT: 5.507 min Scan# 336
 Delta R.T. -0.000 min
 Lab File: BN029324.D
 Acq: 20 Jan 2024 03:19

Tgt Ion:112 Resp: 1330

Ion	Ratio	Lower	Upper
112	100		
64	57.0	45.7	68.5
63	33.0	26.6	39.8


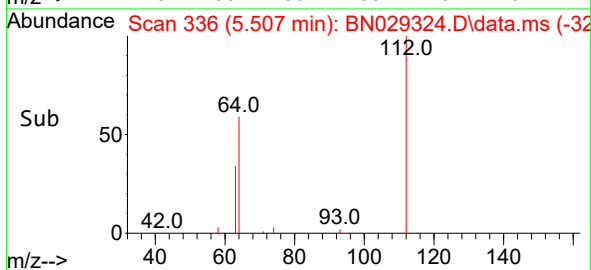
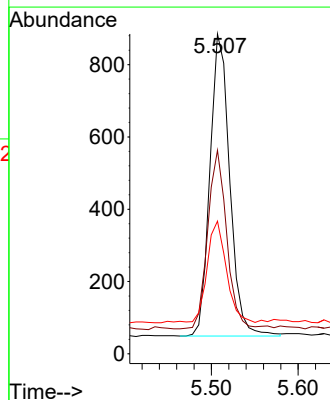
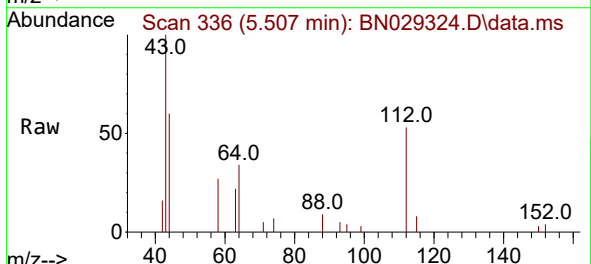


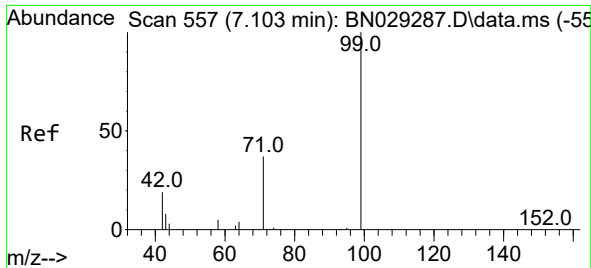

#5
Phenol-d6
Concen: 0.103 ng
RT: 7.103 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-320-322


Tgt Ion: 99 Resp: 1148
Ion Ratio Lower Upper
99 100
42 24.2 19.1 28.7
71 45.2 31.2 46.8

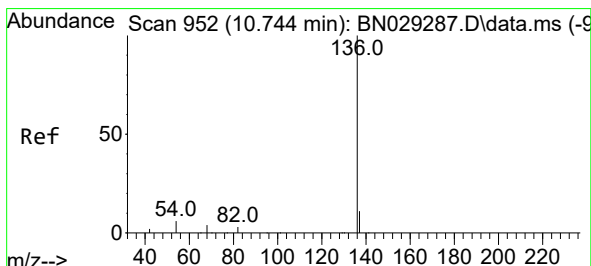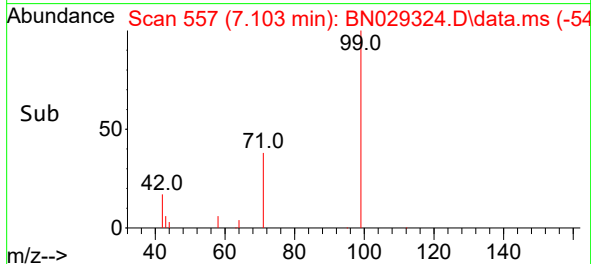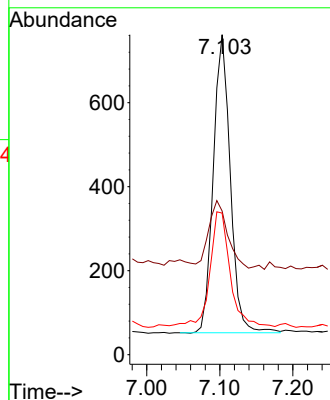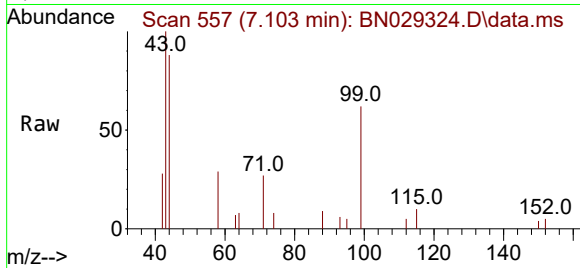

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.744 min Scan# 952
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19

Tgt Ion: 136 Resp: 9556
Ion Ratio Lower Upper
136 100
137 12.0 8.9 13.3
54 7.3 5.2 7.8
68 5.8 4.1 6.1


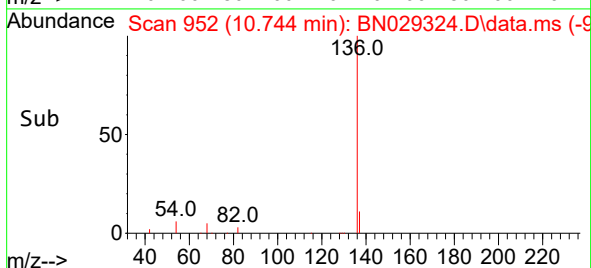
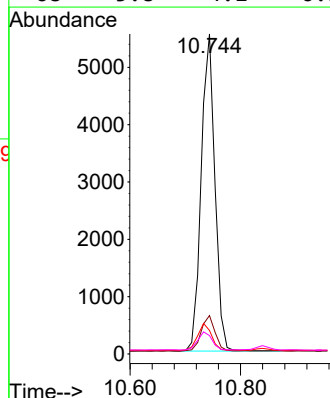
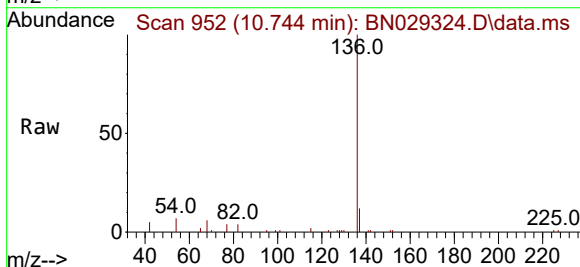


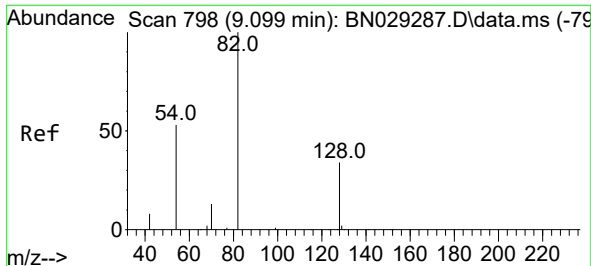

#8
Nitrobenzene-d5
Concen: 0.253 ng
RT: 9.099 min Scan# 798
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-320-322


Tgt Ion: 82 Resp: 2238
Ion Ratio Lower Upper
82 100
128 35.5 28.6 43.0
54 56.5 42.9 64.3

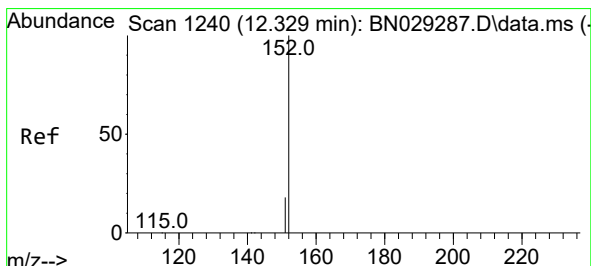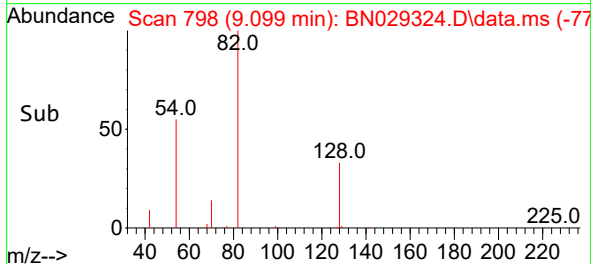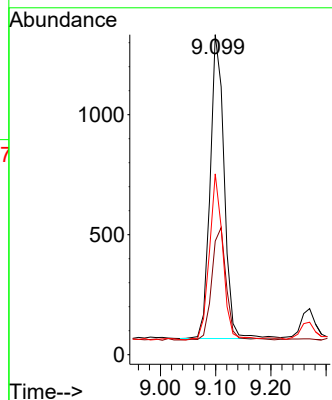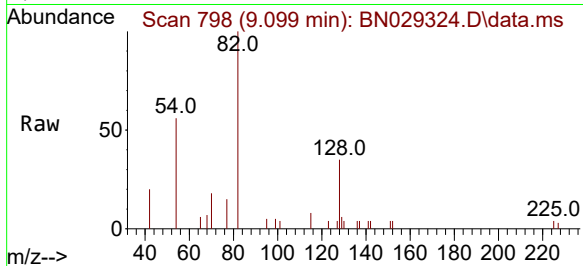

#11
2-Methylnaphthalene-d10
Concen: 0.236 ng
RT: 12.329 min Scan# 1240
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19

Tgt Ion: 152 Resp: 3851
Ion Ratio Lower Upper
152 100
151 21.8 16.6 24.8


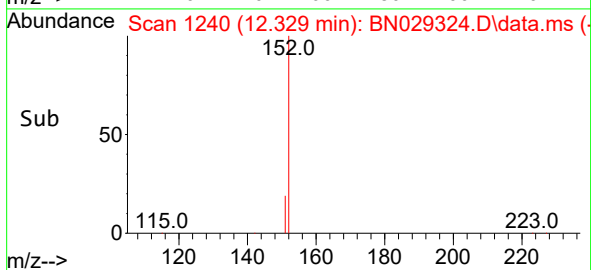
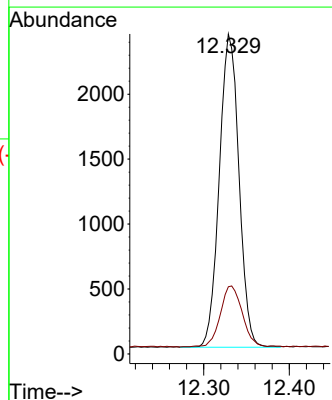
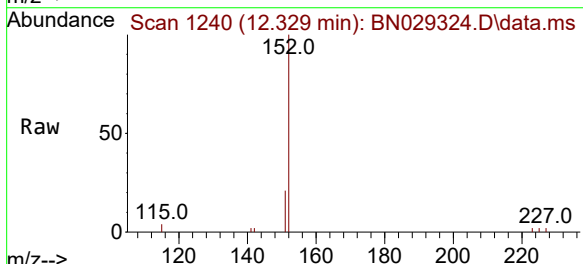


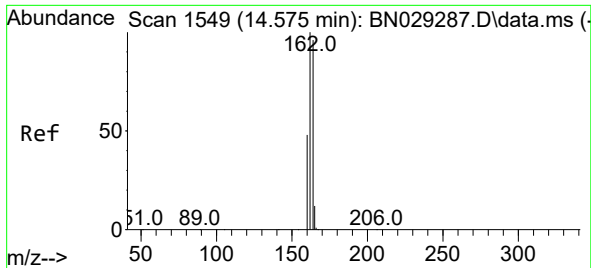

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.575 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-320-322


Tgt Ion:164 Resp: 5421
Ion Ratio Lower Upper
164 100
162 104.2 83.4 125.2
160 53.0 40.6 61.0

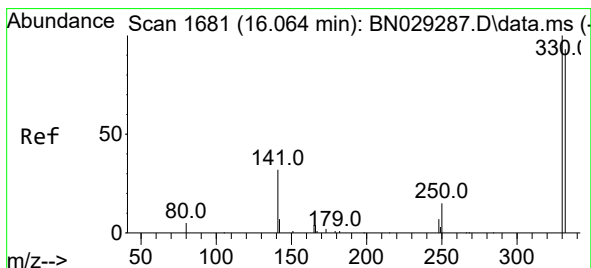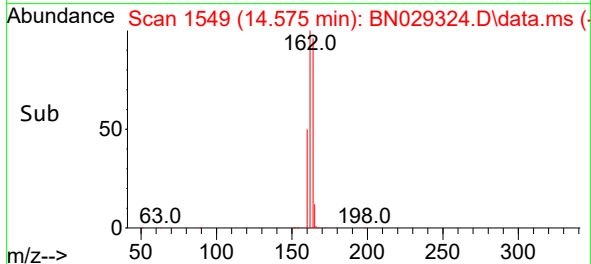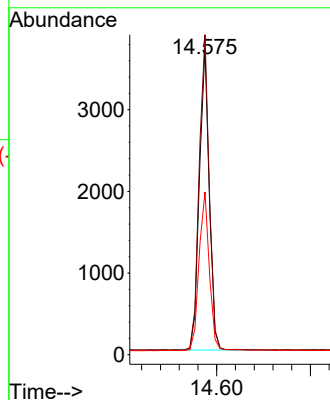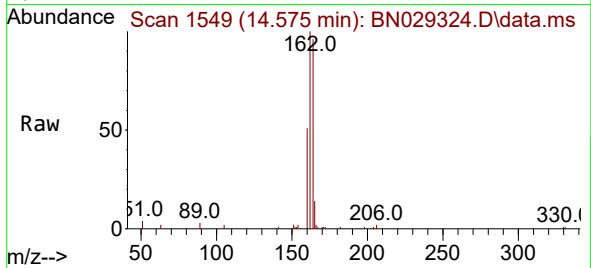

#14
2,4,6-Tribromophenol
Concen: 0.434 ng
RT: 16.064 min Scan# 1681
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19

Tgt Ion:330 Resp: 722
Ion Ratio Lower Upper
330 100
332 95.2 77.0 115.6
141 43.8 34.3 51.5


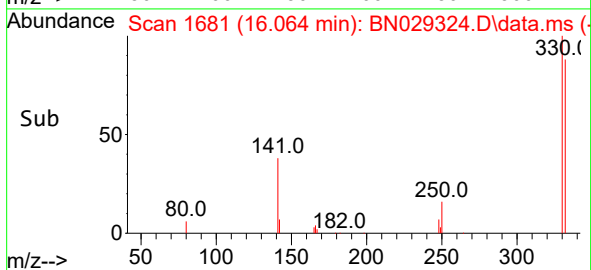
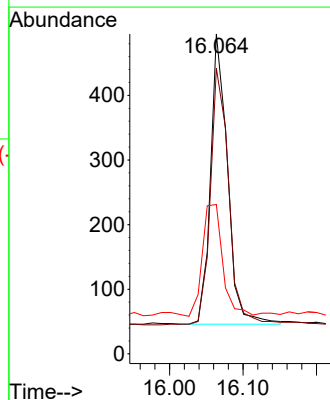
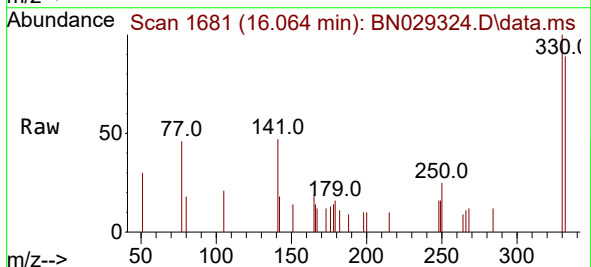


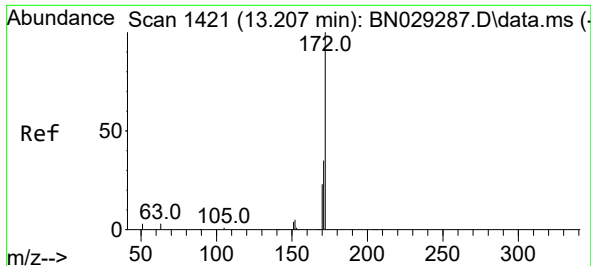

#15
2-Fluorobiphenyl
Concen: 0.260 ng
RT: 13.207 min Scan# 1421
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-320-322


Tgt Ion:172 Resp: 6561
Ion Ratio Lower Upper
172 100
171 35.3 28.0 42.0
170 23.8 18.7 28.1

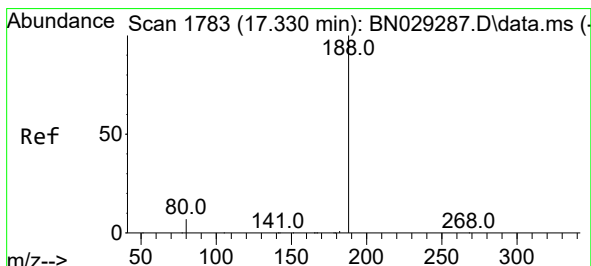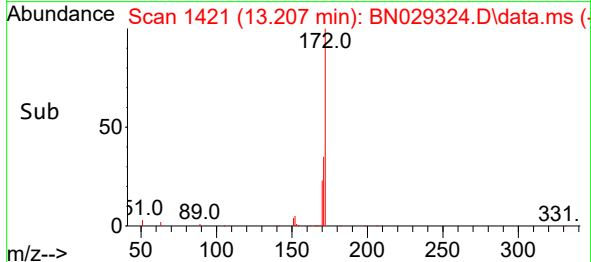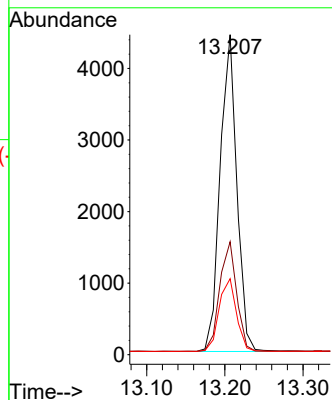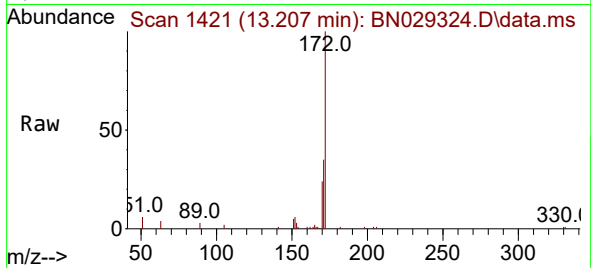

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.330 min Scan# 1783
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19

Tgt Ion:188 Resp: 13795
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.7 5.7 8.5


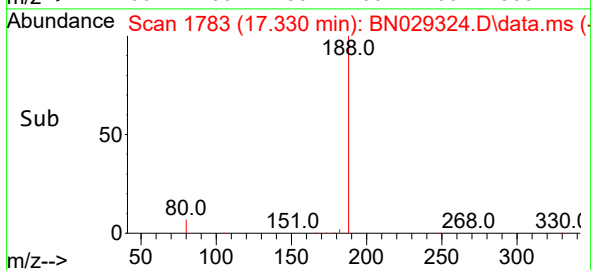
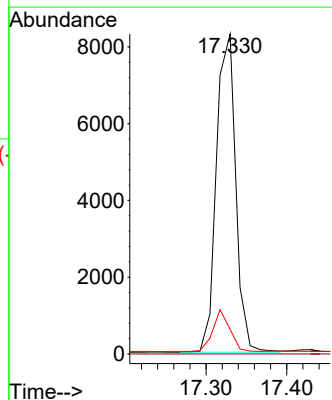
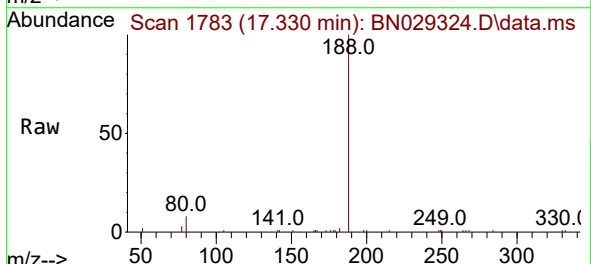


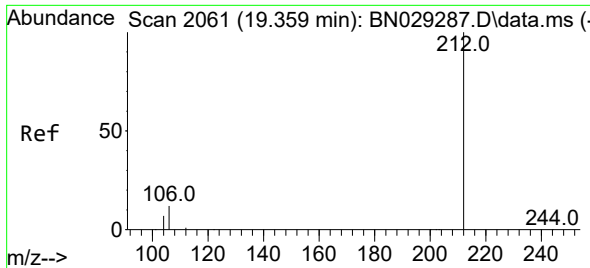

#27
Fluoranthene-d10
Concen: 0.281 ng
RT: 19.359 min Scan# 2061
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-320-322


Tgt Ion:212 Resp: 11763
Ion Ratio Lower Upper
212 100
106 13.1 9.9 14.9
104 7.9 5.8 8.8

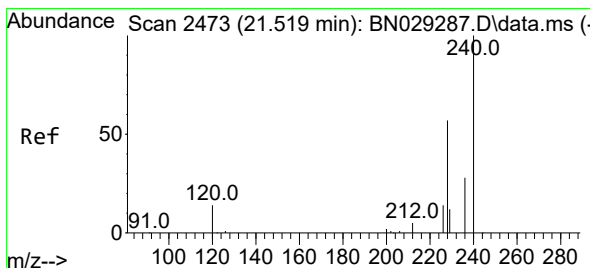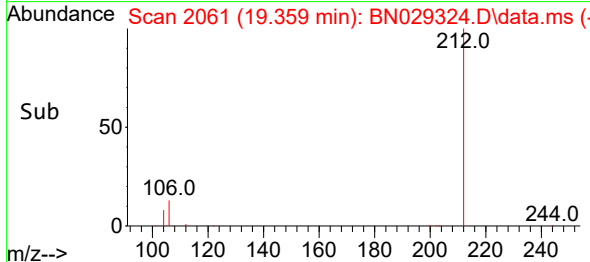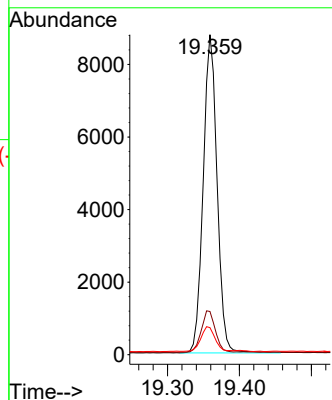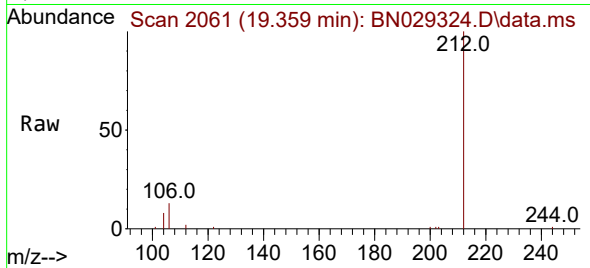

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.528 min Scan# 2474
Delta R.T. 0.009 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19

Tgt Ion:240 Resp: 11945
Ion Ratio Lower Upper
240 100
120 7.7 11.8 17.8#
236 27.8 22.7 34.1


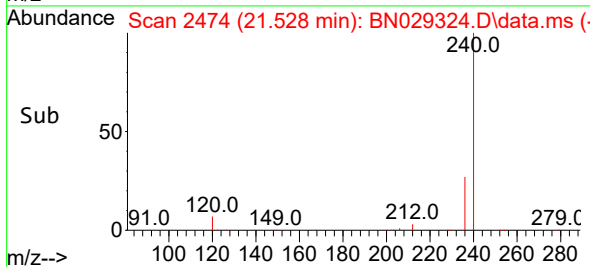
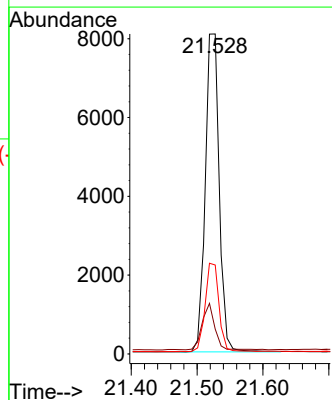
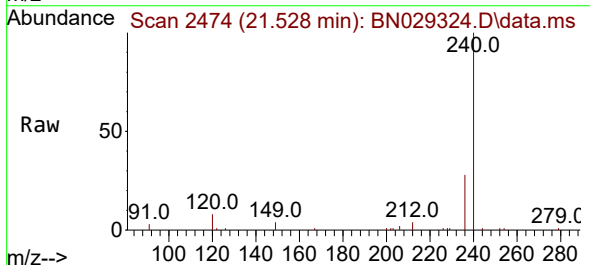


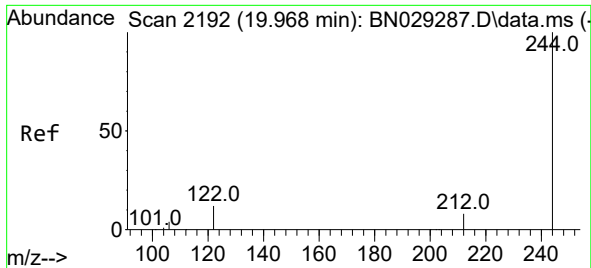

#31
 Terphenyl-d14
 Concen: 0.413 ng
 RT: 19.968 min Scan# 2192
 Delta R.T. -0.000 min
 Lab File: BN029324.D
 Acq: 20 Jan 2024 03:19




Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-195-GW-320-322


Tgt Ion:244 Resp: 12364
 Ion Ratio Lower Upper
 244 100
 212 9.2 7.0 10.4
 122 13.4 10.2 15.4

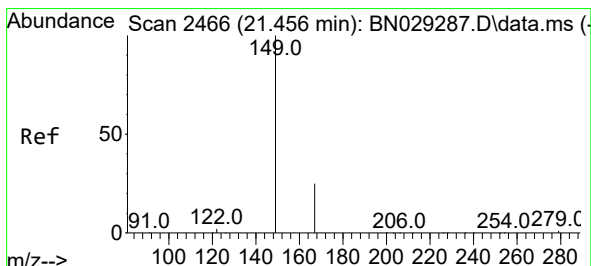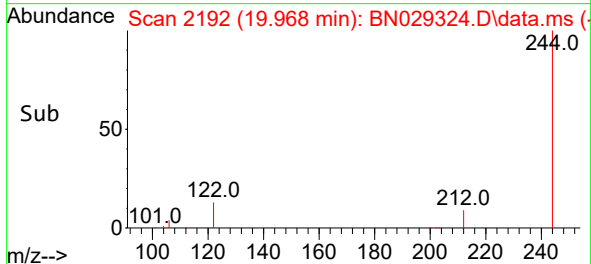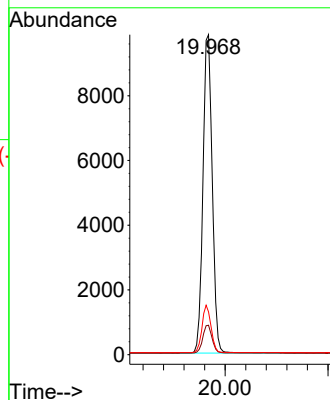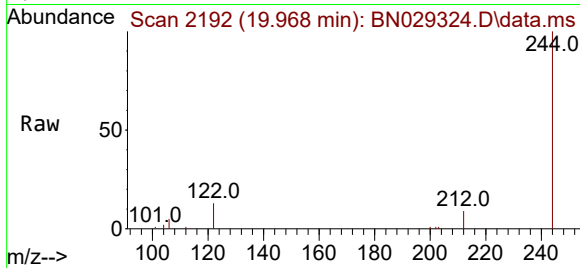

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.300 ng
 RT: 21.456 min Scan# 2466
 Delta R.T. -0.000 min
 Lab File: BN029324.D
 Acq: 20 Jan 2024 03:19


Tgt Ion:149 Resp: 6240
 Ion Ratio Lower Upper
 149 100
 167 25.3 20.3 30.5
 279 2.8 2.6 4.0

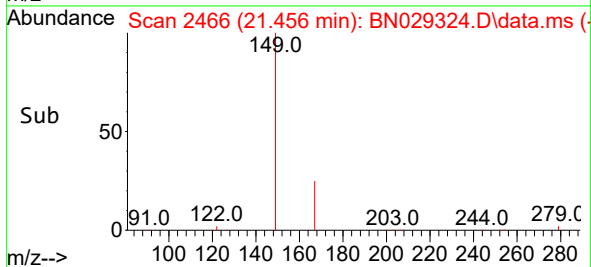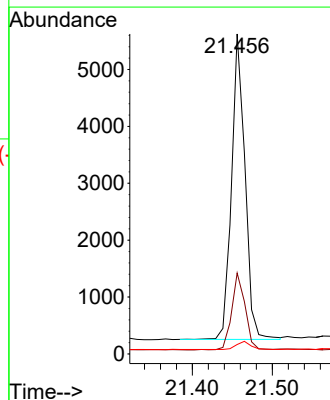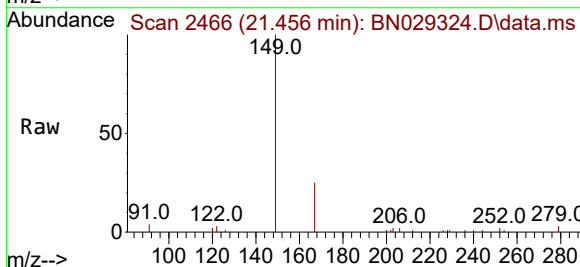

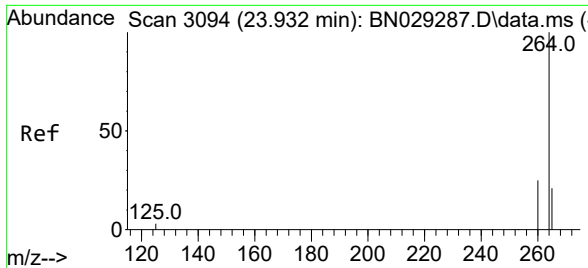

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.932 min Scan# 3094
Delta R.T. -0.000 min
Lab File: BN029324.D
Acq: 20 Jan 2024 03:19

Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-320-322

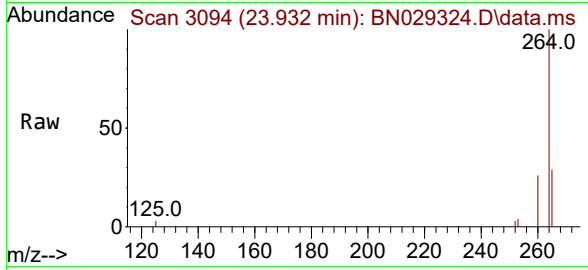

Tgt Ion:264 Resp: 12078

Ion	Ratio	Lower	Upper
264	100		
260	25.8	20.7	31.1
265	29.3	21.4	32.0

