
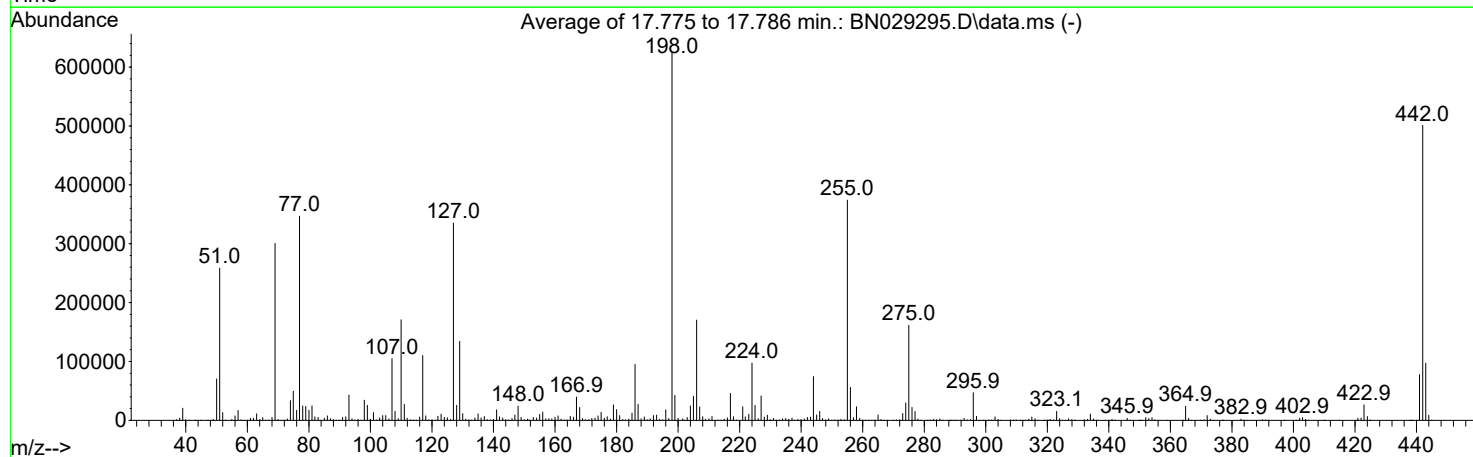


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029295.D
Acq On : 19 Jan 2024 08:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 18 16:49:42 2024

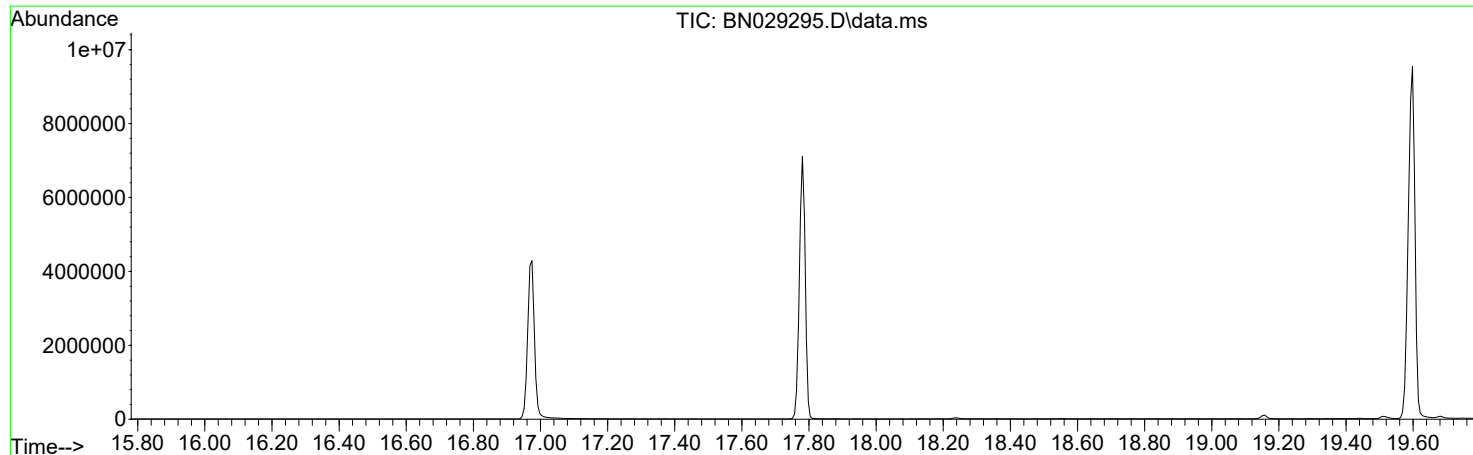

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	258645	PASS
68	69	0.00	2	1.7	5153	PASS
69	198	0.00	100	48.1	300587	PASS
70	69	0.00	2	0.5	1582	PASS
127	198	10	80	53.6	335189	PASS
197	198	0.00	2	0.5	3239	PASS
198	198	100	100	100.0	624811	PASS
199	198	5	9	6.8	42283	PASS
275	198	10	60	25.8	161472	PASS
365	198	1	100	3.8	23981	PASS
441	198	0.01	100	12.4	77699	PASS
442	442	50	100	100.0	501141	PASS
443	442	15	24	19.4	96992	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/19/2024	BNA_N	<u>BN029295.D</u>
Compound Name	Response	Retention Time
DDT	2255583	20.833
DDD	31466	20.386
DDE	969	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32435	2288018	1.42

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029295.D
Acq On : 19 Jan 2024 08:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 20 02:57:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 02:57:17 2024
Response via : Initial Calibration

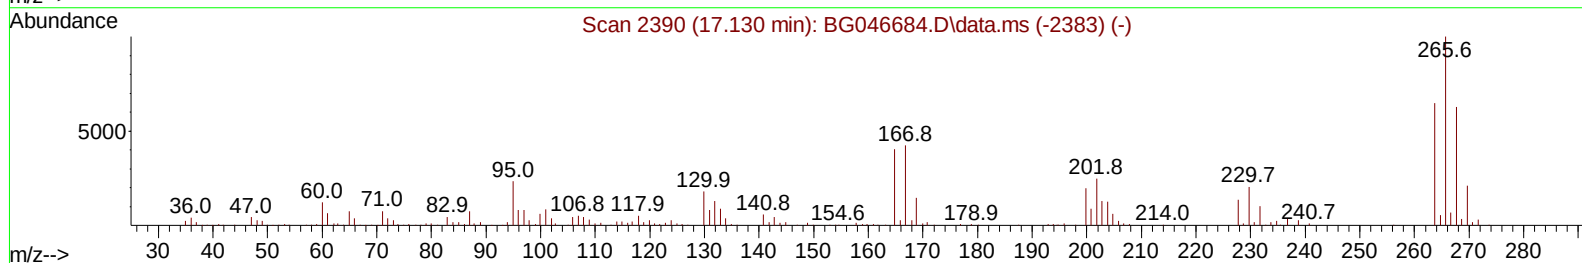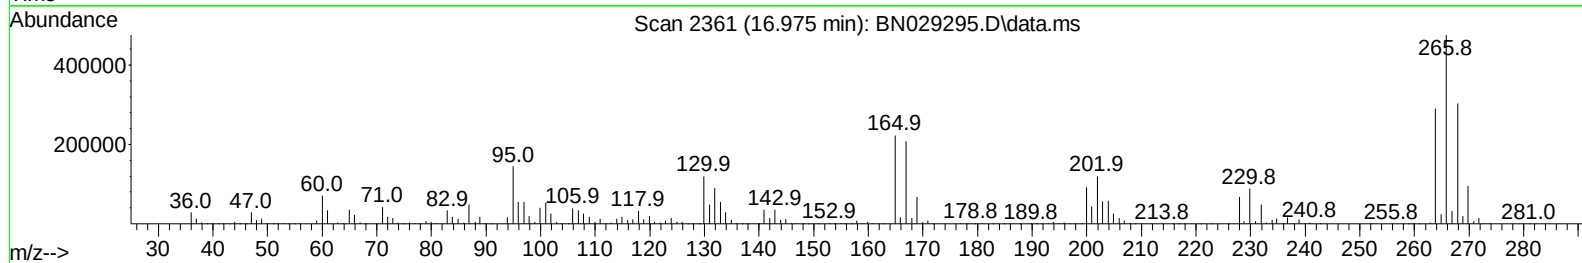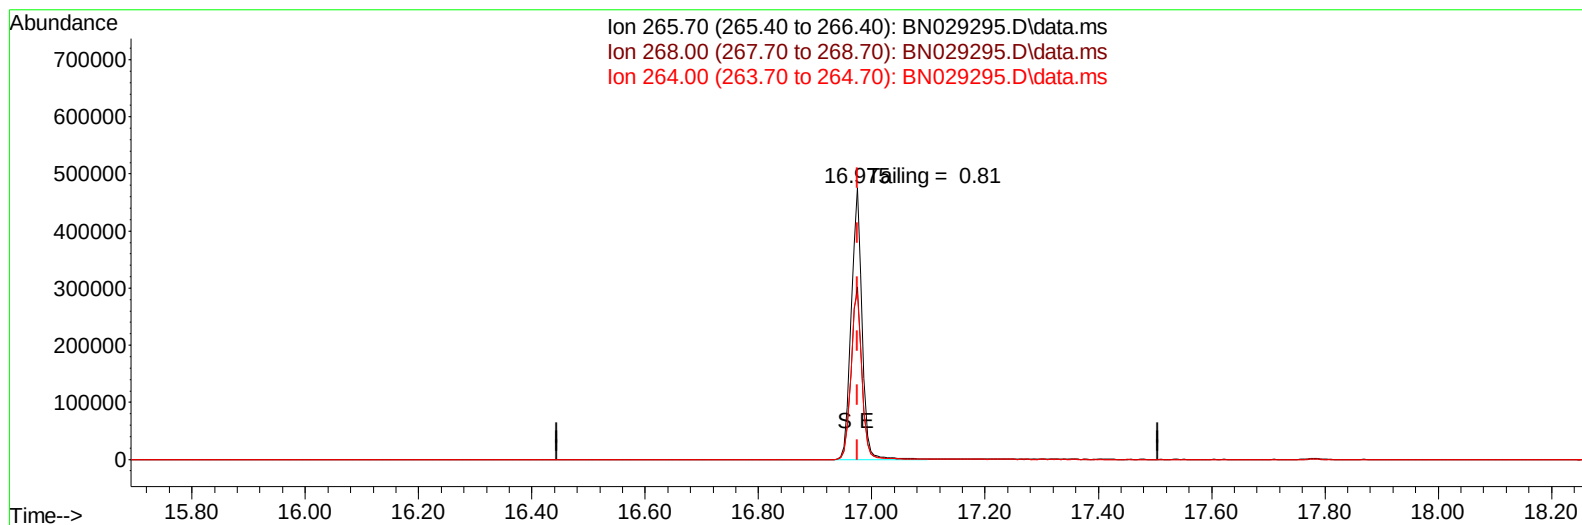

TIC: BN029295.D\data.ms

(70) Pentachlorophenol (C)

16.975min (0.000) 184156.68 ng




response 624333

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.62
264.00	61.60	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029295.D
Acq On : 19 Jan 2024 08:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 20 02:57:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 02:57:17 2024
Response via : Initial Calibration

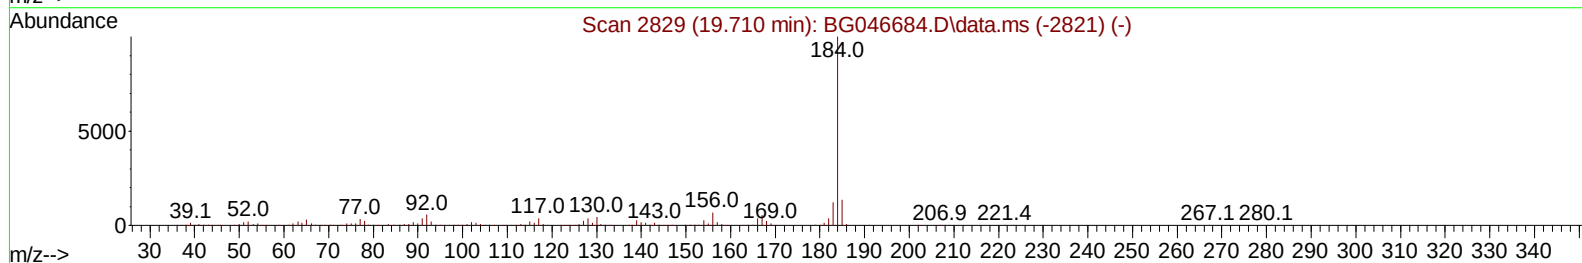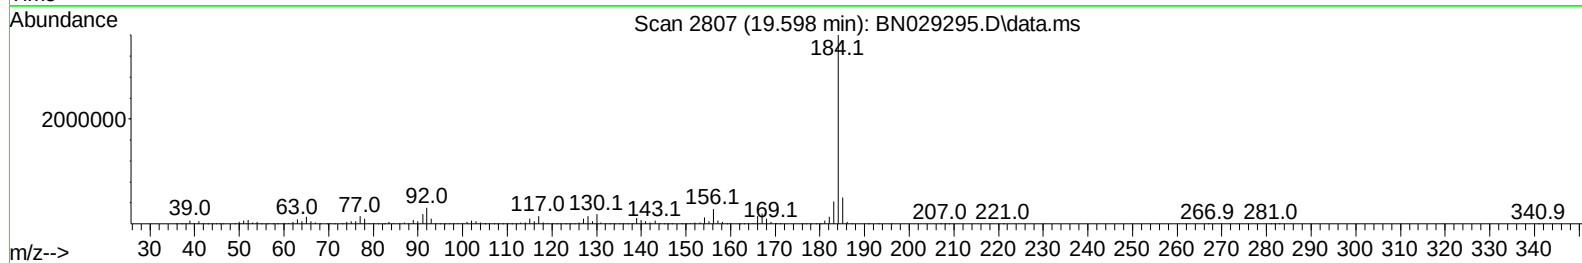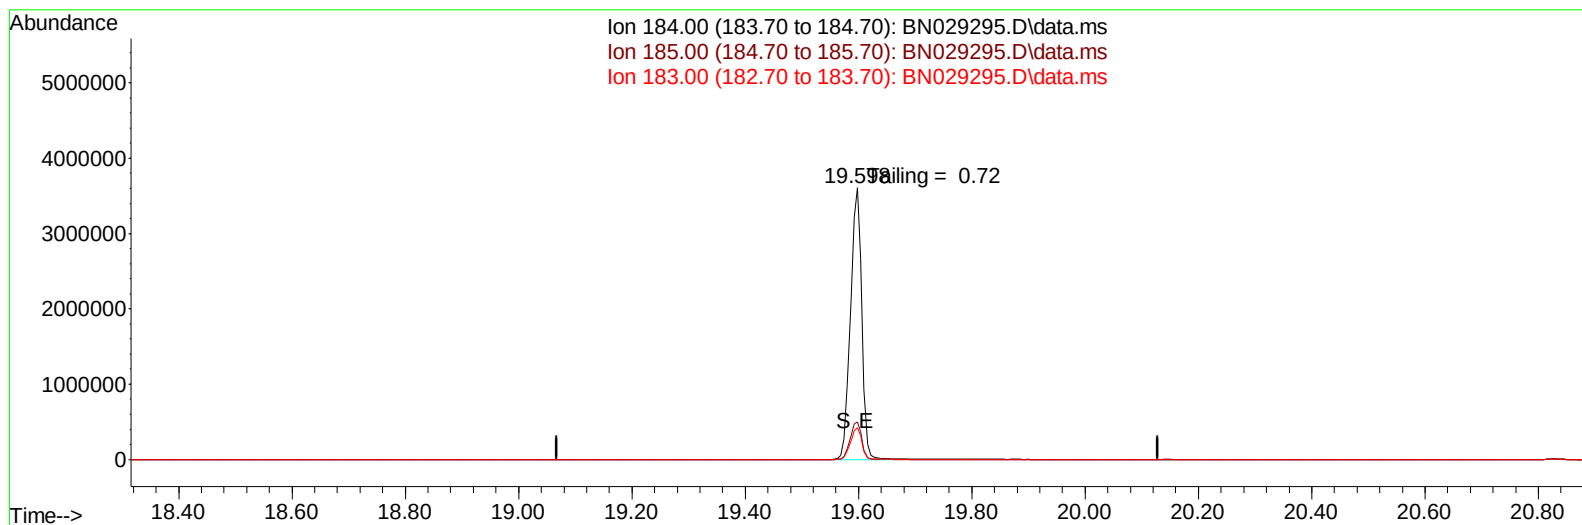

TIC: BN029295.D\data.ms

(77) Benzidine

19.598min (-19.598) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.50	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00