
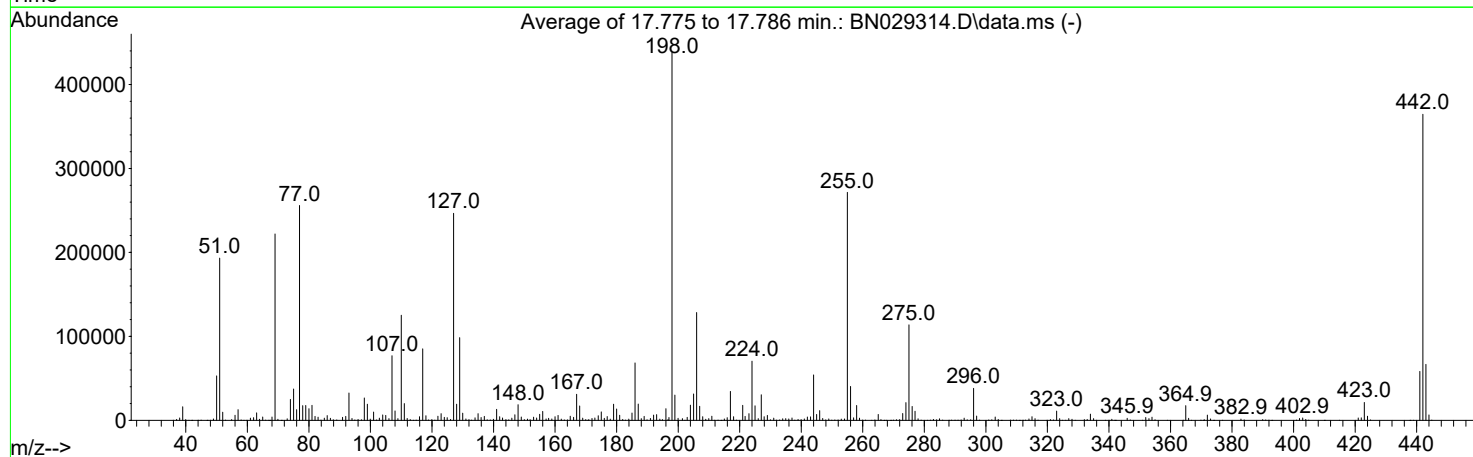


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029314.D
Acq On : 19 Jan 2024 21:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 18 16:49:42 2024

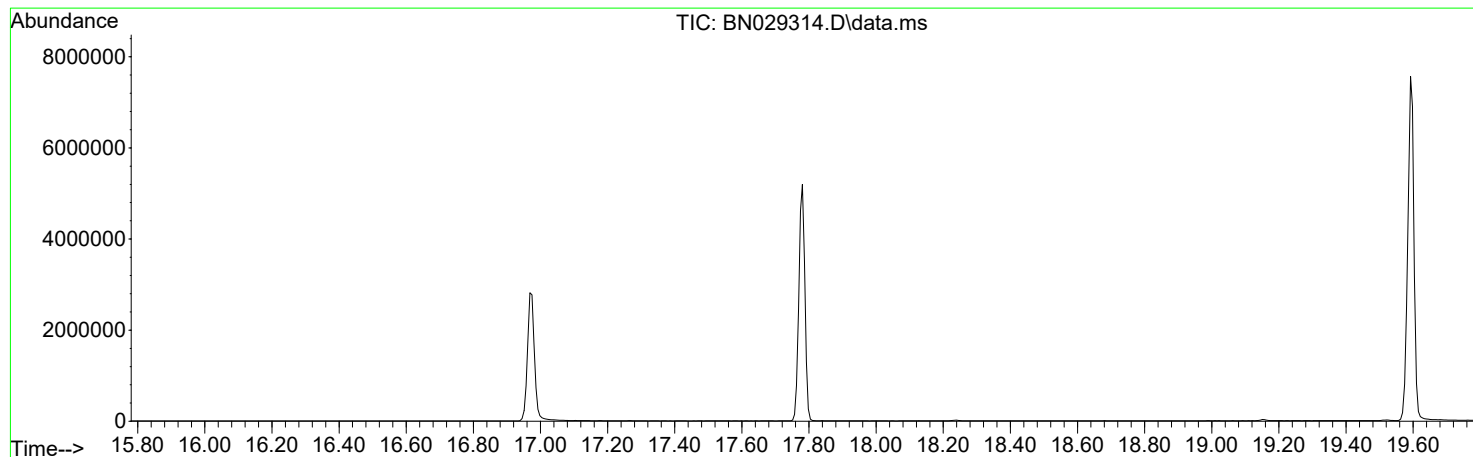

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	44.1	193293	PASS
68	69	0.00	2	1.8	3986	PASS
69	198	0.00	100	50.7	222016	PASS
70	69	0.00	2	0.6	1293	PASS
127	198	10	80	56.3	246635	PASS
197	198	0.00	2	0.8	3406	PASS
198	198	100	100	100.0	438080	PASS
199	198	5	9	6.9	30203	PASS
275	198	10	60	26.0	113864	PASS
365	198	1	100	4.0	17528	PASS
441	198	0.01	100	13.3	58259	PASS
442	442	50	100	100.0	364480	PASS
443	442	15	24	18.3	66648	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/19/2024	BNA_N	<u>BN029314.D</u>
Compound Name	Response	Retention Time
DDT	1657245	20.827
DDD	23251	20.38
DDE	1231	19.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24482	1681727	1.46

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029314.D
Acq On : 19 Jan 2024 21:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 20 02:58:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 02:57:17 2024
Response via : Initial Calibration

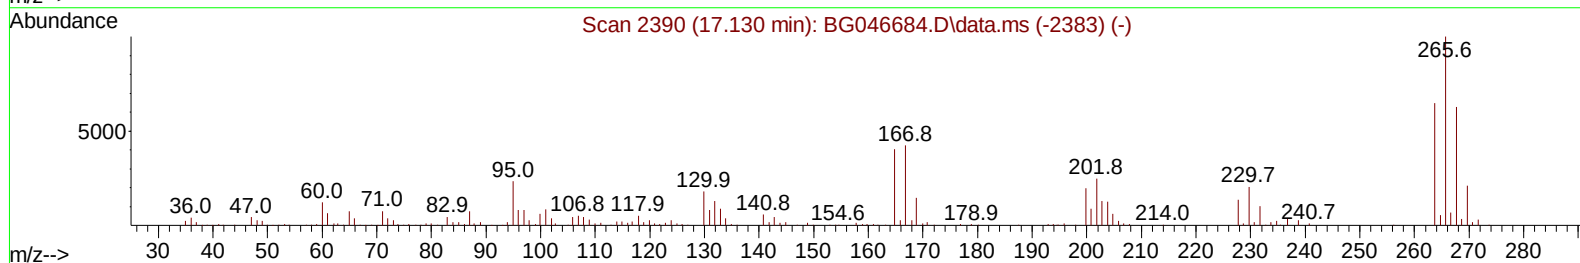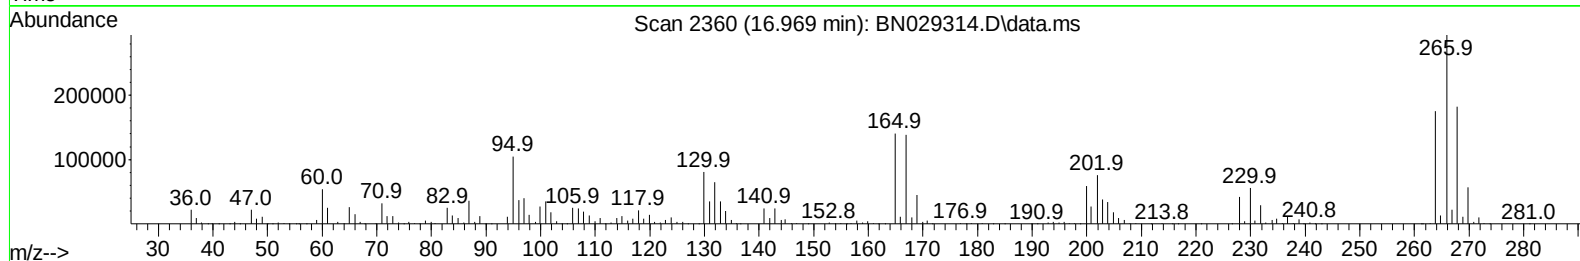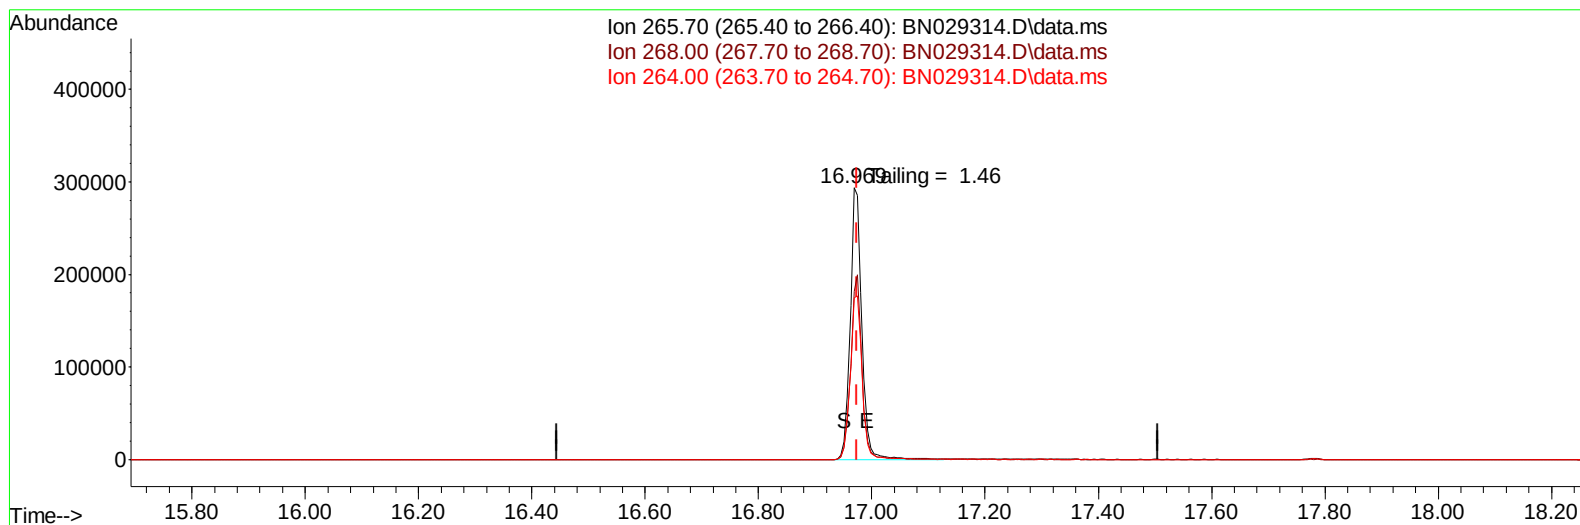

TIC: BN029314.D\data.ms

(70) Pentachlorophenol (C)

16.969min (-0.006) 17423.38 ng




response 419911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.01
264.00	61.60	59.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011924\
Data File : BN029314.D
Acq On : 19 Jan 2024 21:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 20 02:58:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 20 02:57:17 2024
Response via : Initial Calibration

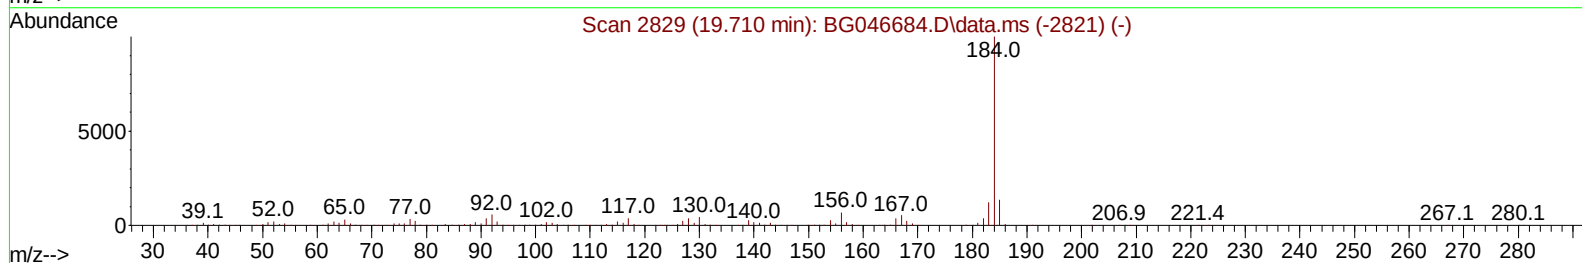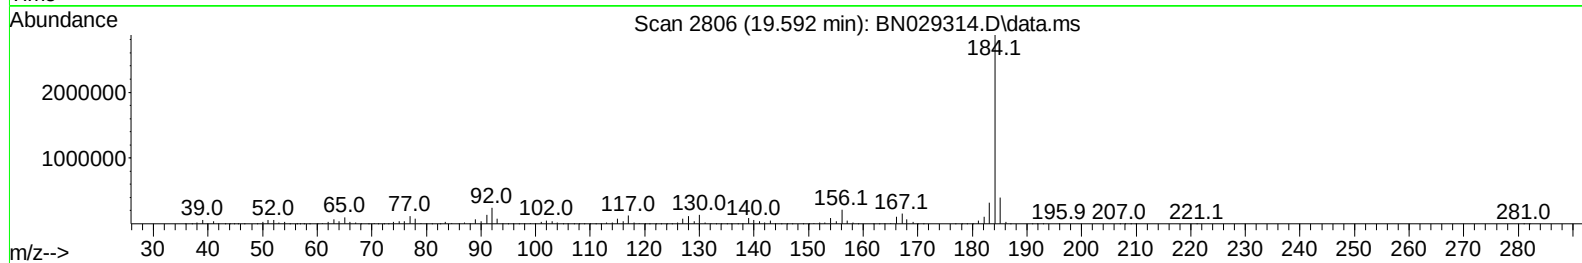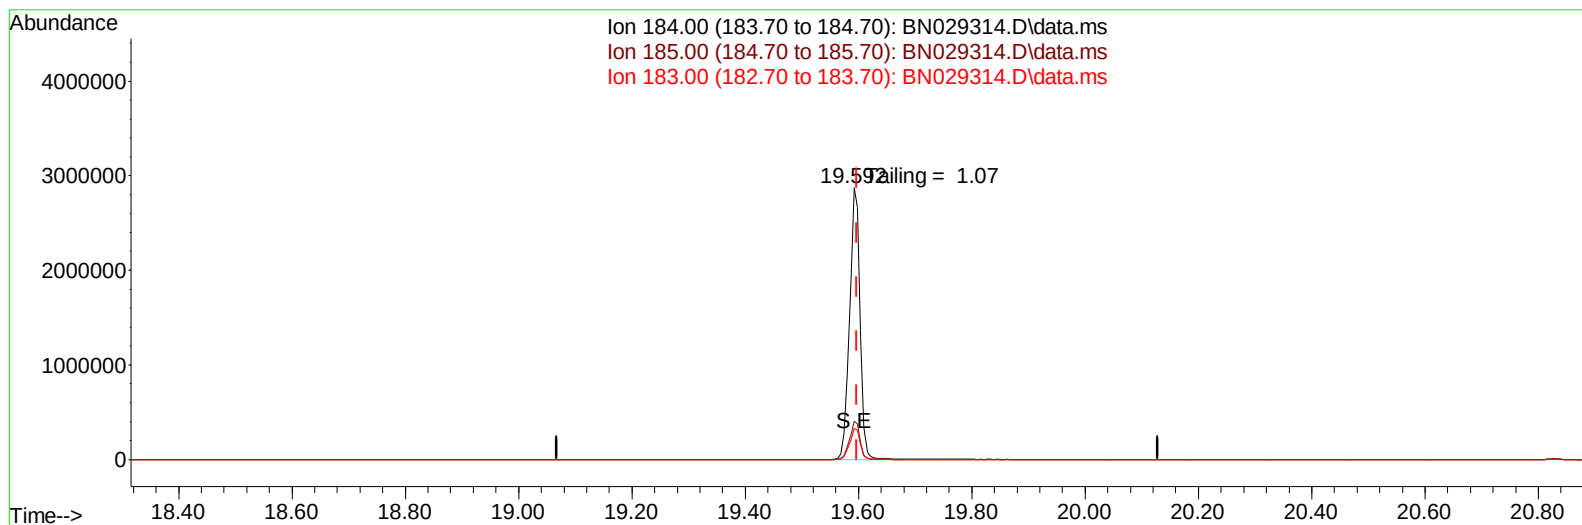

TIC: BN029314.D\data.ms

(77) Benzidine

19.592min (-0.006) 0.00 ng

response 3708933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.36
0.00	0.00	0.00