
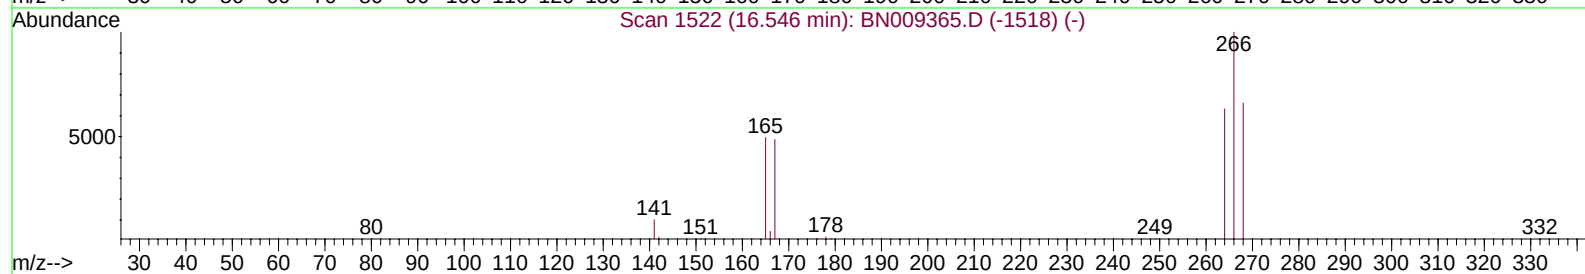
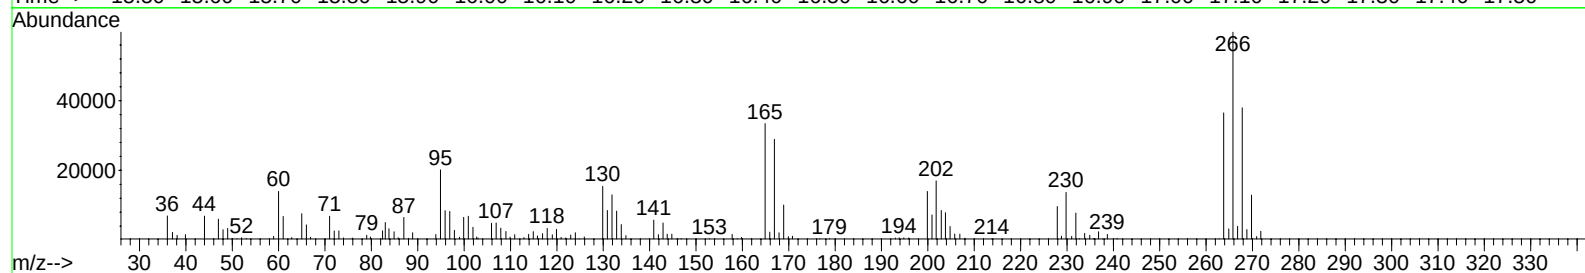


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN012020\
Data File : BN009397.D
Acq On : 20 Jan 2020 10:18
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 18:21:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN011420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 09:33:55 2020
Response via : Initial Calibration

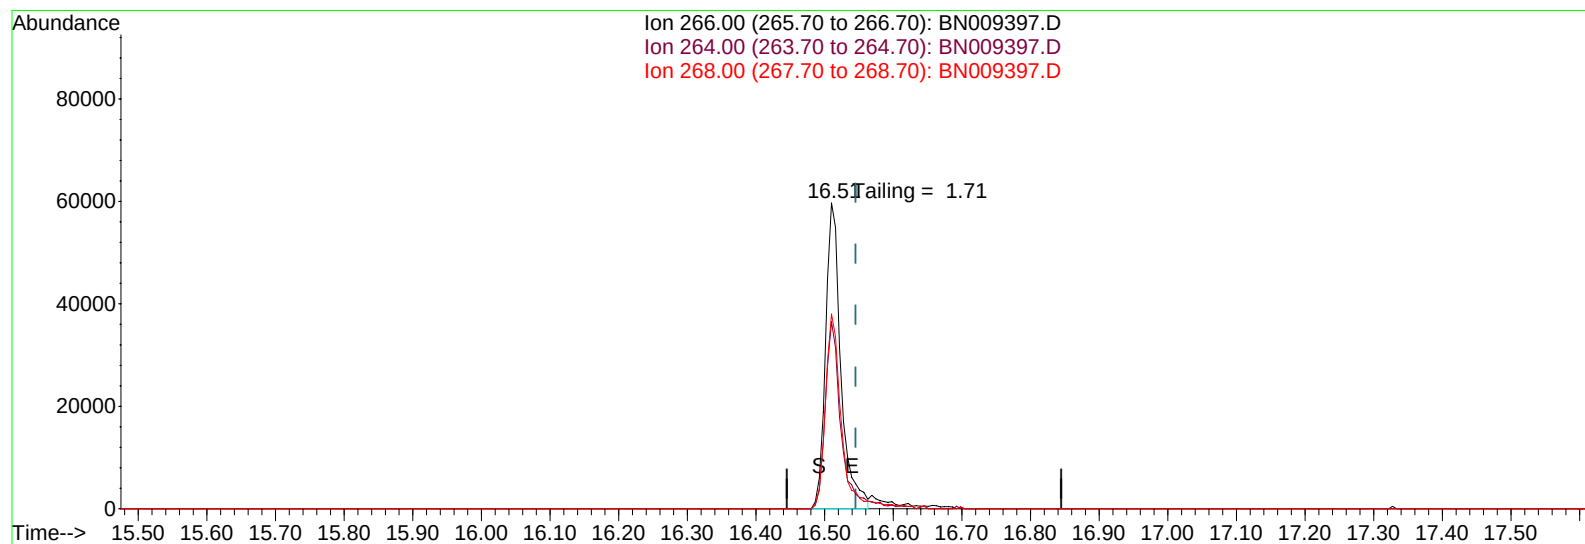

(22) Pentachlorophenol

16.510min (-0.035) 0.00ng

response 97260

Ion	Exp%	Act%
266.00	100	100
264.00	72.20	61.20
268.00	79.70	63.69#
0.00	0.00	0.00