


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012020\
 Data File : BN009397.D
 Acq On : 20 Jan 2020 10:18
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN011420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 09:33:55 2020

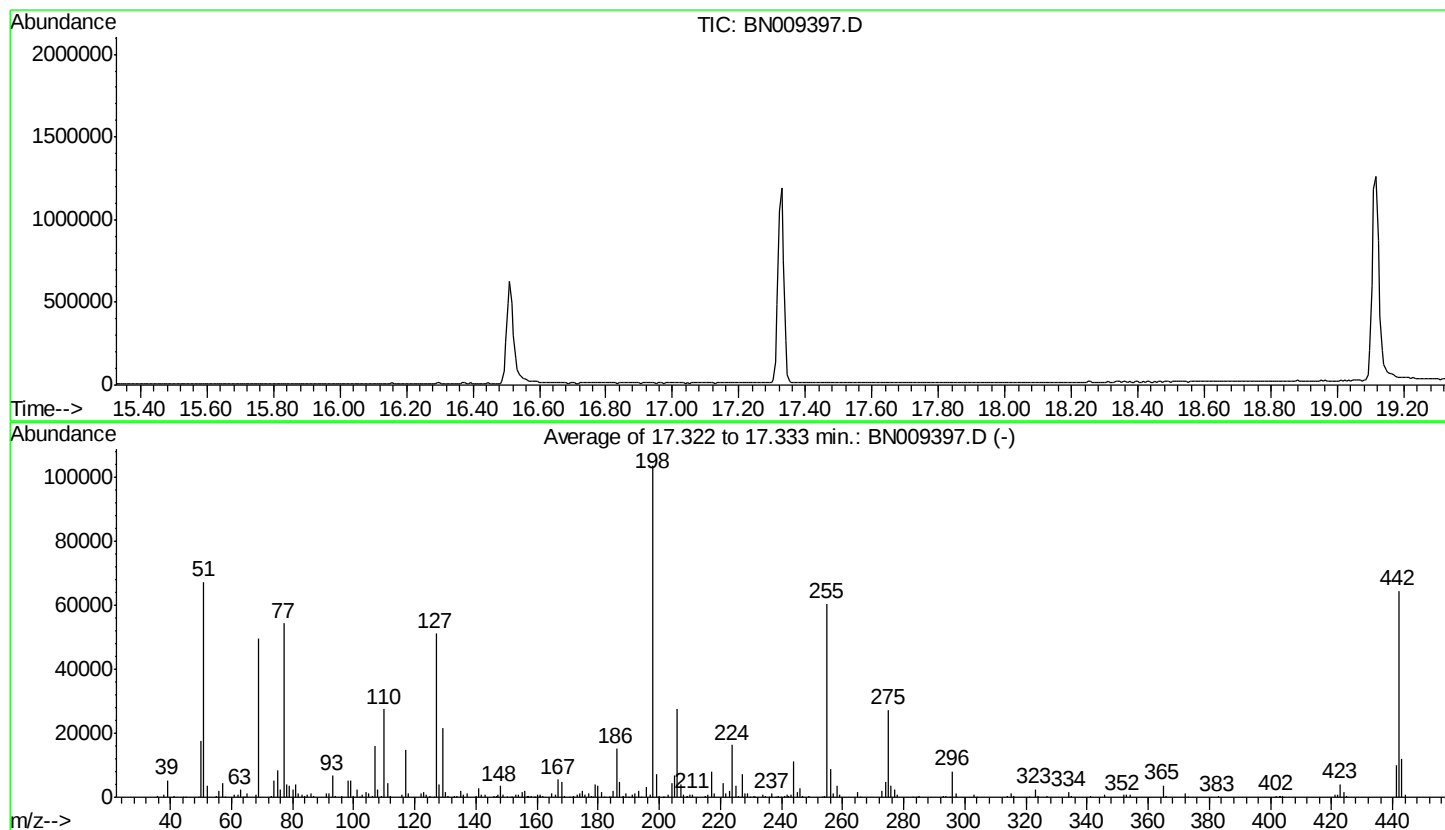

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.9	67112	PASS
68	69	0.00	2	1.6	805	PASS
69	198	0.00	100	48.0	49653	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	51109	PASS
197	198	0.00	2	0.8	792	PASS
198	198	100	100	100.0	103437	PASS
199	198	5	9	7.0	7264	PASS
275	198	10	60	26.3	27240	PASS
365	198	1	100	3.5	3645	PASS
441	198	0.01	100	9.9	10195	PASS
442	198	50	100	62.3	64482	PASS
443	442	15	24	18.8	12138	PASS