

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
 Data File : BN018433.D
 Acq On : 20 Jan 2022 10:58
 Operator : CG/JU
 Sample : PB142140BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK140

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	20	rBV	95119	143331	1.21%	0.111%
2	3.464	78	81	99	rBV	1530039	2486912	21.00%	1.928%
3	3.805	135	139	143	rVB3	23532	30506	0.26%	0.024%
4	6.775	637	644	659	rBV	2194976	3489710	29.46%	2.706%
5	6.928	663	670	682	rVV	1713723	2633648	22.24%	2.042%
6	7.122	694	703	720	rBV	2206400	3537213	29.86%	2.743%
7	7.587	776	782	790	rBV	1528050	2372120	20.03%	1.839%
8	8.305	897	904	917	rBV	2696903	4339880	36.64%	3.365%
9	8.740	969	978	992	rBV	2172027	3498786	29.54%	2.713%
10	9.457	1093	1100	1110	rBV	2014136	3216996	27.16%	2.495%
11	9.993	1184	1191	1204	rBV	2607853	4455561	37.62%	3.455%
12	10.363	1247	1254	1266	rVB	2157254	3593273	30.34%	2.786%
13	10.504	1271	1278	1295	rBV	2671036	4553534	38.45%	3.531%
14	11.975	1521	1528	1535	rBV	35348	66867	0.56%	0.052%
15	13.651	1806	1813	1826	rBV	5023384	6885529	58.13%	5.339%
16	13.922	1852	1859	1874	rBV	5500399	7782002	65.70%	6.034%
17	14.234	1904	1912	1925	rBV	3288336	4836712	40.84%	3.751%
18	14.445	1942	1948	1973	rBV	1944713	3251438	27.45%	2.521%
19	15.228	2074	2081	2095	rBV	6522686	9110064	76.92%	7.064%
20	15.357	2095	2103	2118	rVV	2243624	3291023	27.79%	2.552%
21	15.463	2118	2121	2127	rVB3	44743	70826	0.60%	0.055%
22	16.763	2338	2342	2349	rVB3	16425	26881	0.23%	0.021%
23	16.975	2371	2378	2386	rBV	4067484	5687637	48.02%	4.410%
24	17.075	2389	2395	2408	rVV2	6999290	9881739	83.43%	7.663%
25	18.939	2707	2712	2717	rBV	80461	107109	0.90%	0.083%
26	19.010	2720	2724	2730	rVB2	75469	110195	0.93%	0.085%
27	19.375	2775	2786	2805	rBV	8461365	11668235	98.52%	9.048%
28	20.910	3043	3047	3049	rBV5	10658	15702	0.13%	0.012%
29	21.169	3086	3091	3100	rBV	4847914	6245357	52.73%	4.843%
30	21.345	3119	3121	3125	rVB5	17217	17263	0.15%	0.013%
31	21.774	3191	3194	3201	rVB3	73247	103900	0.88%	0.081%
32	22.239	3269	3273	3277	rBV	100494	126233	1.07%	0.098%
33	22.345	3286	3291	3297	rVB4	80773	119412	1.01%	0.093%
34	22.745	3355	3359	3369	rVB	164013	254491	2.15%	0.197%
35	22.974	3393	3398	3408	rVB2	126426	212878	1.80%	0.165%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
 Data File : BN018433.D
 Acq On : 20 Jan 2022 10:58
 Operator : CG/JU
 Sample : PB142140BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK140

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

36	23.245	3436	3444	3452	rBV	6340321	11844078	100.00%	9.184%
37	23.315	3452	3456	3461	rVV2	261858	478642	4.04%	0.371%
38	23.386	3461	3468	3485	rVB2	3224595	6256662	52.83%	4.852%
39	23.704	3517	3522	3530	rVB4	127043	261118	2.20%	0.202%
40	23.963	3560	3566	3575	rBV2	210229	430530	3.63%	0.334%
41	24.568	3664	3669	3682	rVB5	107202	269873	2.28%	0.209%
42	24.715	3688	3694	3709	rVB2	226096	514703	4.35%	0.399%
43	25.598	3836	3844	3856	rBV4	229717	683115	5.77%	0.530%




Sum of corrected areas: 128961684

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
Data File : BN018433.D
Acq On : 20 Jan 2022 10:58
Operator : CG/JU
Sample : PB142140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

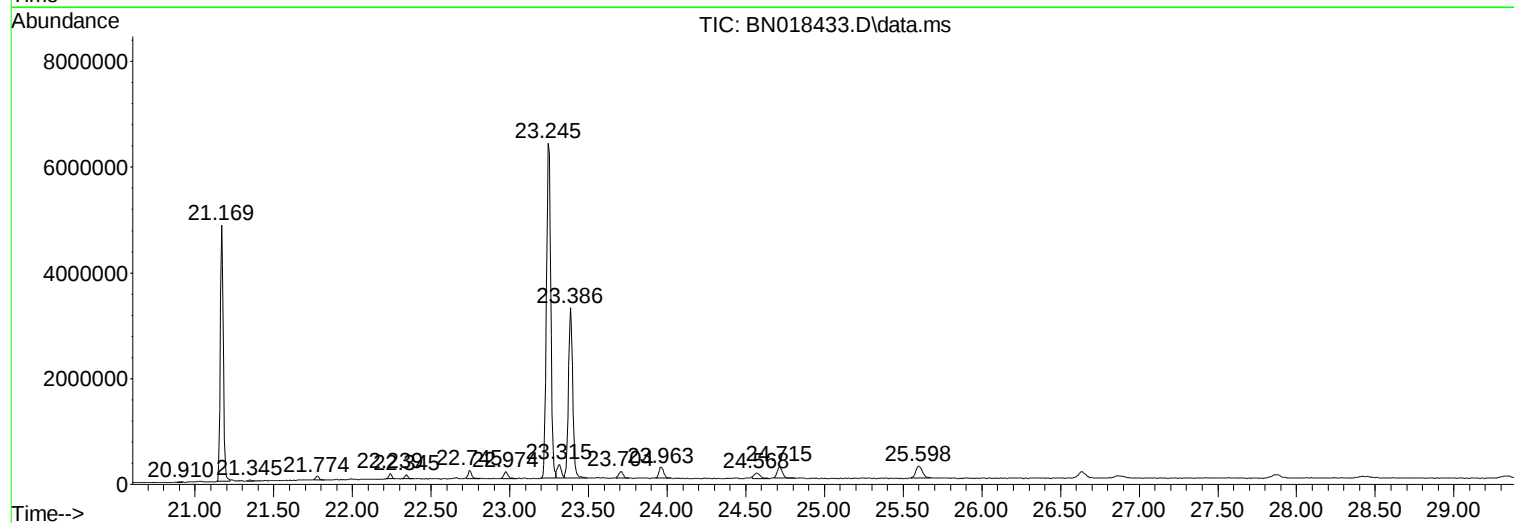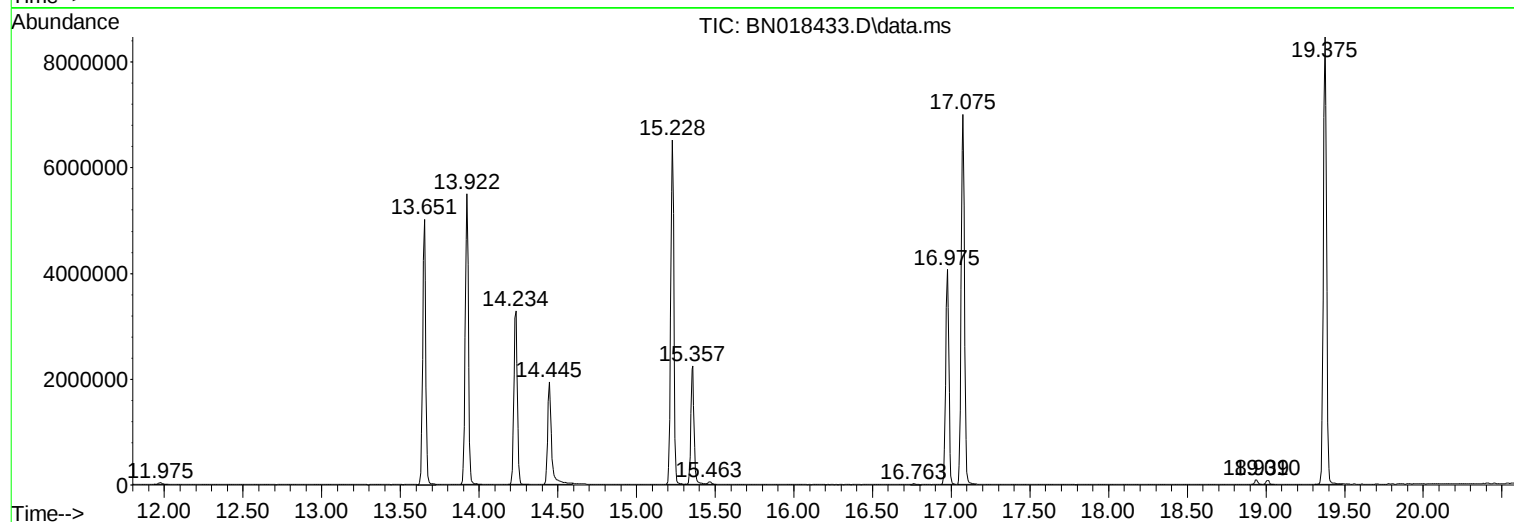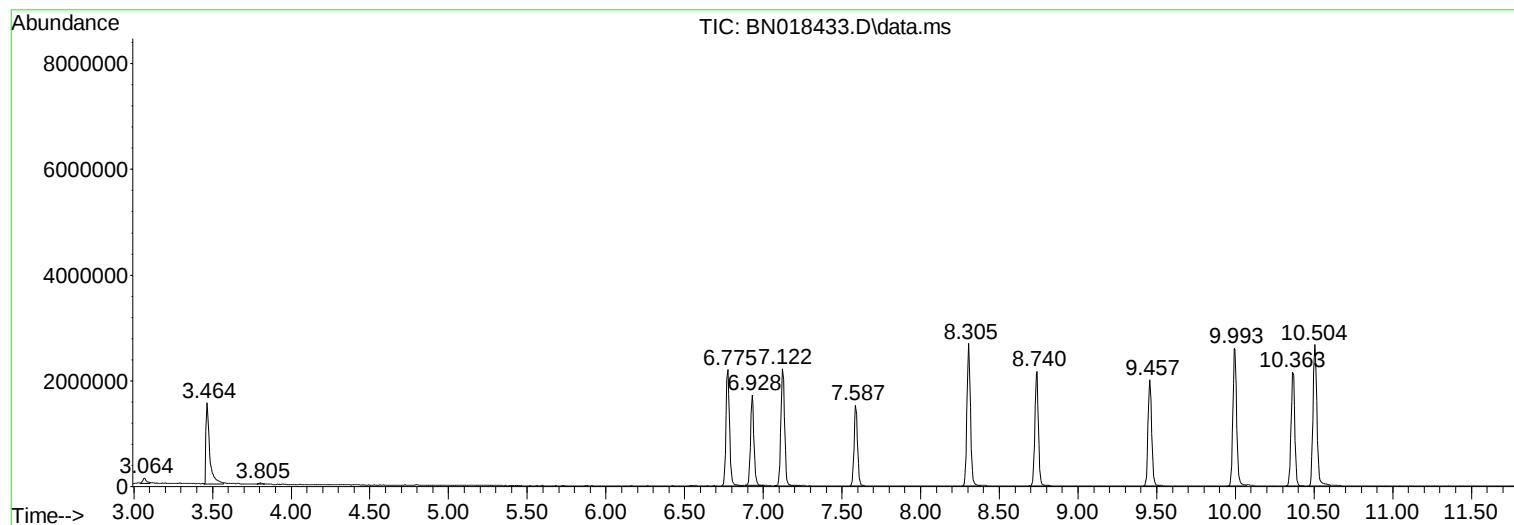

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
Data File : BN018433.D
Acq On : 20 Jan 2022 10:58
Operator : CG/JU
Sample : PB142140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK140










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
25.598	2.18 ng/ul	683115	Perylene-d12	23.386

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heneicosane	296	C21H44	000629-94-7	95
2			Eicosane	282	C20H42	000112-95-8	89
3			Heneicosane	296	C21H44	000629-94-7	87
4			Heptadecane, 2,6,10,15-tetramethyl-	296	C21H44	054833-48-6	64
5			Nonadecane	268	C19H40	000629-92-5	64

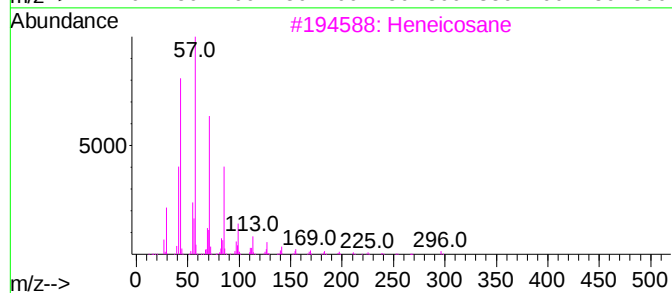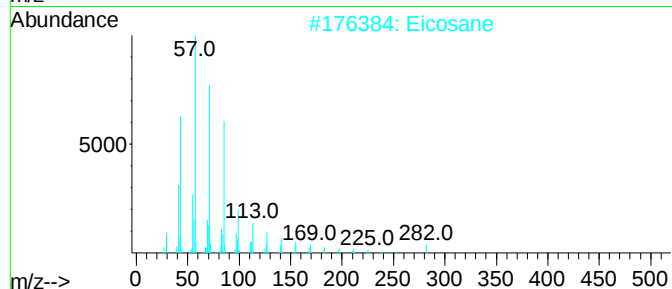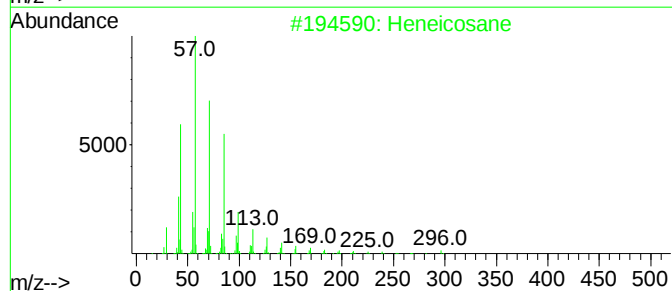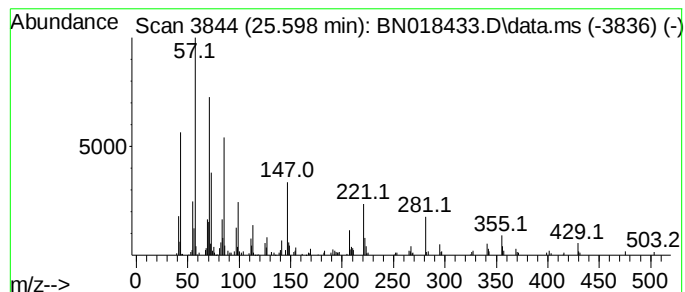

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
Data File : BN018433.D
Acq On : 20 Jan 2022 10:58
Operator : CG/JU
Sample : PB142140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
(DEL) Alkane: S...	25.598	2.2	ng/ul	683115	6	23.386	6256660	20.0