

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
 Data File : BN018434.D
 Acq On : 20 Jan 2022 12:09
 Operator : CG/JU
 Sample : N1193-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBCM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018434.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	16	rBV	70549	94572	0.94%	0.089%
2	3.093	16	18	23	rVB	46186	63922	0.64%	0.060%
3	3.464	77	81	95	rBV	1149316	1841860	18.36%	1.740%
4	3.711	120	123	128	rVB2	29310	47036	0.47%	0.044%
5	3.752	128	130	134	rVV4	11106	11849	0.12%	0.011%
6	3.799	134	138	146	rVB	57667	92210	0.92%	0.087%
7	3.899	153	155	160	rVB4	11646	14974	0.15%	0.014%
8	4.711	288	293	301	rVB3	37380	58096	0.58%	0.055%
9	5.246	380	384	387	rBV3	13964	21113	0.21%	0.020%
10	5.993	506	511	516	rBV7	7259	12865	0.13%	0.012%
11	6.087	523	527	535	rVB7	11024	21325	0.21%	0.020%
12	6.511	594	599	603	rVB7	6193	10505	0.10%	0.010%
13	6.605	610	615	622	rVB	203404	293331	2.92%	0.277%
14	6.775	637	644	651	rBV	1887274	2929079	29.19%	2.767%
15	6.834	651	654	663	rVB4	67851	142048	1.42%	0.134%
16	6.928	663	670	679	rBV	1351904	2153596	21.46%	2.034%
17	7.122	697	703	717	rVB	1833952	2950085	29.40%	2.787%
18	7.252	719	725	731	rVB3	37410	72438	0.72%	0.068%
19	7.410	748	752	755	rBV4	8295	11937	0.12%	0.011%
20	7.452	755	759	764	rVB4	20155	32701	0.33%	0.031%
21	7.499	764	767	771	rBV6	10512	15634	0.16%	0.015%
22	7.587	775	782	794	rVB2	1199409	1900001	18.94%	1.795%
23	7.740	801	808	815	rVB2	31445	56752	0.57%	0.054%
24	7.834	815	824	834	rBV2	100775	230318	2.30%	0.218%
25	8.022	853	856	860	rVB5	8974	10431	0.10%	0.010%
26	8.093	863	868	871	rBV2	22385	33240	0.33%	0.031%
27	8.146	872	877	881	rVV	62323	101410	1.01%	0.096%
28	8.181	881	883	889	rVB3	25217	29994	0.30%	0.028%
29	8.305	894	904	921	rBV	2412417	3795924	37.83%	3.586%
30	8.481	928	934	939	rBV5	19441	41584	0.41%	0.039%
31	8.640	957	961	968	rBV6	7196	14201	0.14%	0.013%
32	8.734	971	977	990	rVV	1716464	2818700	28.09%	2.663%
33	8.834	992	994	1001	rVB6	12819	19953	0.20%	0.019%
34	9.210	1055	1058	1063	rVB3	9292	12423	0.12%	0.012%
35	9.457	1091	1100	1118	rBV	1664583	2679839	26.71%	2.532%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
 Data File : BN018434.D
 Acq On : 20 Jan 2022 12:09
 Operator : CG/JU
 Sample : N1193-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBCM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

36	9.999	1185	1192	1206	rBV	2225855	3736614	37.24%	3.530%
37	10.363	1247	1254	1263	rBV	1560564	2609392	26.01%	2.465%
38	10.504	1271	1278	1301	rBV	2205486	3831102	38.18%	3.619%
39	11.969	1522	1527	1538	rVB2	30396	58166	0.58%	0.055%
40	13.651	1806	1813	1824	rBV	4280189	5791834	57.72%	5.471%
41	13.922	1852	1859	1869	rBV	4502153	6431337	64.10%	6.076%
42	14.234	1905	1912	1920	rBV	2402594	3452735	34.41%	3.262%
43	14.445	1942	1948	1972	rBV	1530894	2636316	26.27%	2.490%
44	14.663	1981	1985	1992	rVB6	28558	50061	0.50%	0.047%
45	15.228	2074	2081	2095	rBV	5687733	7782501	77.56%	7.352%
46	15.357	2097	2103	2116	rVV	2023192	2794898	27.85%	2.640%
47	15.469	2118	2122	2129	rVB5	42581	72110	0.72%	0.068%
48	16.763	2336	2342	2348	rBV5	14164	23009	0.23%	0.022%
49	16.975	2372	2378	2388	rBV	3095154	4252598	42.38%	4.017%
50	17.075	2388	2395	2411	rVV	6043284	8534544	85.06%	8.062%
51	17.192	2411	2415	2422	rVB8	22662	36726	0.37%	0.035%
52	18.939	2708	2712	2718	rBV	74288	98933	0.99%	0.093%
53	19.010	2720	2724	2731	rVB2	75914	97867	0.98%	0.092%
54	19.375	2780	2786	2800	rBV	7428805	9958844	99.25%	9.408%
55	20.751	3017	3020	3023	rBV2	39555	47839	0.48%	0.045%
56	21.174	3086	3092	3103	rBV	3575415	4774113	47.58%	4.510%
57	21.351	3120	3122	3125	rBV4	17870	17141	0.17%	0.016%
58	21.780	3192	3195	3200	rVB3	43536	51915	0.52%	0.049%
59	22.245	3270	3274	3278	rVB3	87292	108064	1.08%	0.102%
60	22.751	3356	3360	3367	rVB2	140792	210221	2.10%	0.199%
61	23.251	3437	3445	3453	rBV	5188071	10033848	100.00%	9.479%
62	23.316	3453	3456	3461	rVV3	221625	371609	3.70%	0.351%
63	23.386	3461	3468	3481	rVB2	2266058	4437204	44.22%	4.192%
64	23.968	3562	3567	3575	rVB2	169805	313083	3.12%	0.296%
65	24.721	3689	3695	3703	rVB2	141323	319026	3.18%	0.301%
66	25.610	3840	3846	3855	rVB6	114475	287143	2.86%	0.271%




Sum of corrected areas: 105856739

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
Data File : BN018434.D
Acq On : 20 Jan 2022 12:09
Operator : CG/JU
Sample : N1193-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBCM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

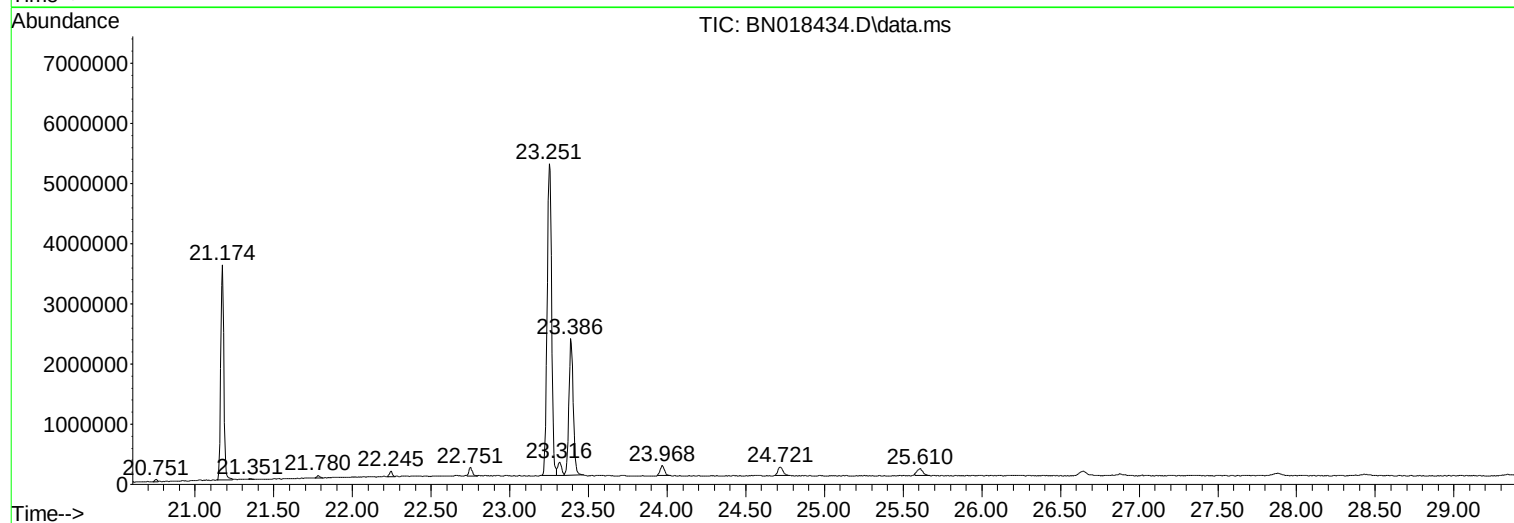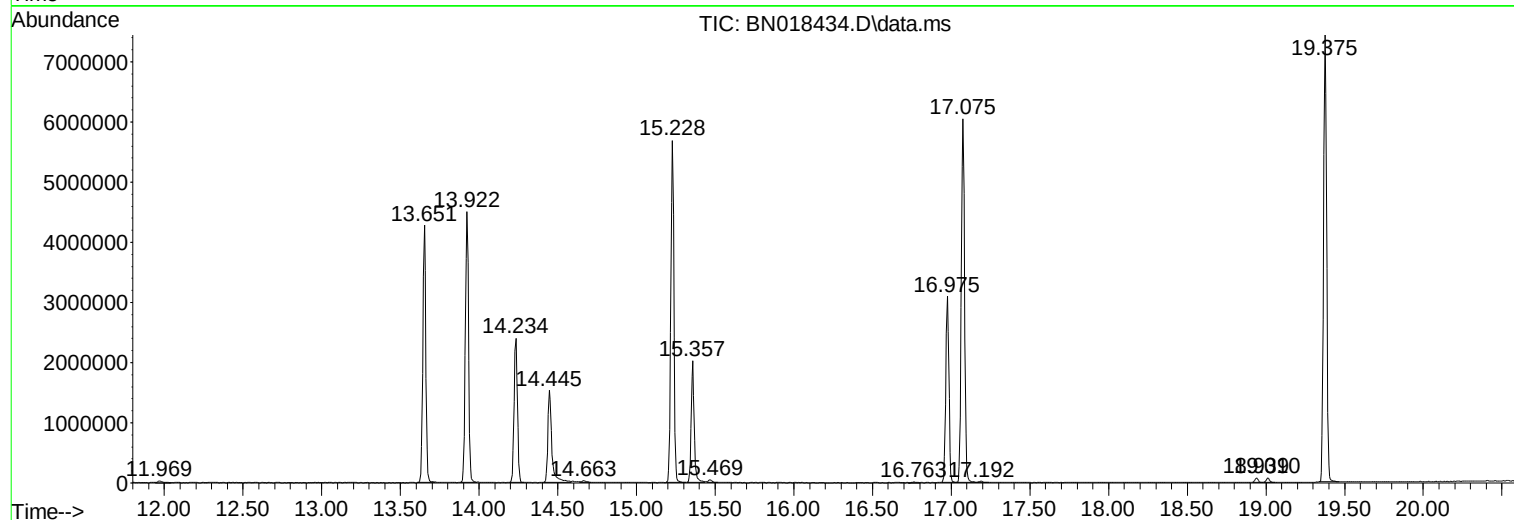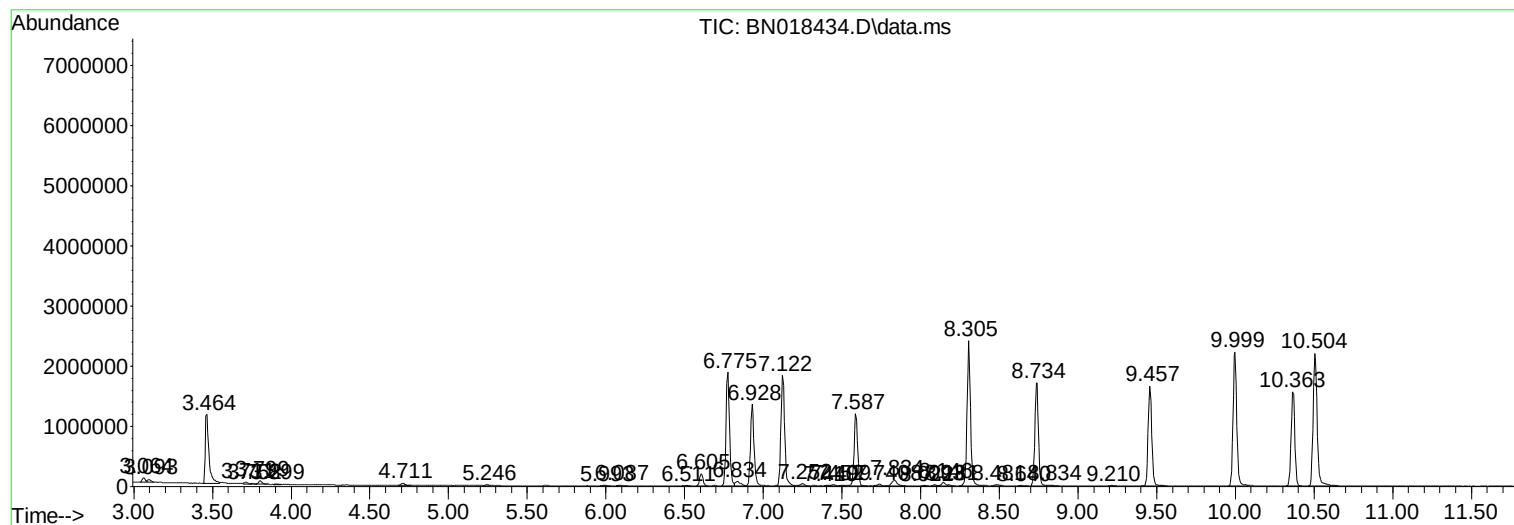

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
Data File : BN018434.D
Acq On : 20 Jan 2022 12:09
Operator : CG/JU
Sample : N1193-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBCM6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.605	3.09 ng/ul	293331	1,4-Dichlorobenzene-d4	7.587

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Octane, 2,2,6-trimethyl-	156	C11H24	062016-28-8	83
2	Decane, 2,6,6-trimethyl-	184	C13H28	062108-24-1	59
3	Tridecane, 3-methyl-	198	C14H30	006418-41-3	59
4	Oxalic acid, isobutyl nonyl ester	272	C15H28O4	1010309-37-4	59
5	2,2,7,7-Tetramethyloctane	170	C12H26	001071-31-4	53

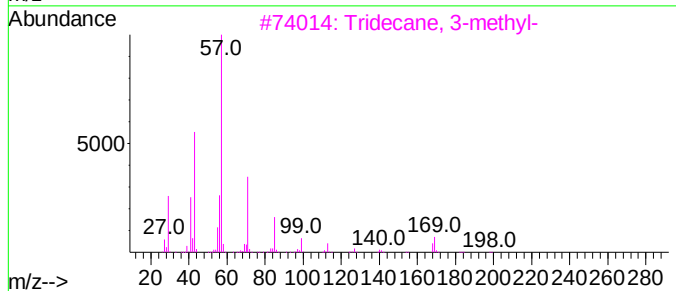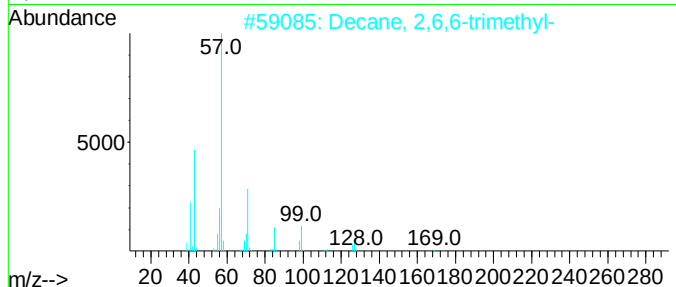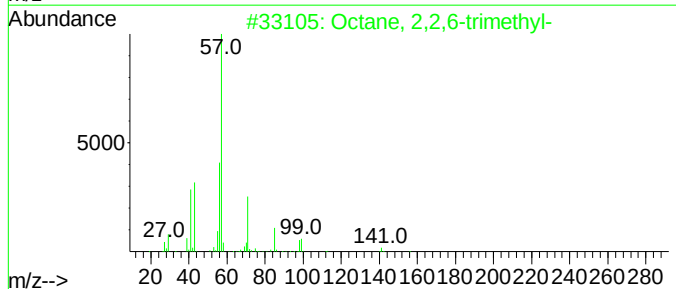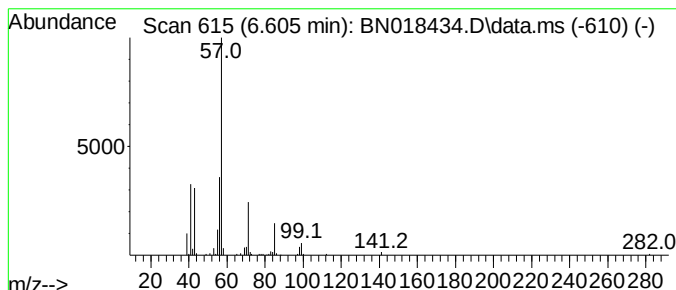

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
Data File : BN018434.D
Acq On : 20 Jan 2022 12:09
Operator : CG/JU
Sample : N1193-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBCM6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.834	2.42 ng/ul	230318	1,4-Dichlorobenzene-d4	7.587

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hentriacontane	437	C31H64	000630-04-6	72
2	Undecane, 2,9-dimethyl-	184	C13H28	017301-26-7	64
3	Undecane, 3,8-dimethyl-	184	C13H28	017301-30-3	64
4	Hexacosane	366	C26H54	000630-01-3	64
5	Pentacosane	352	C25H52	000629-99-2	64

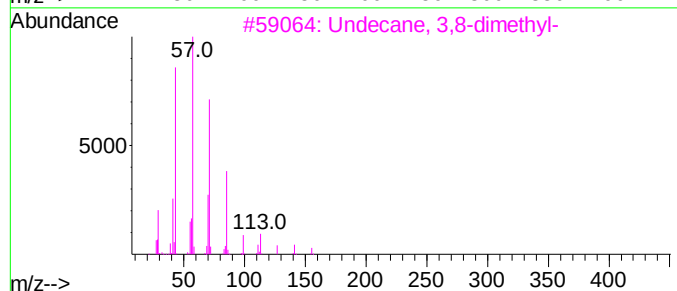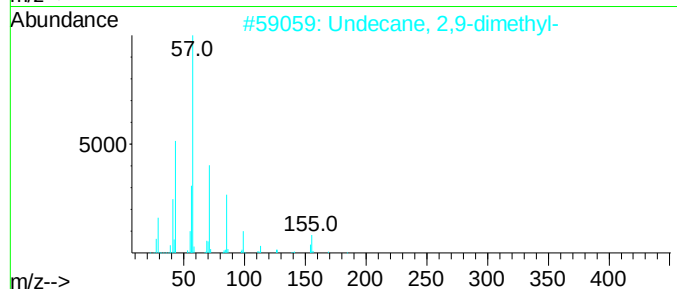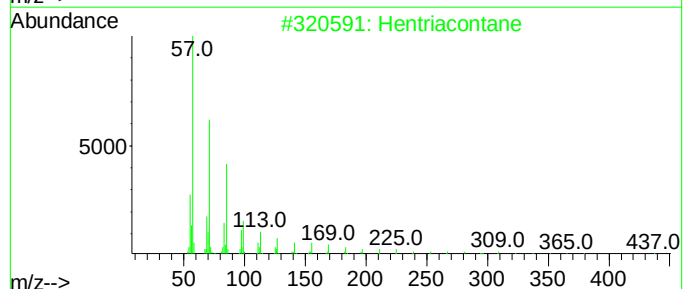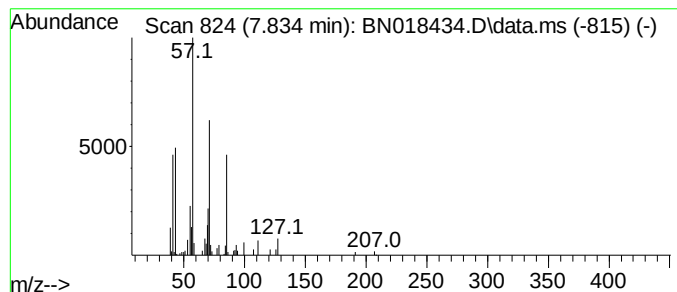

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012022\
Data File : BN018434.D
Acq On : 20 Jan 2022 12:09
Operator : CG/JU
Sample : N1193-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBCM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---	#	RT	Resp	Conc
(DEL) Alkane: S...	6.605	3.1	ng/ul	293331	1	7.587	1900000	20.0	
(DEL) Alkane: S...	7.834	2.4	ng/ul	230318	1	7.587	1900000	20.0	