

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
 Data File : BN035995.D
 Acq On : 20 Jan 2025 12:51
 Operator : RC/JU
 Sample : Q1113-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DSN002

Quant Time: Jan 20 13:23:40 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 02 15:39:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2567	0.400	ng	-0.02
7) Naphthalene-d8	10.611	136	5127	0.400	ng	#-0.01
13) Acenaphthene-d10	14.452	164	3037	0.400	ng	0.00
19) Phenanthrene-d10	17.186	188	5748	0.400	ng	#-0.02
29) Chrysene-d12	21.367	240	5349	0.400	ng	-0.02
35) Perylene-d12	23.663	264	5484	0.400	ng	#-0.03
System Monitoring Compounds						
4) 2-Fluorophenol	5.398	112	876	0.139	ng	-0.01
5) Phenol-d6	6.972	99	647	0.083	ng	-0.01
8) Nitrobenzene-d5	8.956	82	2618	0.645	ng	-0.03
11) 2-Methylnaphthalene-d10	12.198	152	2852	0.415	ng	-0.02
14) 2,4,6-Tribromophenol	15.933	330	515	0.353	ng	-0.02
15) 2-Fluorobiphenyl	13.073	172	4348	0.326	ng	-0.02
27) Fluoranthene-d10	19.216	212	7124	0.499	ng	-0.02
31) Terphenyl-d14	19.815	244	5403	0.507	ng	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.318	88	1795	0.704	ng	# 93
3) n-Nitrosodimethylamine	3.621	42	132	0.030	ng	# 56
6) bis(2-Chloroethyl)ether	7.268	93	361	0.061	ng	# 20
18) Fluorene	15.468	166	905	0.088	ng	# 8
24) Pentachlorophenol	16.839	266	77	0.040	ng	96
34) Bis(2-ethylhexyl)phtha...	21.295	149	6313	0.823	ng	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
Data File : BN035995.D
Acq On : 20 Jan 2025 12:51
Operator : RC/JU
Sample : Q1113-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DSN002


Quant Time: Jan 20 13:23:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 15:39:17 2025
Response via : Initial Calibration

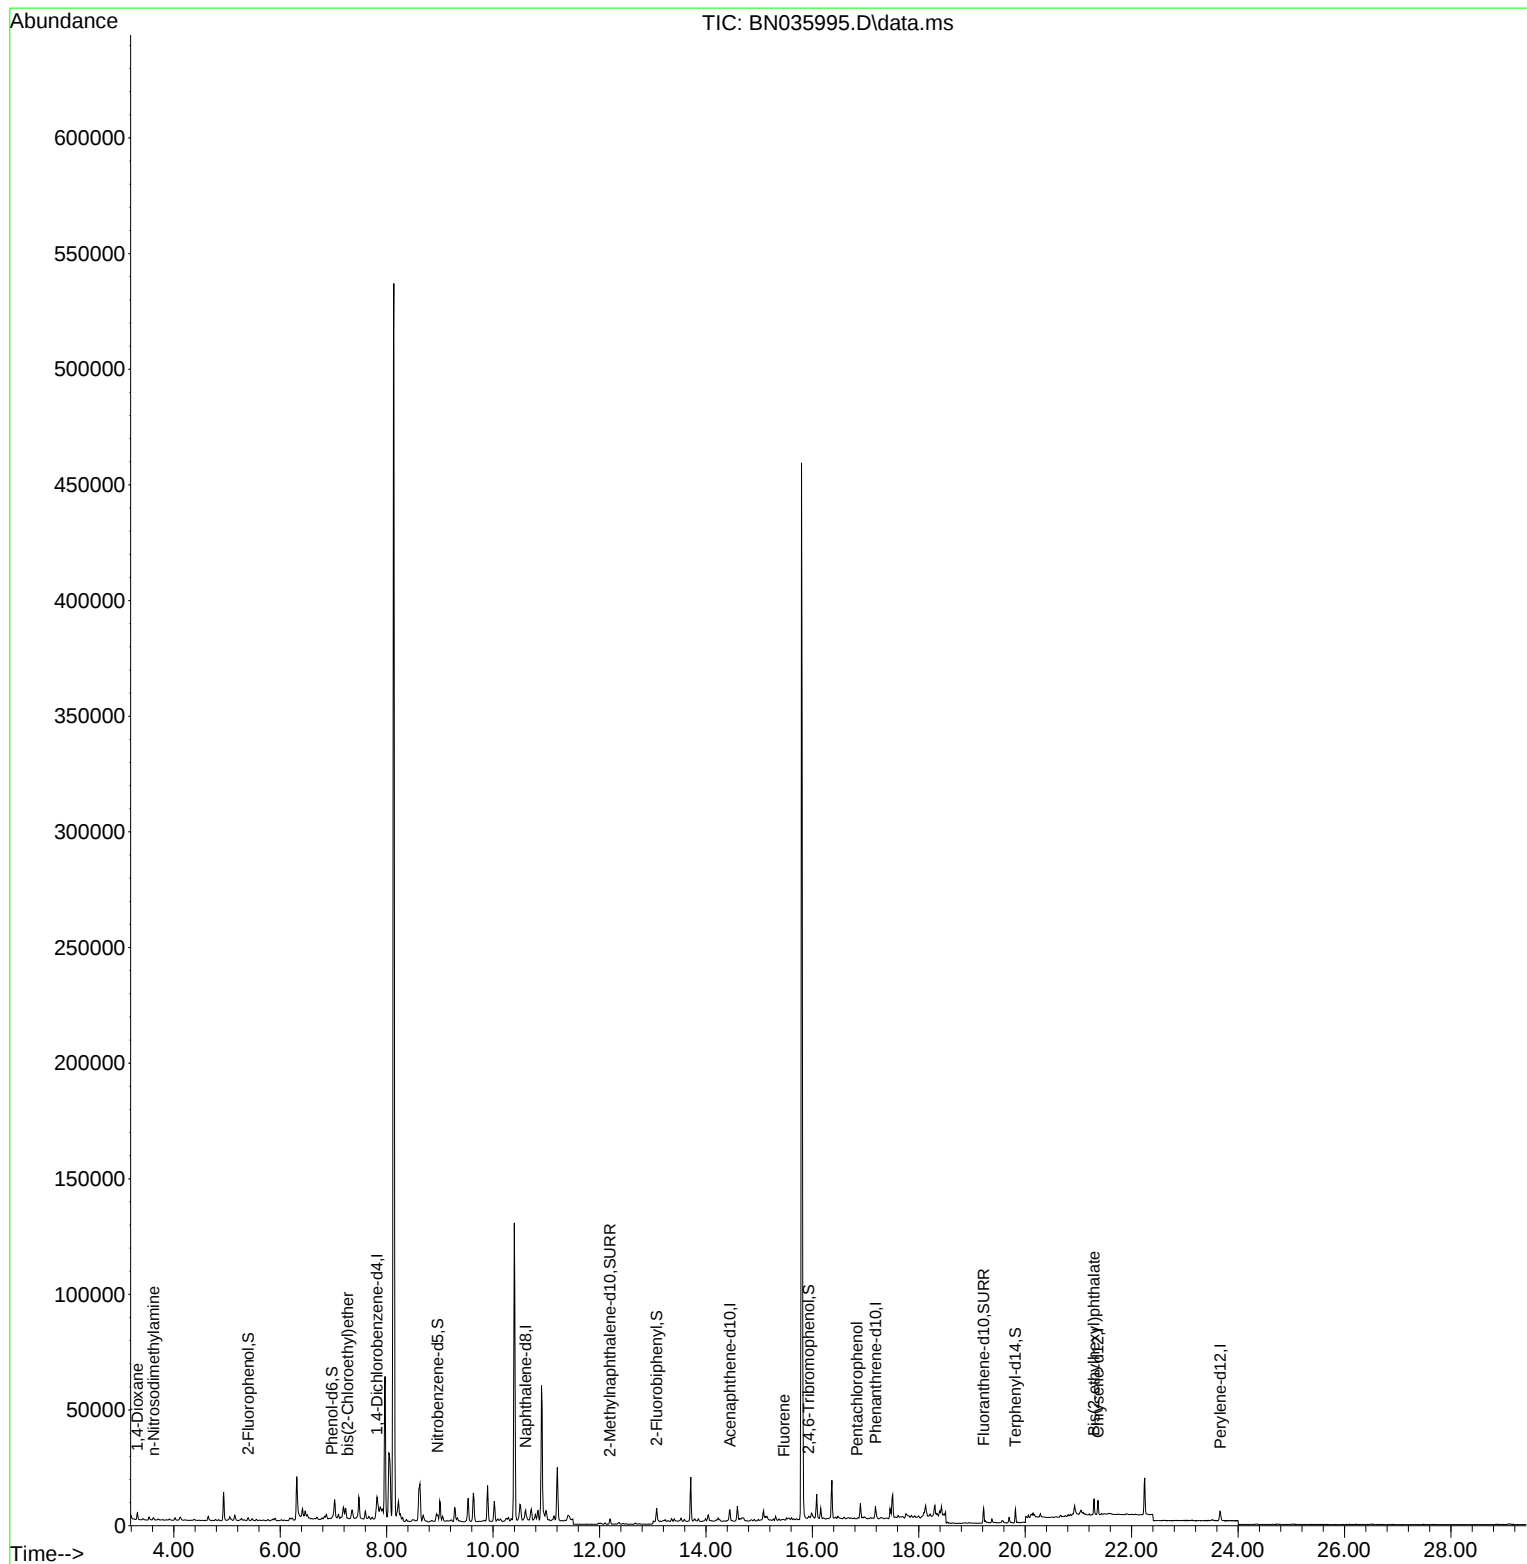






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.817 min Scan# 64
 Delta R.T. -0.019 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51


Instrument :
 BNA_N
 ClientSampleId :
 DSN002





Tgt Ion:152 Resp: 2567
 Ion Ratio Lower Upper
 152 100
 150 151.5 117.8 176.6
 115 67.0 51.0 76.4




#2
 1,4-Dioxane
 Concen: 0.704 ng
 RT: 3.318 min Scan# 19
 Delta R.T. -0.004 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51

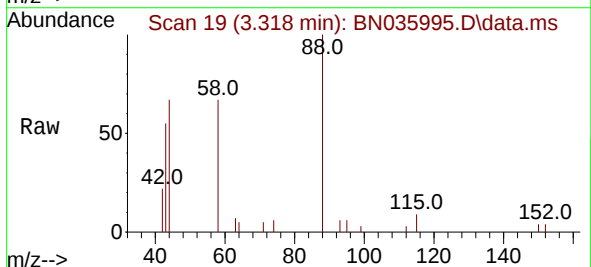

Tgt Ion: 88 Resp: 1795
 Ion Ratio Lower Upper
 88 100
 43 50.8 32.7 49.1#
 58 80.3 63.0 94.4



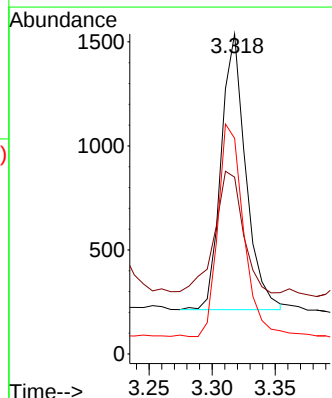





#3
n-Nitrosodimethylamine
Concen: 0.030 ng
RT: 3.621 min Scan# 61
Delta R.T. -0.011 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002


Tgt Ion: 42 Resp: 132
Ion Ratio Lower Upper
42 100
74 37.1 62.2 93.2#
44 0.0 7.1 10.7#

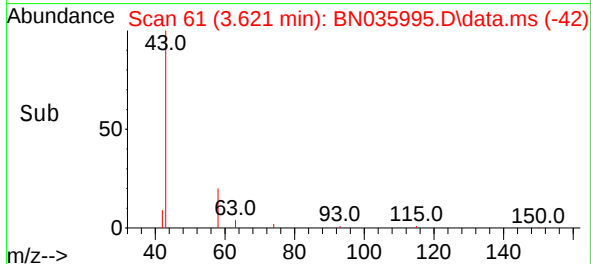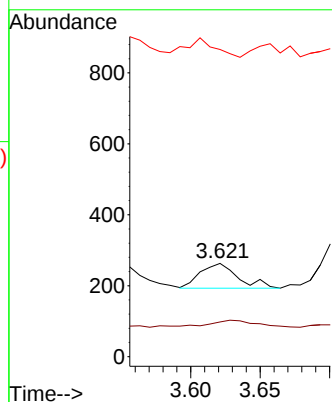

#4
2-Fluorophenol
Concen: 0.139 ng
RT: 5.398 min Scan# 307
Delta R.T. -0.011 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Tgt Ion: 112 Resp: 876
Ion Ratio Lower Upper
112 100
64 65.8 48.2 72.2
63 39.4 30.0 45.0


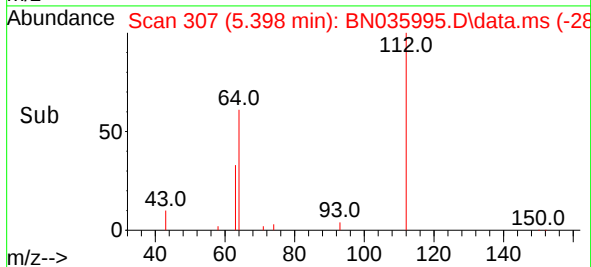

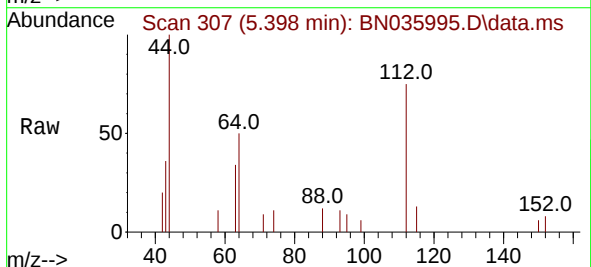




#5
Phenol-d6
Concen: 0.083 ng
RT: 6.972 min Scan# 51
Delta R.T. -0.011 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002


Tgt Ion: 99 Resp: 647
Ion Ratio Lower Upper
99 100
42 0.0 23.5 35.3#
71 39.9 35.5 53.3

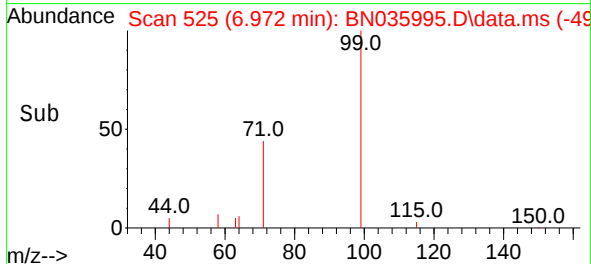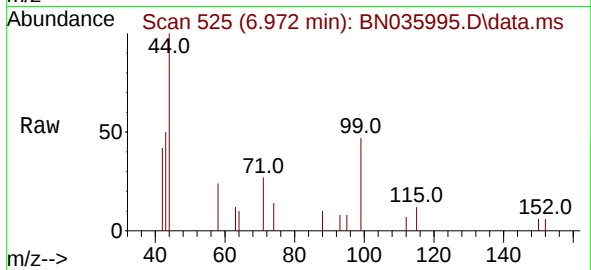

#6
bis(2-Chloroethyl)ether
Concen: 0.061 ng
RT: 7.268 min Scan# 566
Delta R.T. 0.011 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Tgt Ion: 93 Resp: 361
Ion Ratio Lower Upper
93 100
63 0.0 62.0 93.0#
95 0.0 25.5 38.3#




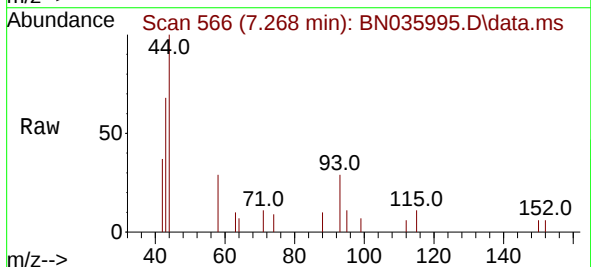




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.611 min Scan# 91
Delta R.T. -0.015 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002


Tgt Ion:136 Resp: 5127
Ion Ratio Lower Upper
136 100
137 12.2 10.6 15.8
54 11.4 9.8 14.6
68 13.9 6.6 10.0#

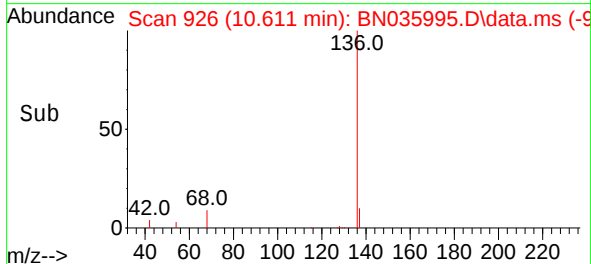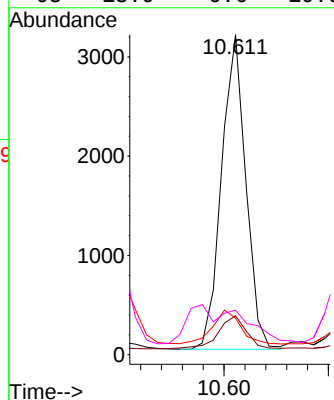

#8
Nitrobenzene-d5
Concen: 0.645 ng
RT: 8.956 min Scan# 771
Delta R.T. -0.025 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Tgt Ion: 82 Resp: 2618
Ion Ratio Lower Upper
82 100
128 32.5 36.9 55.3#
54 68.7 50.4 75.6

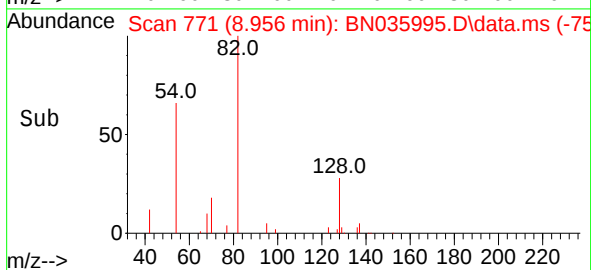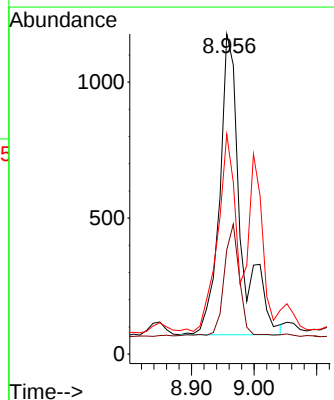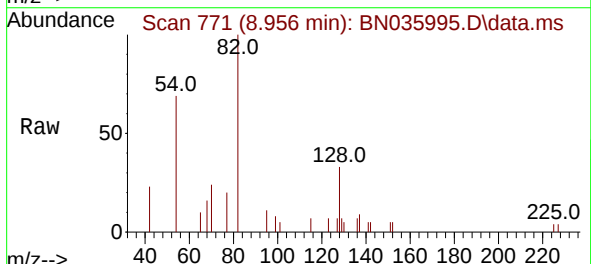



#11

2-Methylnaphthalene-d10

Concen: 0.415 ng

RT: 12.198 min Scan# 1146

Delta R.T. -0.019 min

Lab File: BN035995.D

Acq: 20 Jan 2025 12:51

Instrument :

BNA_N

ClientSampleId :





DSN002

Tgt Ion:152 Resp: 2852

Ion Ratio Lower Upper

152 100

151 21.8 17.0 25.6

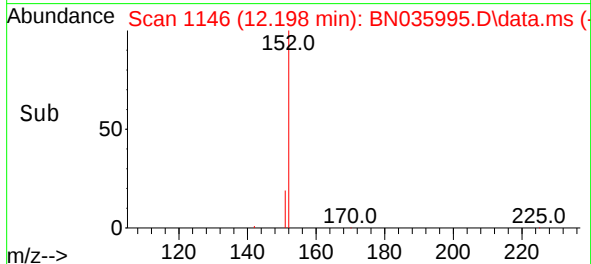

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.452 min Scan# 1441

Delta R.T. -0.010 min

Lab File: BN035995.D

Acq: 20 Jan 2025 12:51




Tgt Ion:164 Resp: 3037


Ion Ratio Lower Upper

164 100

162 103.0 83.1 124.7

160 49.5 46.0 69.0


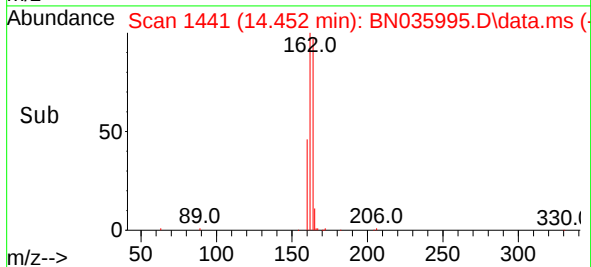

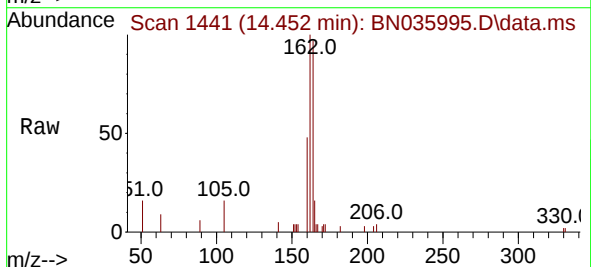




#14
2,4,6-Tribromophenol
Concen: 0.353 ng
RT: 15.933 min Scan# 11
Delta R.T. -0.024 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002


Tgt Ion:330 Resp: 515
Ion Ratio Lower Upper
330 100
332 93.6 77.2 115.8
141 69.5 31.6 47.4#

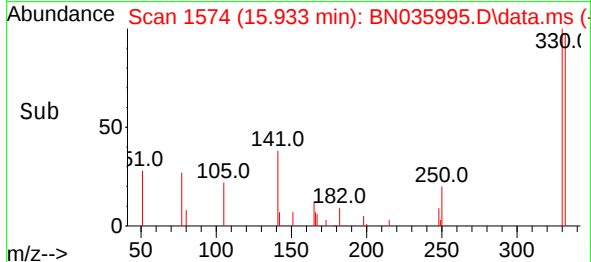

#15
2-Fluorobiphenyl
Concen: 0.326 ng
RT: 13.073 min Scan# 1312
Delta R.T. -0.020 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Tgt Ion:172 Resp: 4348
Ion Ratio Lower Upper
172 100
171 37.6 30.5 45.7
170 26.3 20.8 31.2


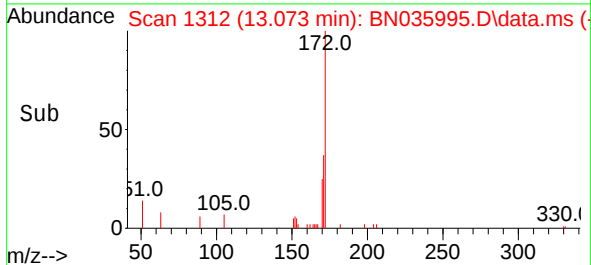

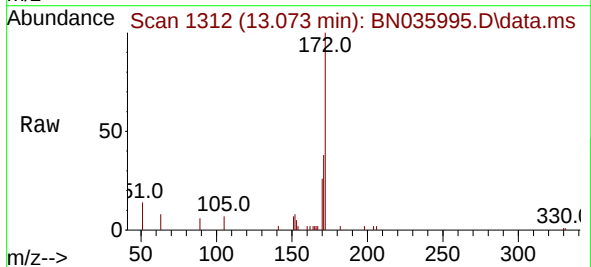




#18
Fluorene
Concen: 0.088 ng
RT: 15.468 min Scan# 1536
Delta R.T. -0.042 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002


Tgt Ion:166 Resp: 905
Ion Ratio Lower Upper
166 100
165 0.0 80.6 120.8#
167 0.0 11.4 17.0#

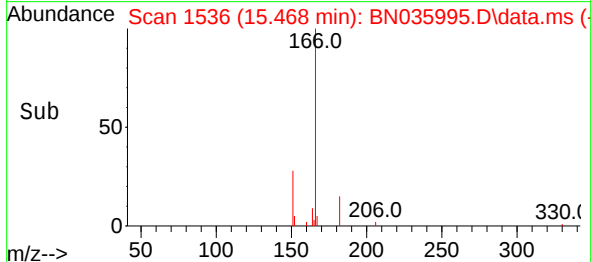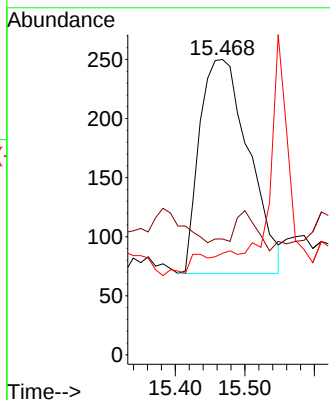

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.186 min Scan# 1675
Delta R.T. -0.024 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Tgt Ion:188 Resp: 5748
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.6 7.3 10.9#


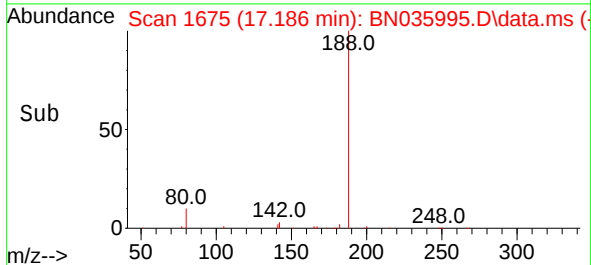
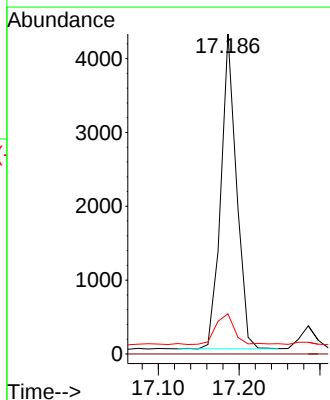
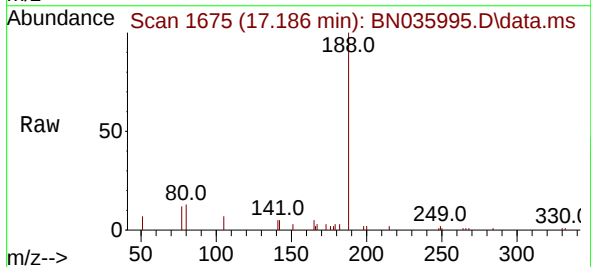


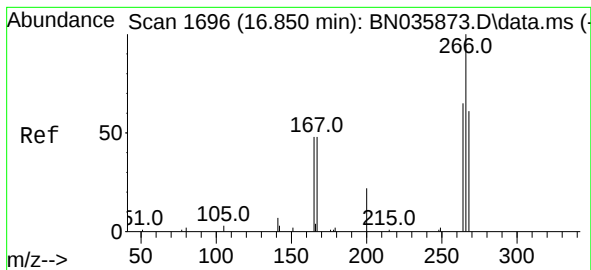

#24
 Pentachlorophenol
 Concen: 0.040 ng
 RT: 16.839 min Scan# 1647
 Delta R.T. -0.011 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51




Instrument :
 BNA_N
 ClientSampleId :
 DSN002


Tgt Ion:266 Resp: 77
 Ion Ratio Lower Upper
 266 100
 264 58.4 49.9 74.9
 268 61.0 50.2 75.2

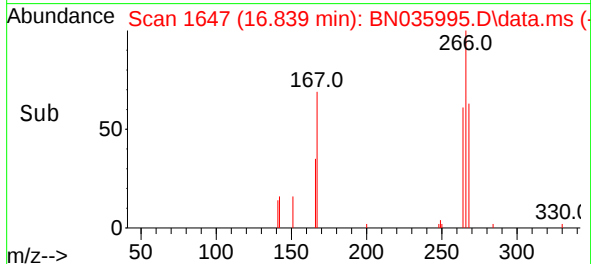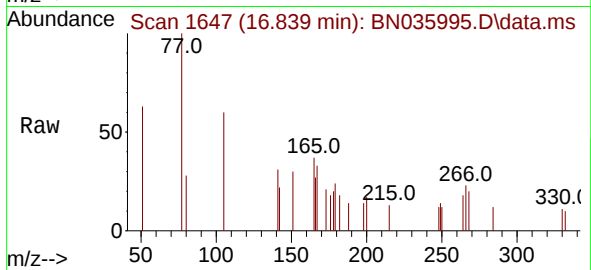

#27
 Fluoranthene-d10
 Concen: 0.499 ng
 RT: 19.216 min Scan# 1933
 Delta R.T. -0.022 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51

Tgt Ion:212 Resp: 7124
 Ion Ratio Lower Upper
 212 100
 106 12.4 9.0 13.6
 104 7.3 5.4 8.2


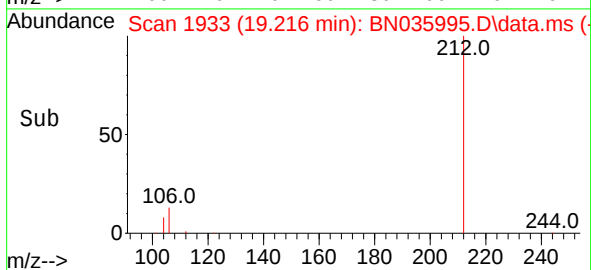

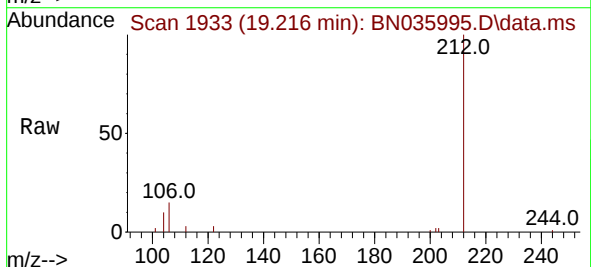




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.367 min Scan# 21
Delta R.T. -0.017 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002


Tgt Ion:240 Resp: 5349
Ion Ratio Lower Upper
240 100
120 15.2 11.1 16.7
236 29.4 24.6 36.8

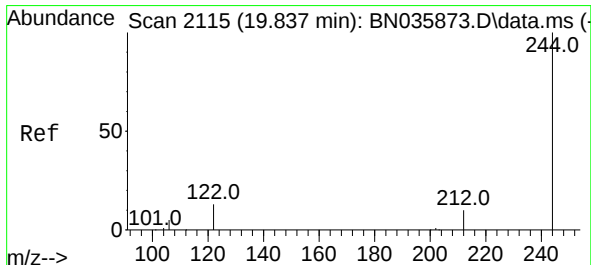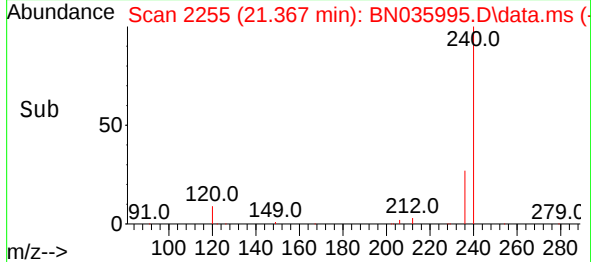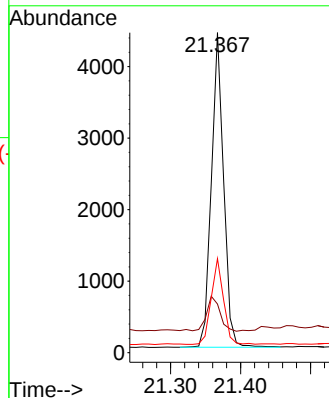

#31
Terphenyl-d14
Concen: 0.507 ng
RT: 19.815 min Scan# 2062
Delta R.T. -0.022 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Tgt Ion:244 Resp: 5403
Ion Ratio Lower Upper
244 100
212 11.7 10.1 15.1
122 16.9 12.2 18.4


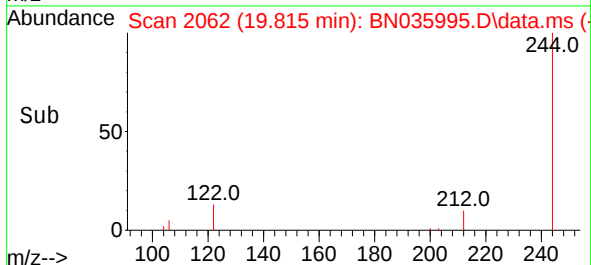
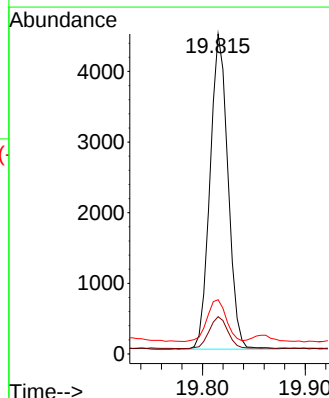
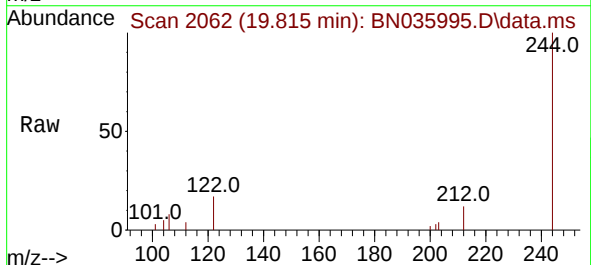


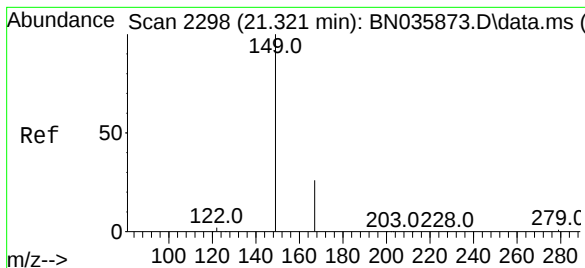

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.823 ng
 RT: 21.295 min Scan# 21
 Delta R.T. -0.026 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51

Instrument :
 BNA_N
 ClientSampleId :
 DSN002

Tgt Ion:149 Resp: 6313
 Ion Ratio Lower Upper
 149 100
 167 31.3 21.4 32.0
 279 3.5 3.0 4.6

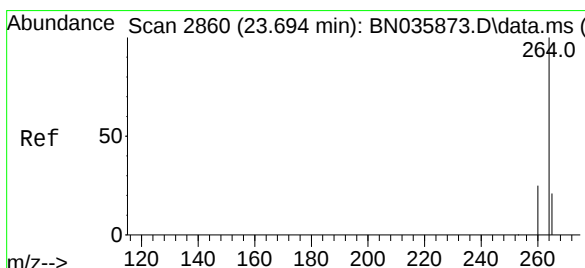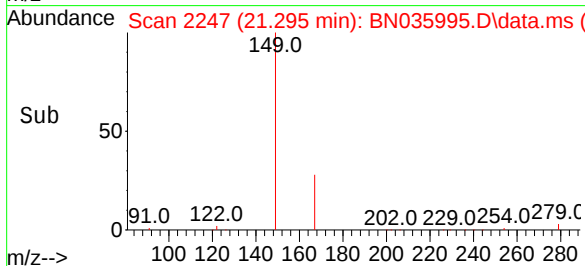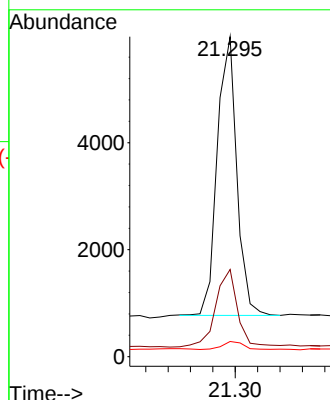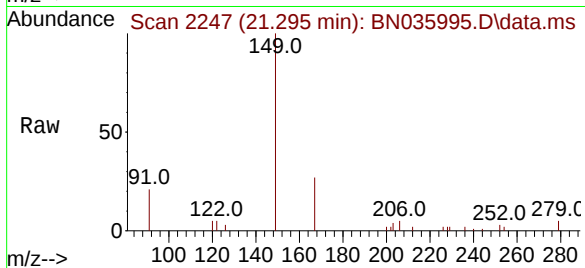

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.663 min Scan# 2801
 Delta R.T. -0.031 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51

Tgt Ion:264 Resp: 5484
 Ion Ratio Lower Upper
 264 100
 260 25.7 21.7 32.5
 265 59.5 33.9 50.9#

