
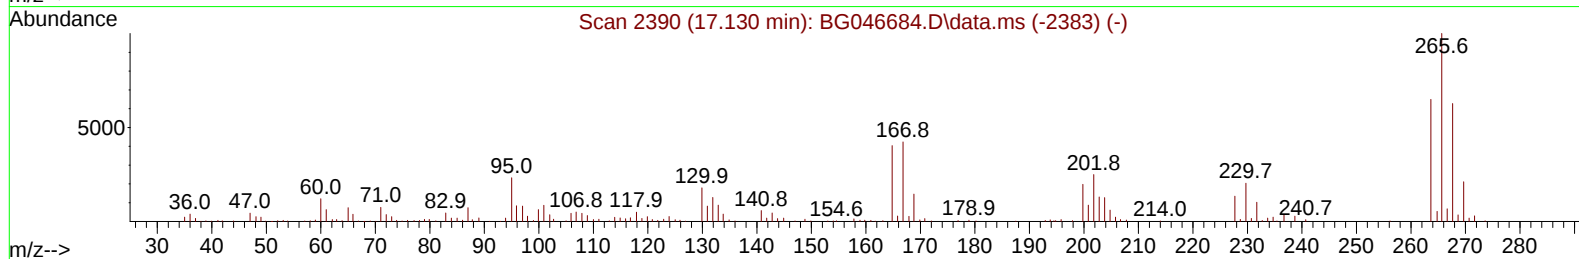
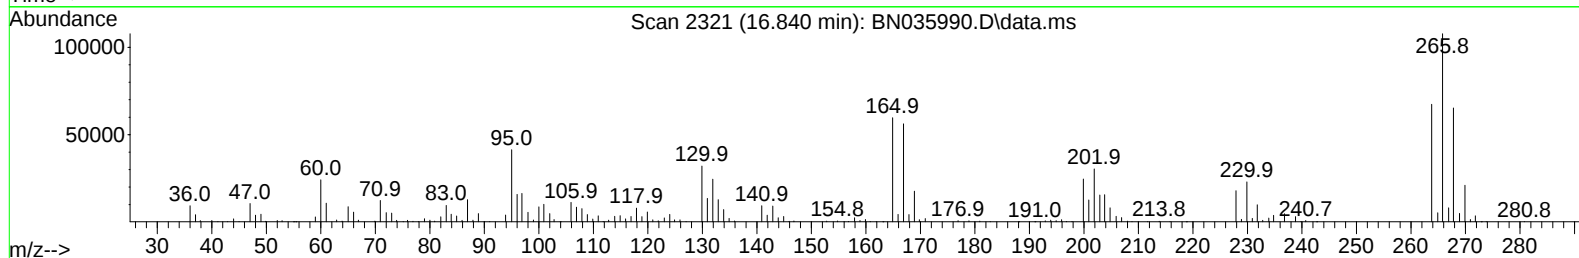


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
Data File : BN035990.D
Acq On : 20 Jan 2025 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 11:00:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

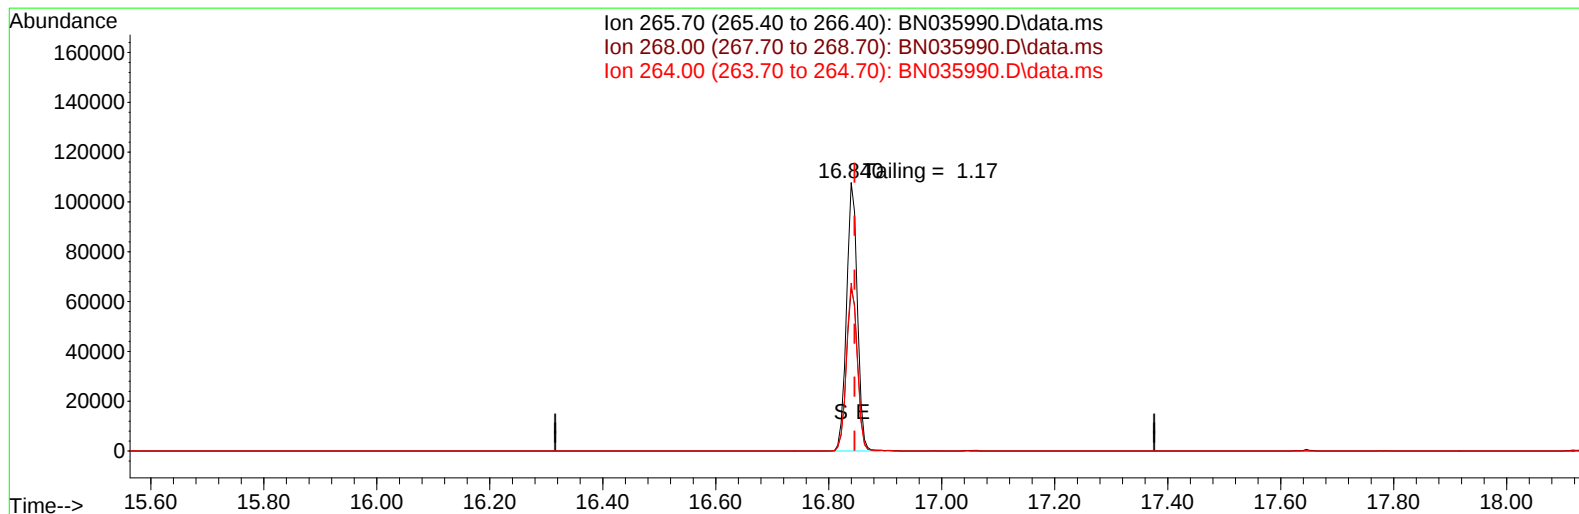

TIC: BN035990.D\data.ms

(70) Pentachlorophenol (C)




16.840min (-0.006) 16779.47 ng

response 143269

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.53
264.00	61.60	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
Data File : BN035990.D
Acq On : 20 Jan 2025 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 11:00:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

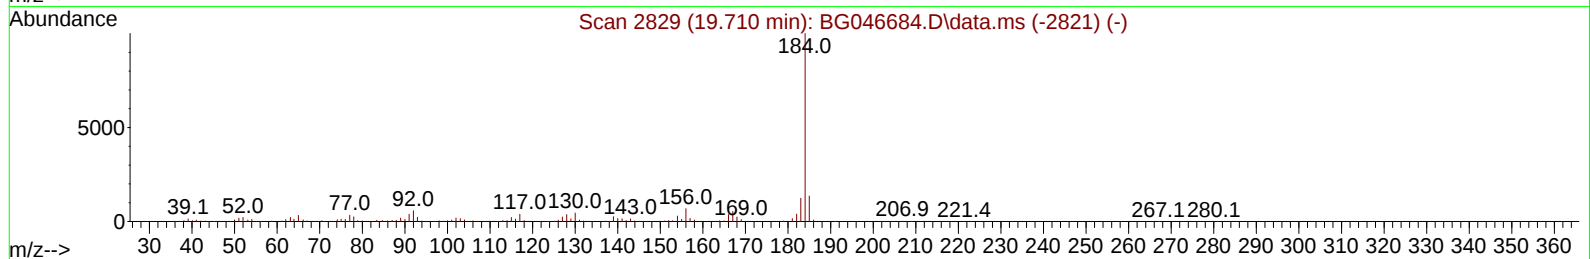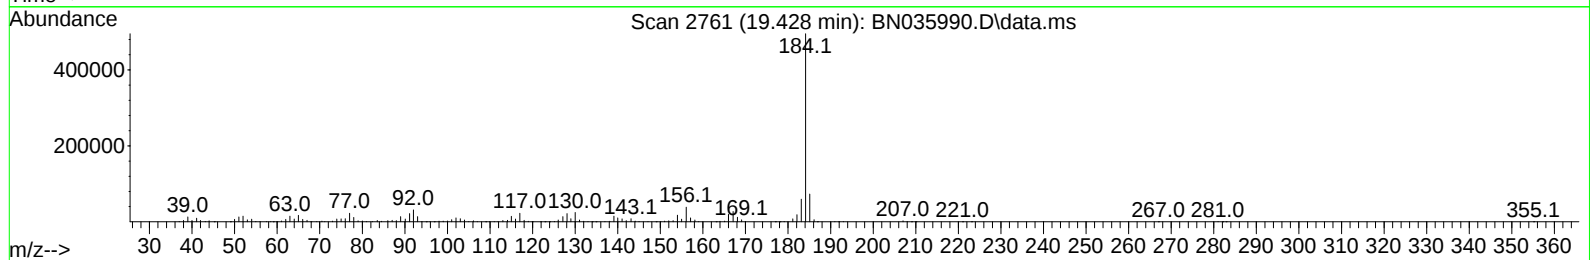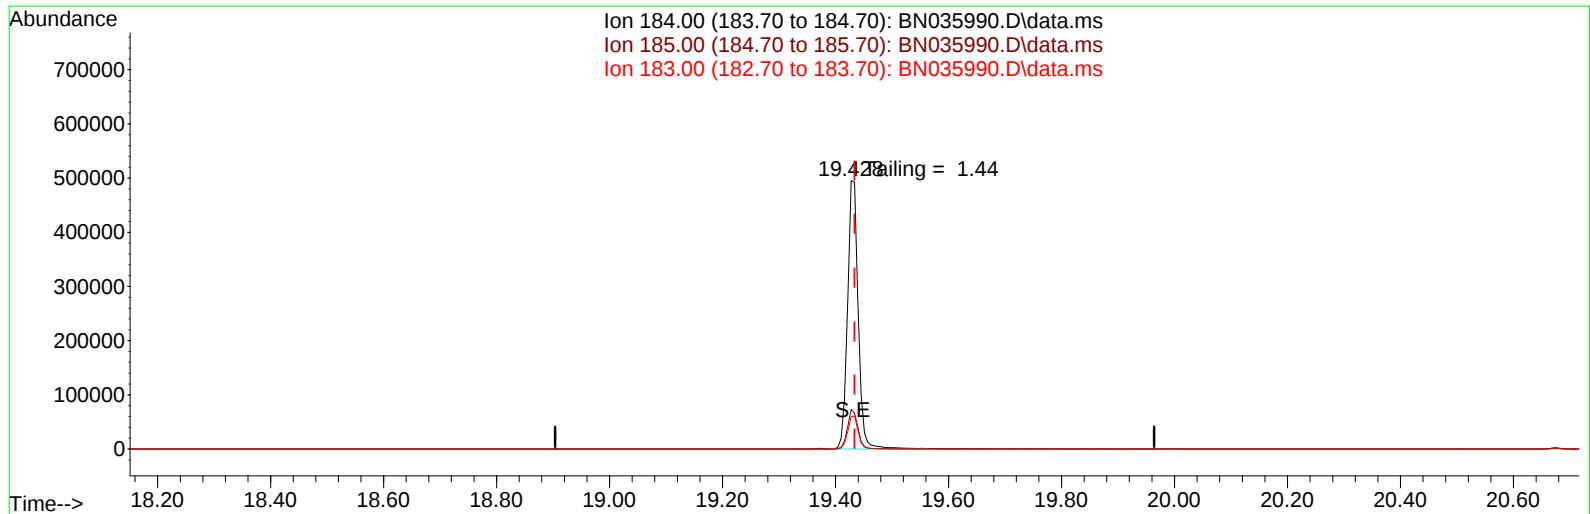

TIC: BN035990.D\data.ms

(77) Benzidine

19.428min (-0.006) 0.00 ng

response 652716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	12.07
0.00	0.00	0.00