

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
 Data File : BN035995.D
 Acq On : 20 Jan 2025 12:51
 Operator : RC/JU
 Sample : Q1113-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DSN002

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/21/2025
 Supervised By :mohammad ahmed 01/21/2025

Quant Time: Jan 20 13:23:40 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 02 15:39:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2567	0.400	ng	-0.02
7) Naphthalene-d8	10.611	136	5127	0.400	ng	#-0.01
13) Acenaphthene-d10	14.452	164	3037	0.400	ng	0.00
19) Phenanthrene-d10	17.186	188	5748	0.400	ng	#-0.02
29) Chrysene-d12	21.367	240	5349	0.400	ng	-0.02
35) Perylene-d12	23.663	264	5484	0.400	ng	#-0.03
System Monitoring Compounds						
4) 2-Fluorophenol	5.398	112	876	0.139	ng	-0.01
5) Phenol-d6	6.972	99	647	0.083	ng	-0.01
8) Nitrobenzene-d5	8.956	82	2155m	0.531	ng	-0.03
11) 2-Methylnaphthalene-d10	12.198	152	2852	0.415	ng	-0.02
14) 2,4,6-Tribromophenol	15.933	330	515	0.353	ng	-0.02
15) 2-Fluorobiphenyl	13.073	172	4348	0.326	ng	-0.02
27) Fluoranthene-d10	19.216	212	7124	0.499	ng	-0.02
31) Terphenyl-d14	19.815	244	5403	0.507	ng	-0.02
Target Compounds						Qvalue
2) 1,4-Dioxane	3.318	88	1795	0.704	ng	# 93
24) Pentachlorophenol	16.839	266	77	0.040	ng	96
34) Bis(2-ethylhexyl)phtha...	21.295	149	6313	0.823	ng	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
Data File : BN035995.D
Acq On : 20 Jan 2025 12:51
Operator : RC/JU
Sample : Q1113-02
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DSN002

Quant Time: Jan 20 13:23:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 15:39:17 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 01/21/2025
Supervised By :mohammad ahmed 01/21/2025

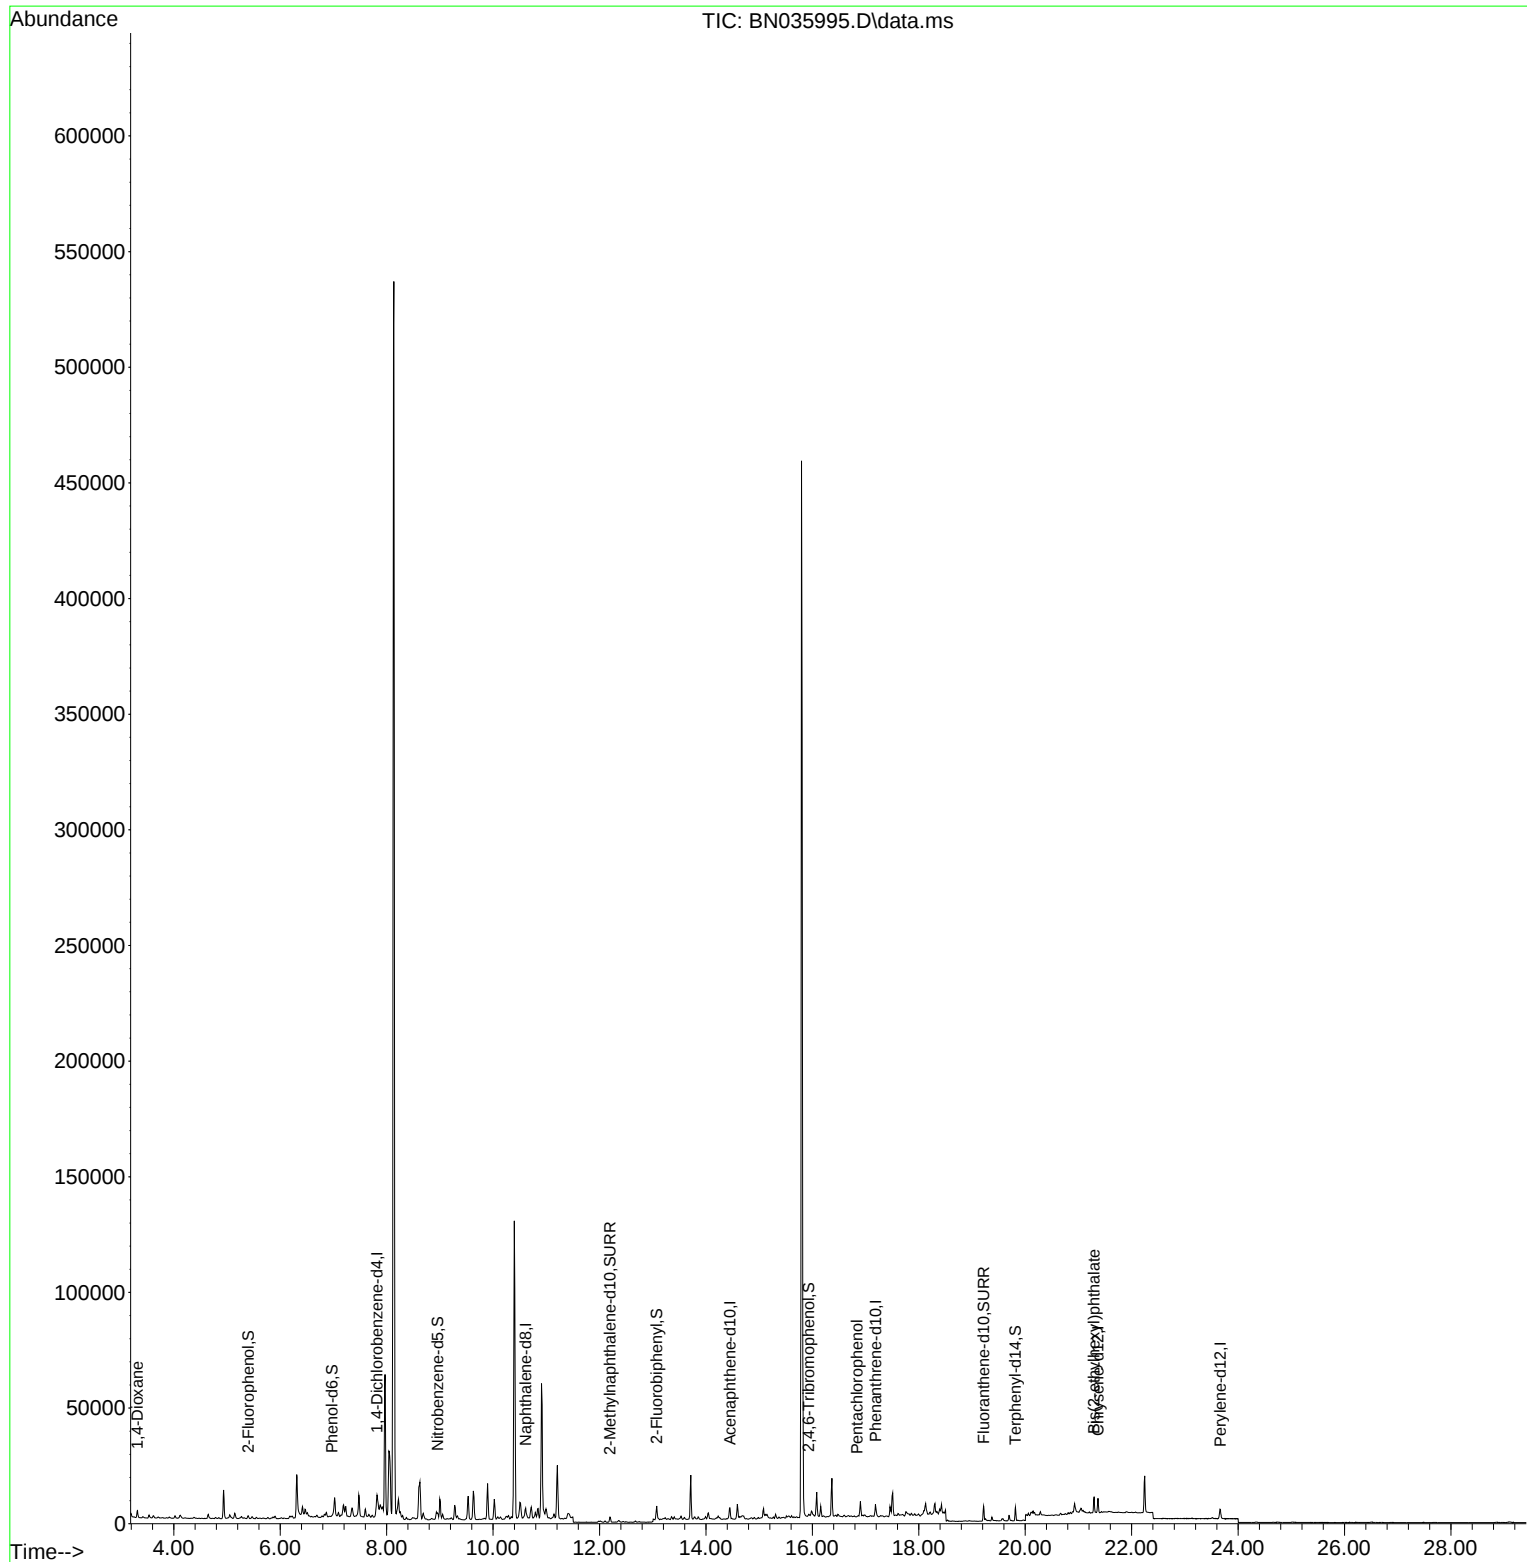



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.817 min Scan# 64
 Delta R.T. -0.019 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51




Instrument :
 BNA_N
 ClientSampleId :
 DSN002




Tgt Ion:152 Resp: 256
 Ion Ratio Lower Upper
 152 100
 150 151.5 117.8 176.6
 115 67.0 51.0 76.4

Manual Integrations
 APPROVED



Reviewed By :Yogesh Patel 01/21/2025
 Supervised By :mohammad ahmed 01/21/2025

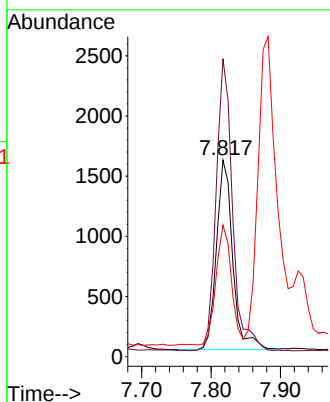


#2
 1,4-Dioxane
 Concen: 0.704 ng
 RT: 3.318 min Scan# 19
 Delta R.T. -0.004 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51



Tgt Ion: 88 Resp: 1795
 Ion Ratio Lower Upper
 88 100
 43 50.8 32.7 49.1#
 58 80.3 63.0 94.4

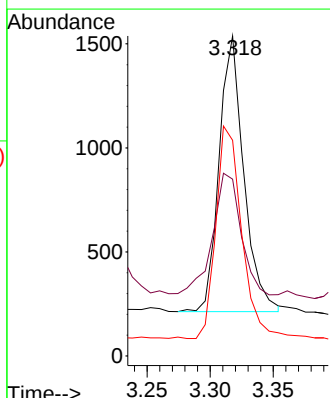







#4
2-Fluorophenol
Concen: 0.139 ng
RT: 5.398 min Scan# 307
Delta R.T. -0.011 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Instrument :
BNA_N
ClientSampleId :
DSN002

Tgt Ion: 112 Resp: 870
Ion Ratio Lower Upper
112 100
64 65.8 48.2 72.2
63 39.4 30.0 45.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 01/21/2025
Supervised By :mohammad ahmed 01/21/2025

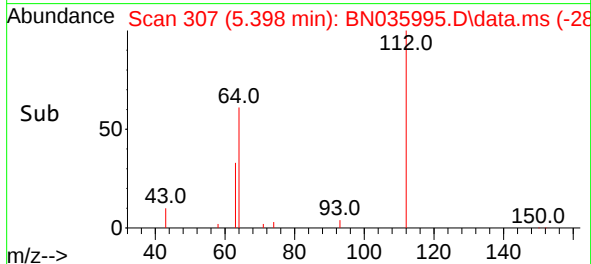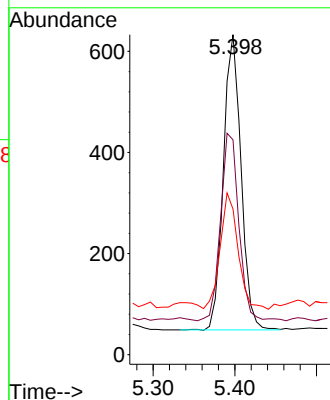

#5
Phenol-d6
Concen: 0.083 ng
RT: 6.972 min Scan# 525
Delta R.T. -0.011 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51


Tgt Ion: 99 Resp: 647
Ion Ratio Lower Upper
99 100
42 0.0 23.5 35.3#
71 39.9 35.5 53.3

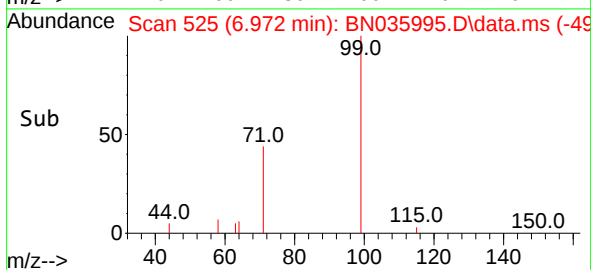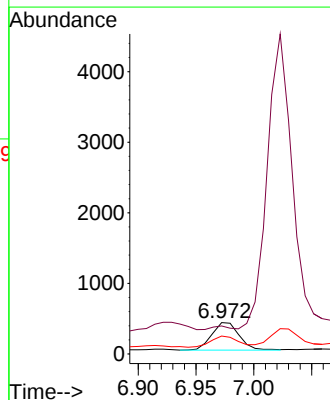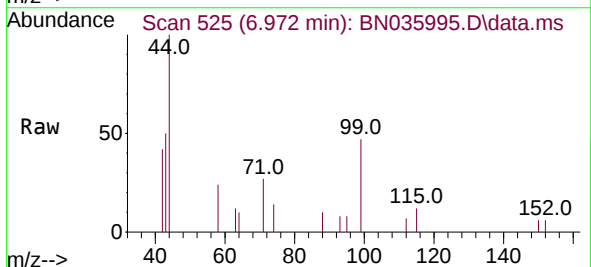



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.611 min Scan# 91
Delta R.T. -0.015 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002



Tgt Ion:136 Resp: 512
Ion Ratio Lower Upper
136 100
137 12.2 10.6 15.8
54 11.4 9.8 14.6
68 13.9 6.6 10.0#




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 01/21/2025
Supervised By :mohammad ahmed 01/21/2025

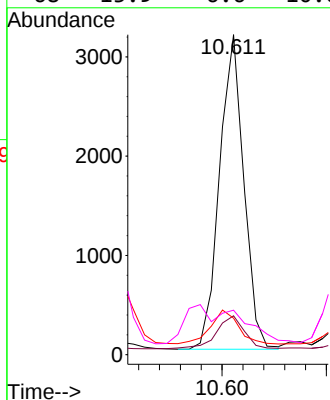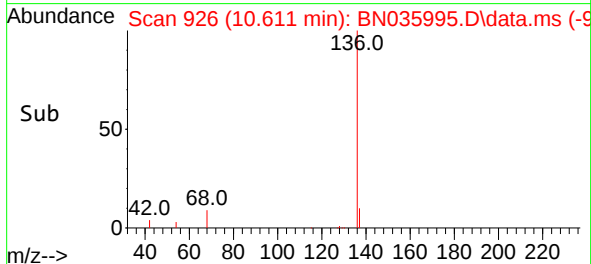

#8
Nitrobenzene-d5
Concen: 0.531 ng m
RT: 8.956 min Scan# 771
Delta R.T. -0.025 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51


Tgt Ion: 82 Resp: 2155
Ion Ratio Lower Upper
82 100
128 32.5 36.9 55.3#
54 68.7 50.4 75.6

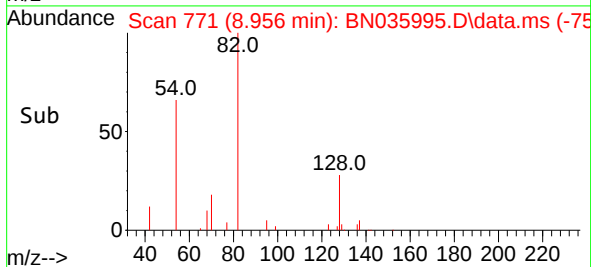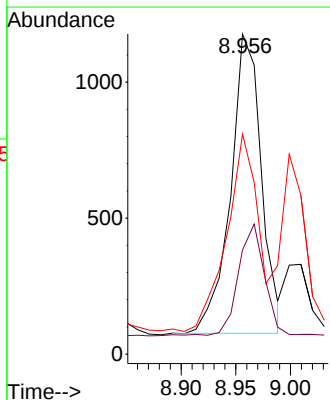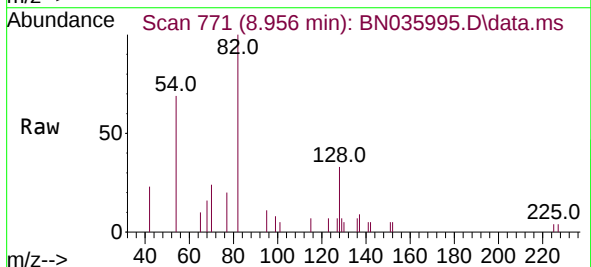



#11
2-Methylnaphthalene-d10
Concen: 0.415 ng
RT: 12.198 min Scan# 1198
Delta R.T. -0.019 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002



Tgt Ion:152 Resp: 2852
Ion Ratio Lower Upper
152 100
151 21.8 17.0 25.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 01/21/2025
Supervised By :mohammad ahmed 01/21/2025

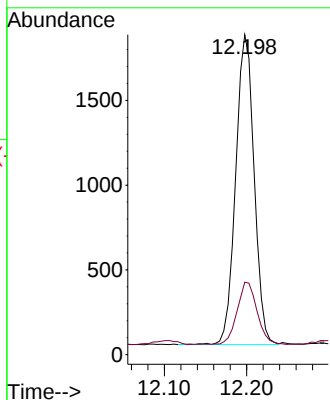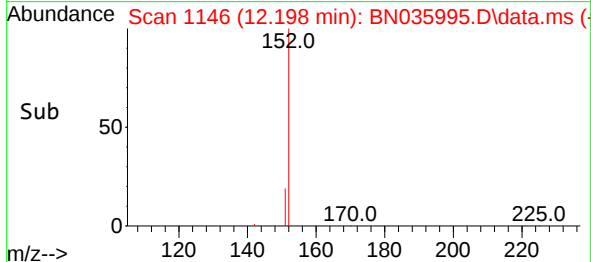

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.452 min Scan# 1441
Delta R.T. -0.010 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51


Tgt Ion:164 Resp: 3037
Ion Ratio Lower Upper
164 100
162 103.0 83.1 124.7
160 49.5 46.0 69.0

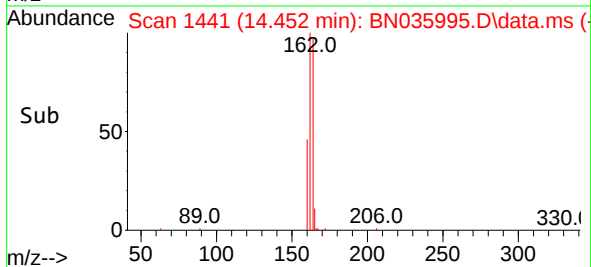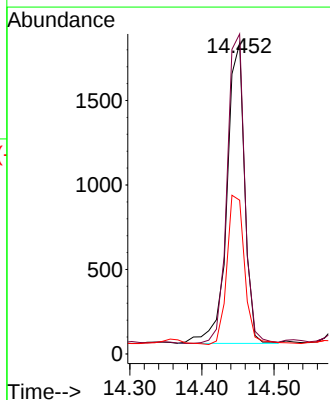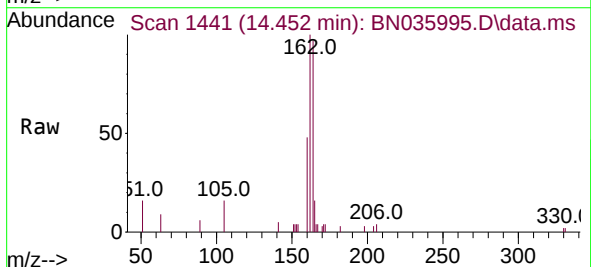



#14
2,4,6-Tribromophenol
Concen: 0.353 ng
RT: 15.933 min Scan# 11
Delta R.T. -0.024 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002




Tgt Ion:330 Resp: 51
Ion Ratio Lower Upper
330 100
332 93.6 77.2 115.8
141 69.5 31.6 47.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 01/21/2025
Supervised By :mohammad ahmed 01/21/2025

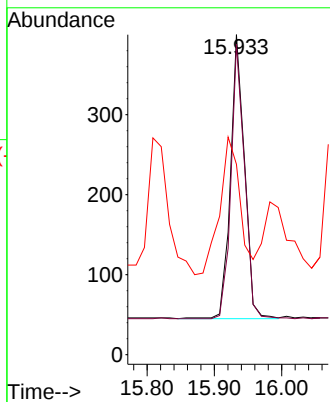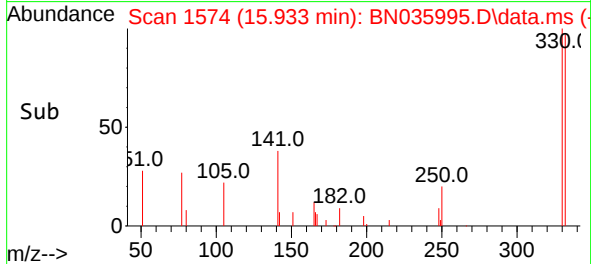


#15
2-Fluorobiphenyl
Concen: 0.326 ng
RT: 13.073 min Scan# 1312
Delta R.T. -0.020 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

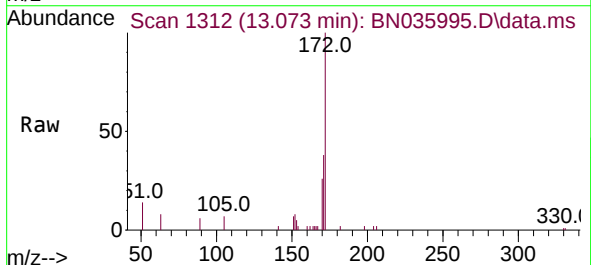

Tgt Ion:172 Resp: 4348
Ion Ratio Lower Upper
172 100
171 37.6 30.5 45.7
170 26.3 20.8 31.2

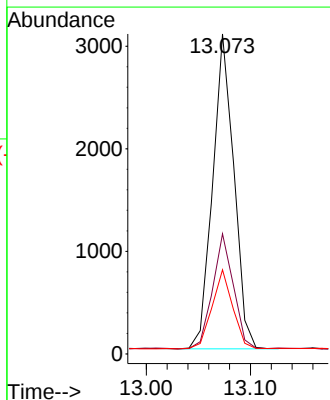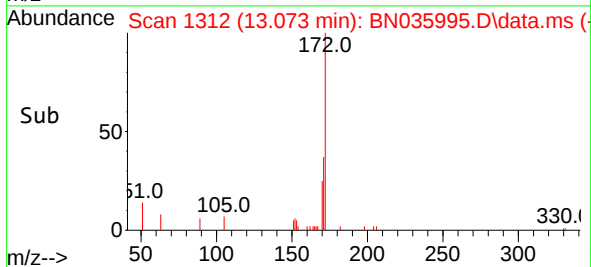

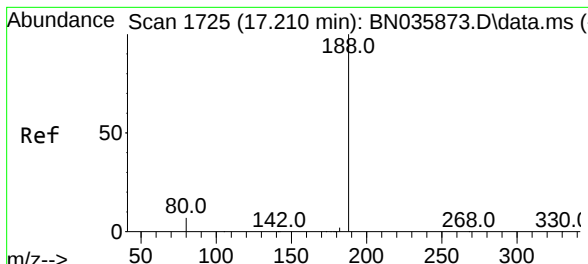

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.186 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51





Instrument : BNA_N
 ClientSampleId : DSN002

Tgt Ion:188 Resp: 574

Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.6	7.3	10.9

Manual Integrations
 APPROVED




Reviewed By :Yogesh Patel 01/21/2025
 Supervised By :mohammad ahmed 01/21/2025

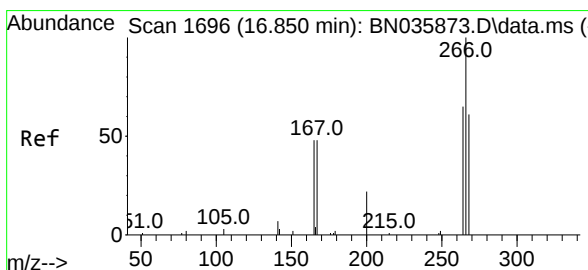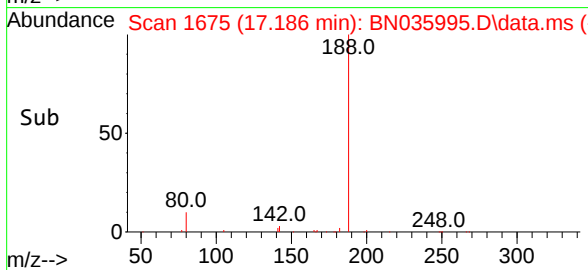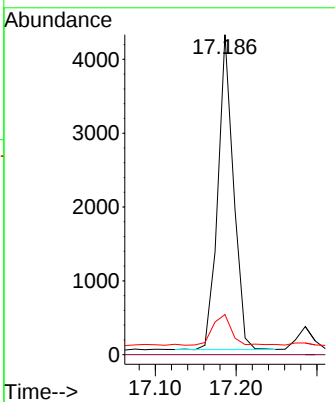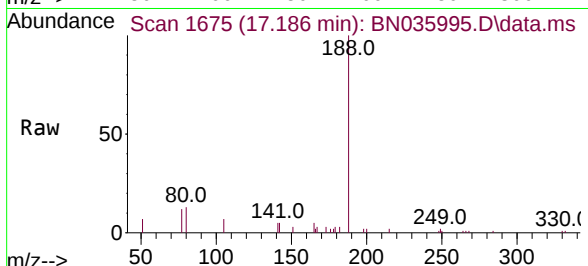


#24
 Pentachlorophenol
 Concen: 0.040 ng
 RT: 16.839 min Scan# 1647
 Delta R.T. -0.011 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51

Tgt Ion:266 Resp: 77


Ion	Ratio	Lower	Upper
266	100		
264	58.4	49.9	74.9
268	61.0	50.2	75.2

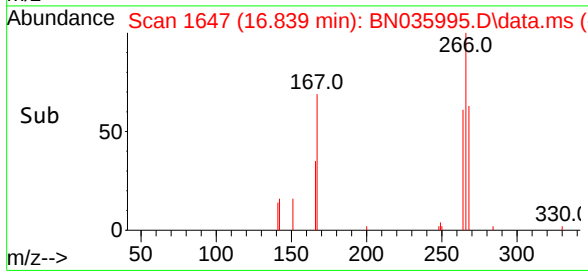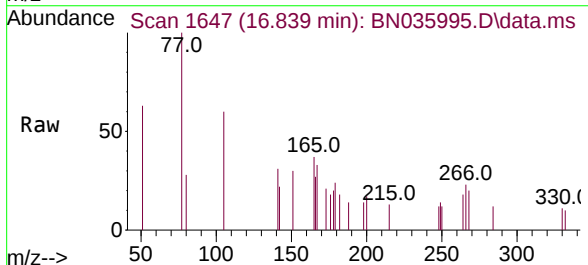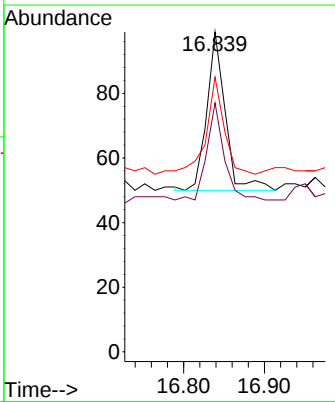



#27
Fluoranthene-d10
Concen: 0.499 ng
RT: 19.216 min Scan# 1924
Delta R.T. -0.022 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51




Instrument :
BNA_N
ClientSampleId :
DSN002




Tgt Ion:212 Resp: 7124
Ion Ratio Lower Upper
212 100
106 12.4 9.0 13.6
104 7.3 5.4 8.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 01/21/2025
Supervised By :mohammad ahmed 01/21/2025

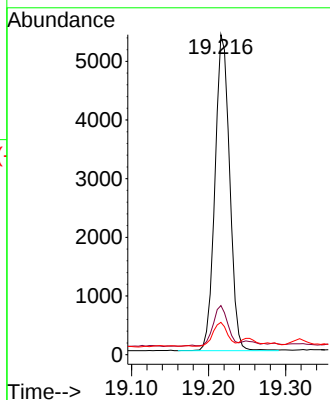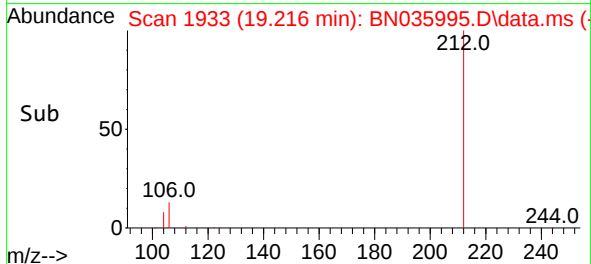


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.367 min Scan# 2255
Delta R.T. -0.017 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

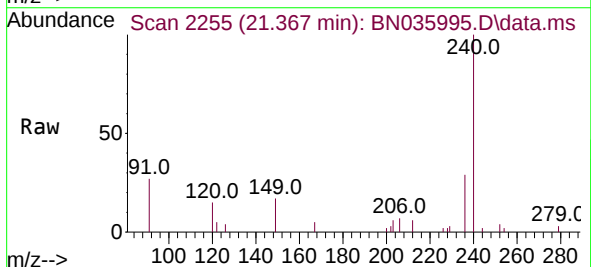


Tgt Ion:240 Resp: 5349
Ion Ratio Lower Upper
240 100
120 15.2 11.1 16.7
236 29.4 24.6 36.8

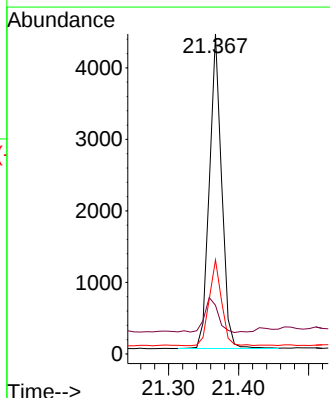



#31
 Terphenyl-d14
 Concen: 0.507 ng
 RT: 19.815 min Scan# 2062
 Delta R.T. -0.022 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51




Instrument :
 BNA_N
 ClientSampleId :
 DSN002



Tgt Ion:244 Resp: 540
 Ion Ratio Lower Upper
 244 100
 212 11.7 10.1 15.1
 122 16.9 12.2 18.4




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 01/21/2025
 Supervised By :mohammad ahmed 01/21/2025

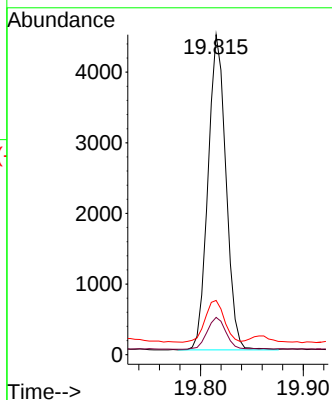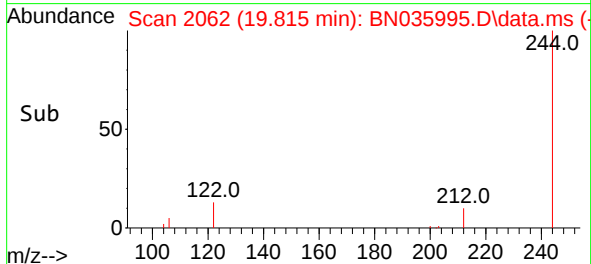

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.823 ng
 RT: 21.295 min Scan# 2247
 Delta R.T. -0.026 min
 Lab File: BN035995.D
 Acq: 20 Jan 2025 12:51


Tgt Ion:149 Resp: 6313
 Ion Ratio Lower Upper
 149 100
 167 31.3 21.4 32.0
 279 3.5 3.0 4.6

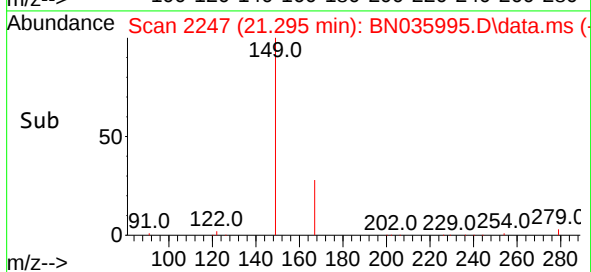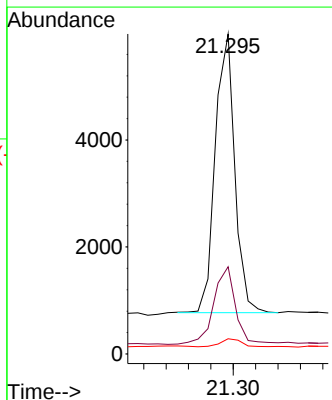

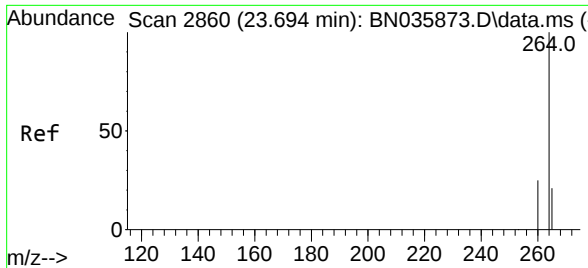

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.663 min Scan# 21
Delta R.T. -0.031 min
Lab File: BN035995.D
Acq: 20 Jan 2025 12:51

Instrument :
BNA_N
ClientSampleId :
DSN002

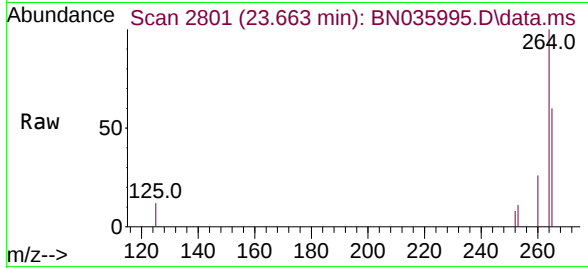

Tgt Ion:264 Resp: 5484
Ion Ratio Lower Upper
264 100
260 25.7 21.7 32.5
265 59.5 33.9 50.9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/21/2025
Supervised By :mohammad ahmed 01/21/2025

