
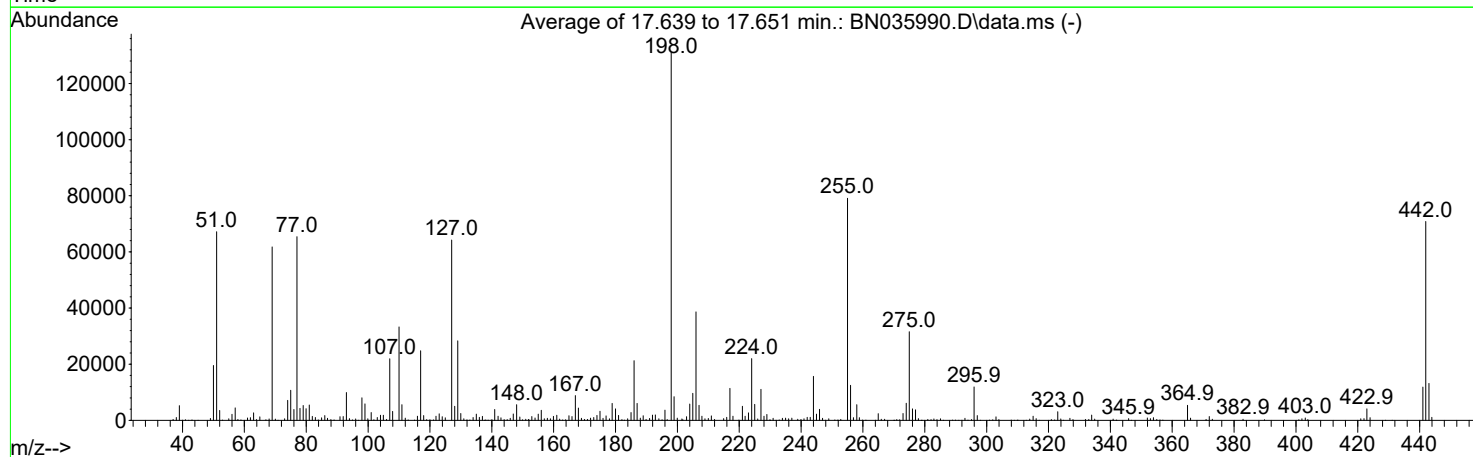


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
Data File : BN035990.D
Acq On : 20 Jan 2025 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 15:39:17 2025

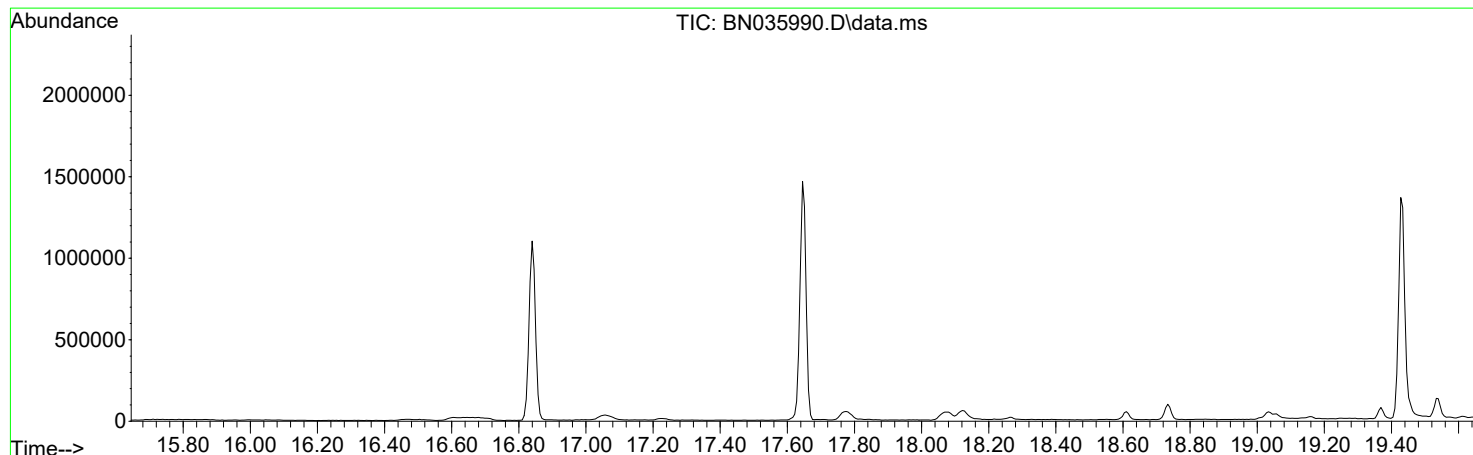

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	67213	PASS
68	69	0.00	2	0.8	492	PASS
69	198	0.00	100	47.1	61771	PASS
70	69	0.00	2	0.7	439	PASS
127	198	10	80	49.0	64256	PASS
197	198	0.00	2	0.2	293	PASS
198	198	100	100	100.0	131045	PASS
199	198	5	9	6.4	8433	PASS
275	198	10	60	24.1	31595	PASS
365	198	1	100	4.1	5388	PASS
441	198	0.01	100	9.1	11885	PASS
442	442	50	100	100.0	70829	PASS
443	442	15	24	18.6	13182	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/20/2025	BNA_N	<u>BN035990.D</u>
Compound Name	Response	Retention Time
DDT	436464	20.675
DDD	13351	20.233
DDE	932	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14283	450747	3.17

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
Data File : BN035990.D
Acq On : 20 Jan 2025 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 20 11:00:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

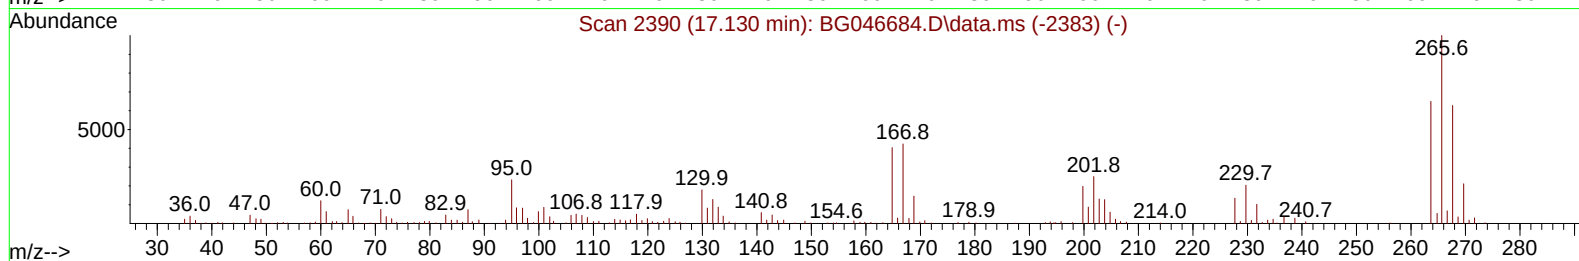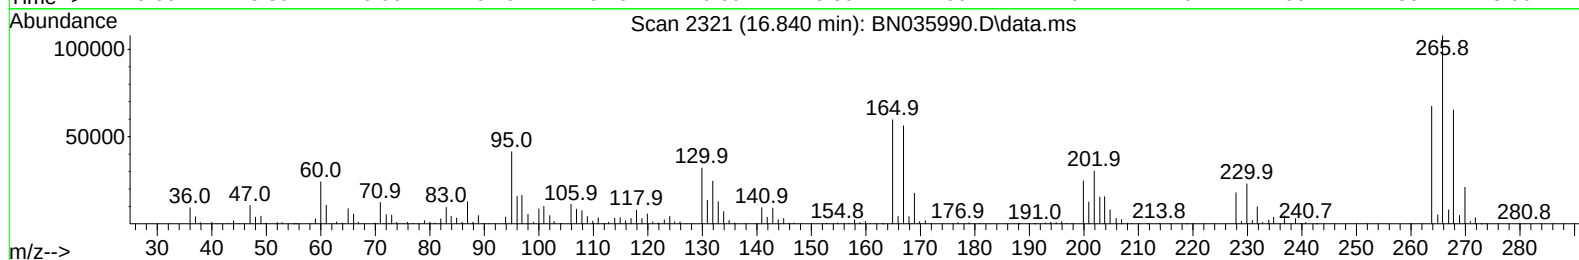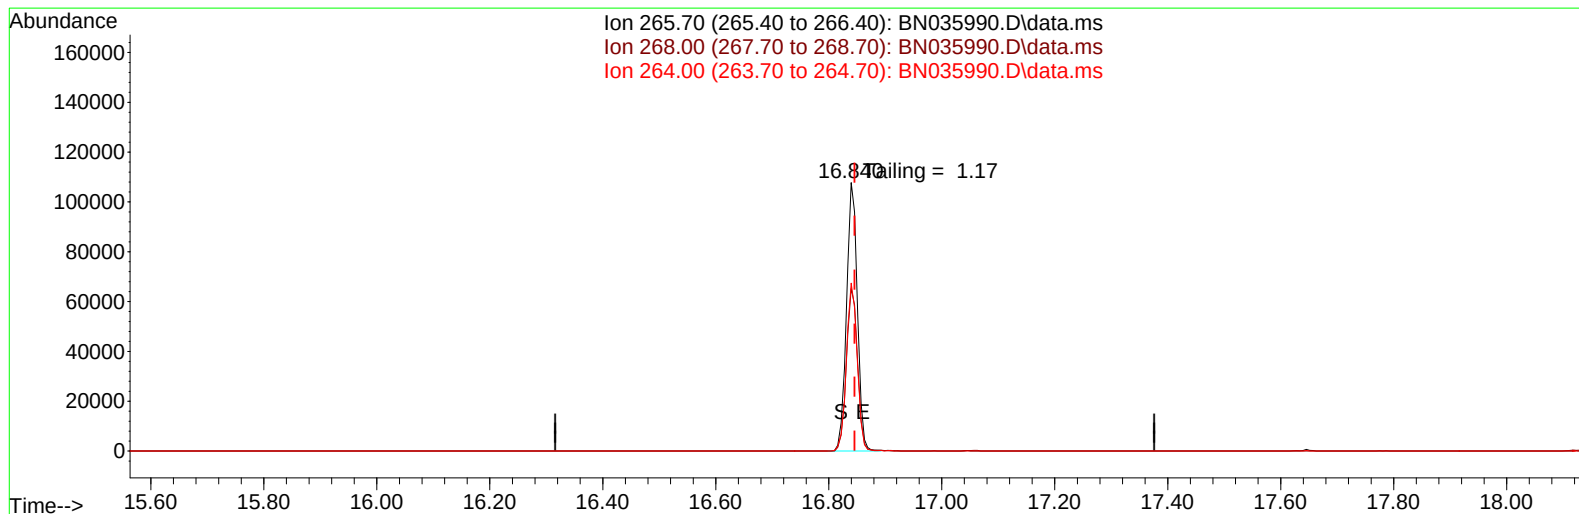

TIC: BN035990.D\data.ms

(70) Pentachlorophenol (C)

16.840min (-0.006) 16779.47 ng




response 143269

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.53
264.00	61.60	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012025\
Data File : BN035990.D
Acq On : 20 Jan 2025 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 20 11:00:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

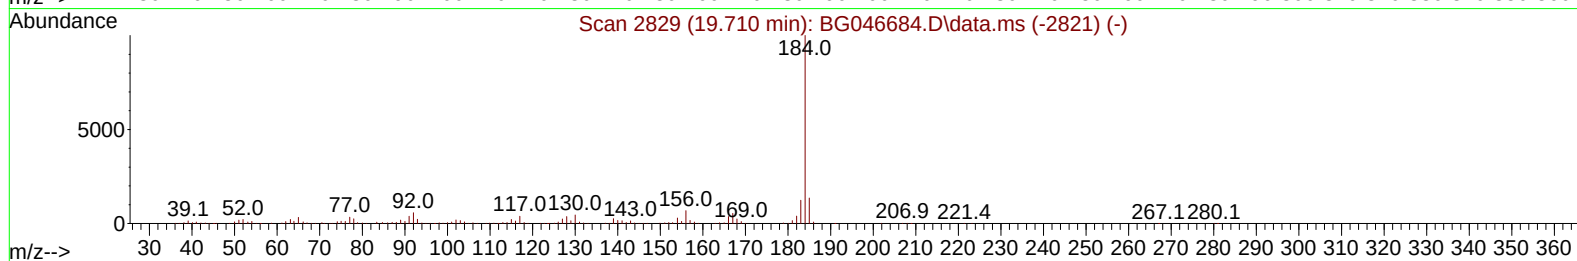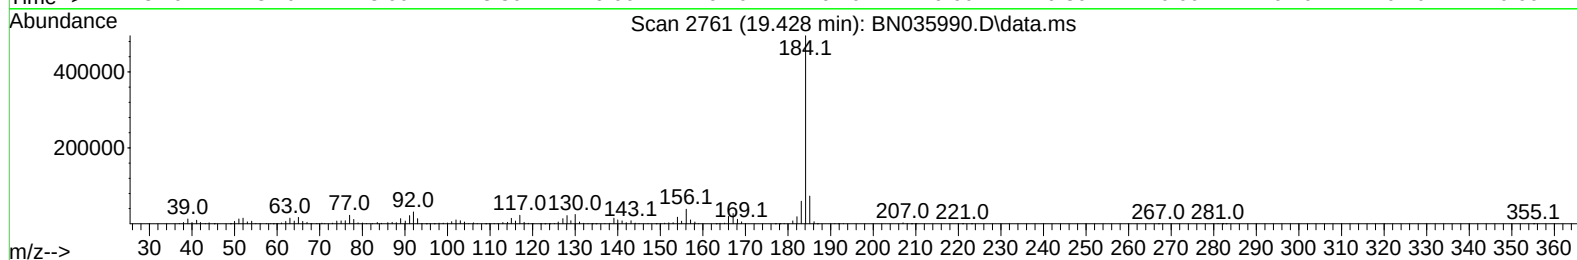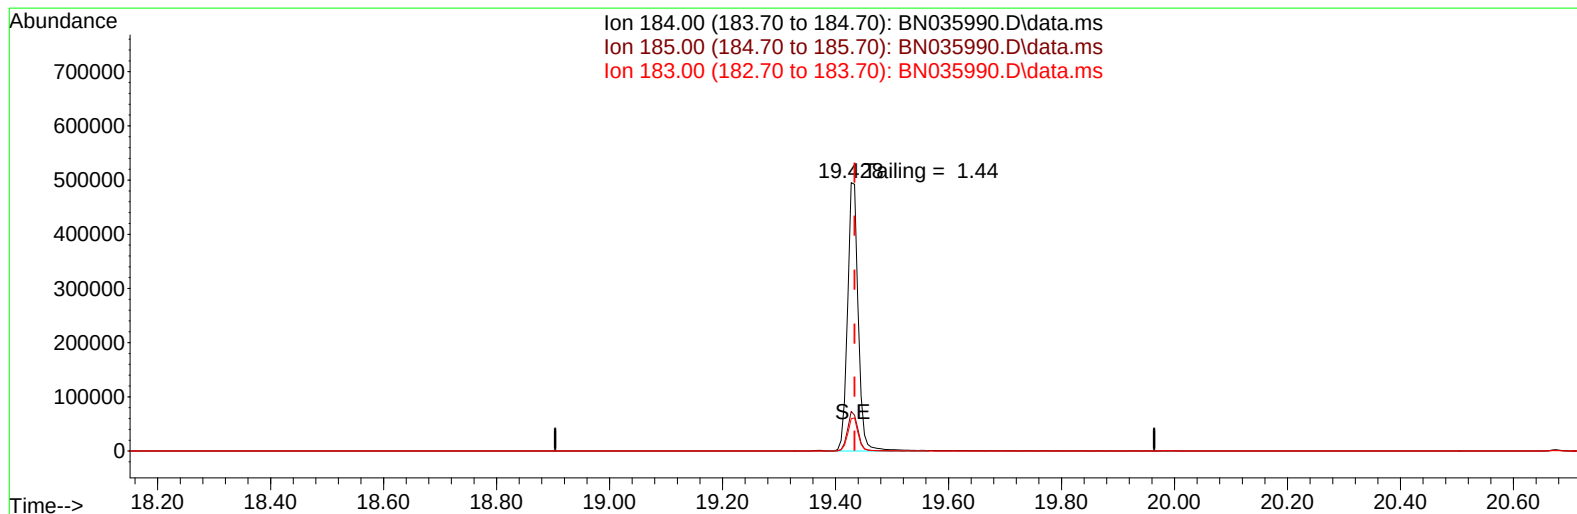

TIC: BN035990.D\data.ms

(77) Benzidine

19.428min (-0.006) 0.00 ng

response 652716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	12.07
0.00	0.00	0.00