

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012120\  
 Data File : BN009409.D  
 Acq On : 21 Jan 2020 11:41  
 Operator : JU  
 Sample : PB125983BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB125983BL

Quant Time: Jan 21 16:10:24 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN011420.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jan 14 09:33:55 2020  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.48  | 152  | 1425     | 0.40 | ng    | 0.00     |
| 7) Naphthalene-d8         | 10.23 | 136  | 4606     | 0.40 | ng    | 0.00     |
| 13) Acenaphthene-d10      | 14.10 | 164  | 3042     | 0.40 | ng    | 0.00     |
| 19) Phenanthrene-d10      | 16.86 | 188  | 6769     | 0.40 | ng    | 0.00     |
| 27) Chrysene-d12          | 21.07 | 240  | 6121     | 0.40 | ng    | 0.00     |
| 34) Perylene-d12          | 23.19 | 264  | 6313     | 0.40 | ng    | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|-----------------------------|-------|------|----------|------|-------|----------|
| 4) 2-Fluorophenol           | 5.12  | 112  | 968      | 0.30 | ng    | 0.00     |
| 5) Phenol-d6                | 6.68  | 99   | 1156     | 0.30 | ng    | 0.00     |
| 8) Nitrobenzene-d5          | 8.64  | 82   | 1032     | 0.28 | ng    | 0.01     |
| 11) 2-Methylnaphthalene-d10 | 11.83 | 152  | 2369     | 0.27 | ng    | 0.00     |
| 14) 2,4,6-Tribromophenol    | 15.62 | 330  | 276      | 0.24 | ng    | 0.00     |
| 15) 2-Fluorobiphenyl        | 12.72 | 172  | 3613     | 0.32 | ng    | 0.00     |
| 25) Fluoranthene-d10        | 18.90 | 212  | 6418     | 0.28 | ng    | 0.00     |
| 29) Terphenyl-d14           | 19.51 | 244  | 4783     | 0.33 | ng    | 0.00     |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012120\  
Data File : BN009409.D  
Acq On : 21 Jan 2020 11:41  
Operator : JU  
Sample : PB125983BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
PB125983BL

Quant Time: Jan 21 16:10:24 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN011420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 14 09:33:55 2020  
Response via : Initial Calibration

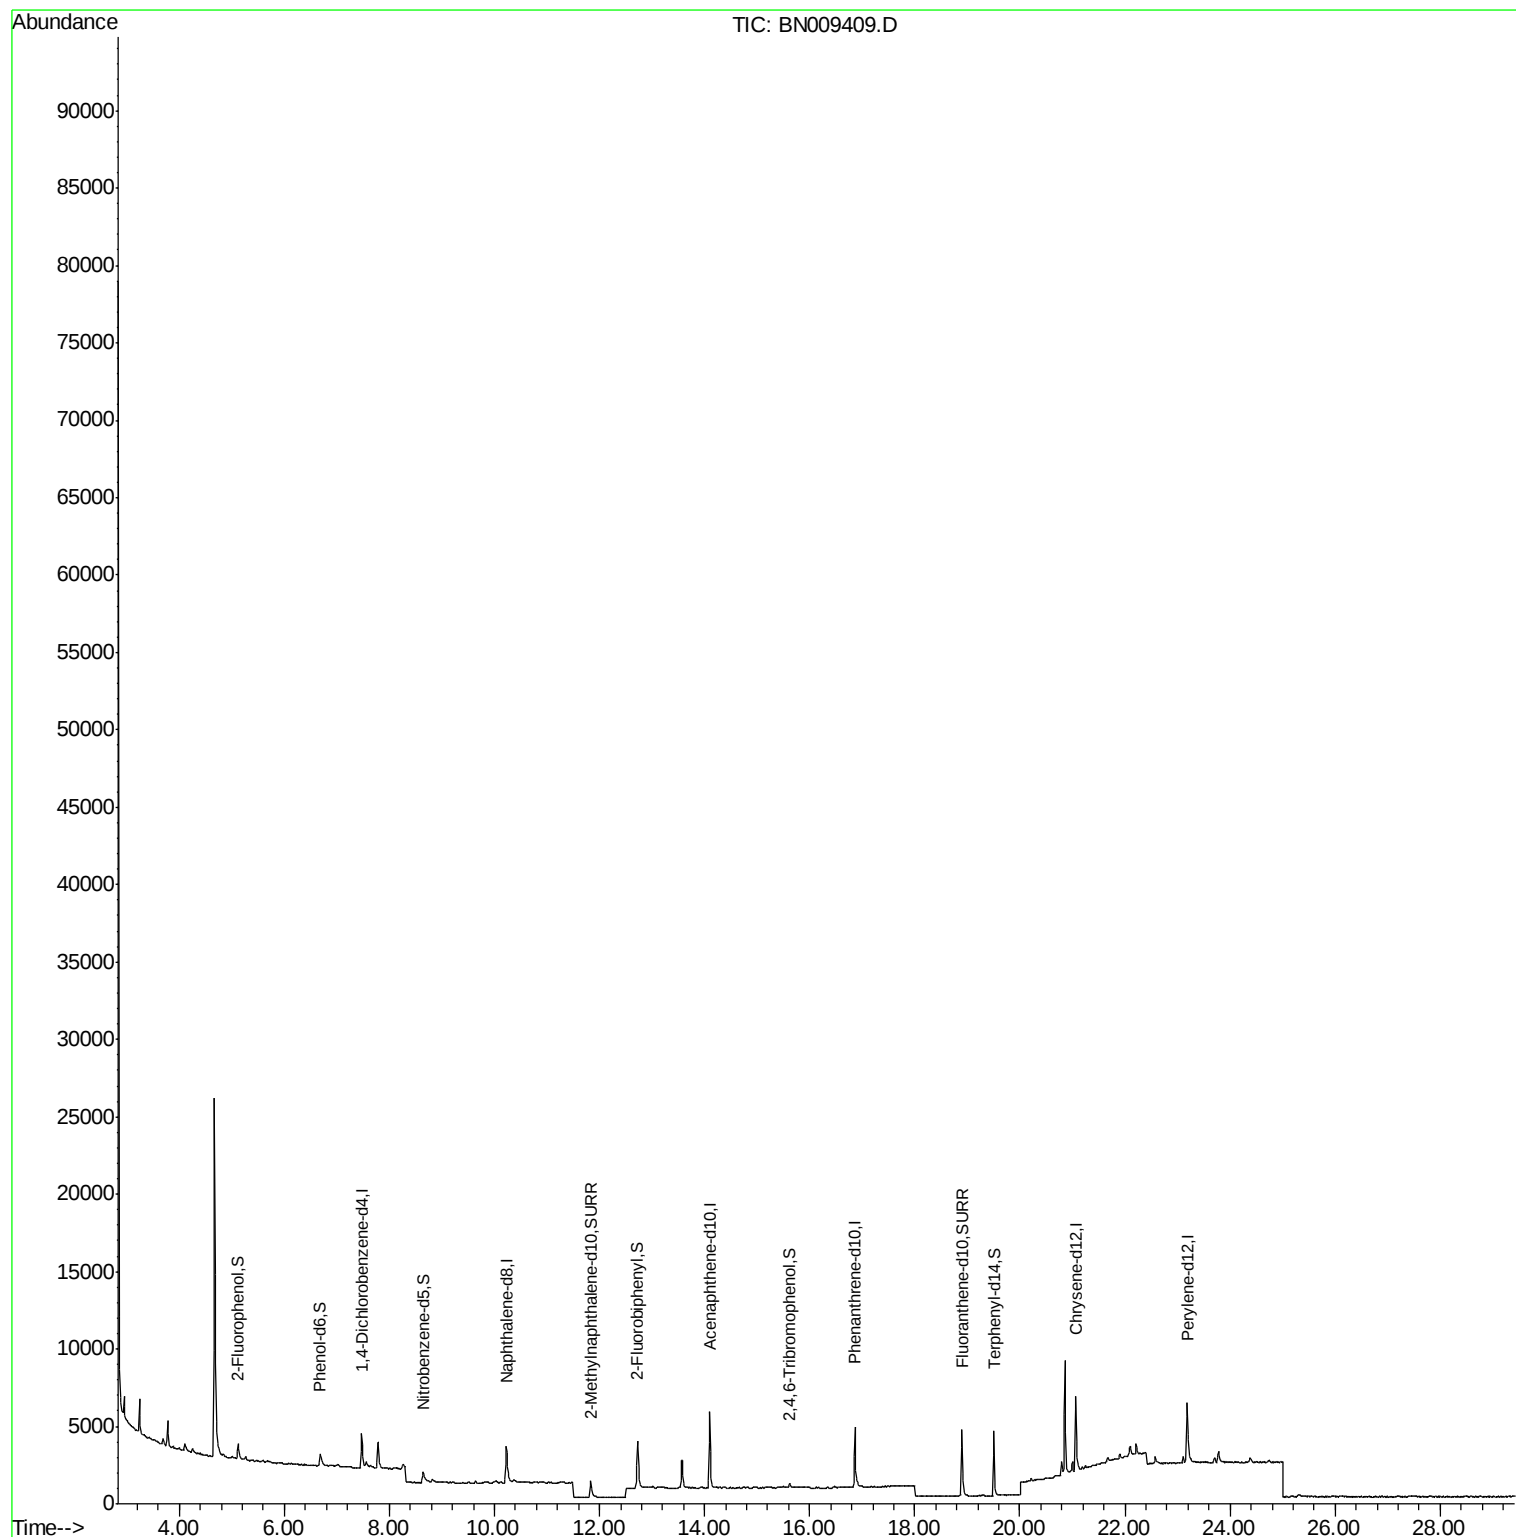




#1




1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.48 min Scan# 577  
Delta R.T. -0.00 min  
Lab File: BN009409.D  
Acq: 21 Jan 2020 11:41

Instrument :  
BNA\_N  
ClientSampleId :  
PB125983BL

Tot Ion:152 Resp: 1425  
Ion Ratio Lower Upper  
152 100  
150 148.9 125.7 188.5  
115 63.1 53.3 79.9

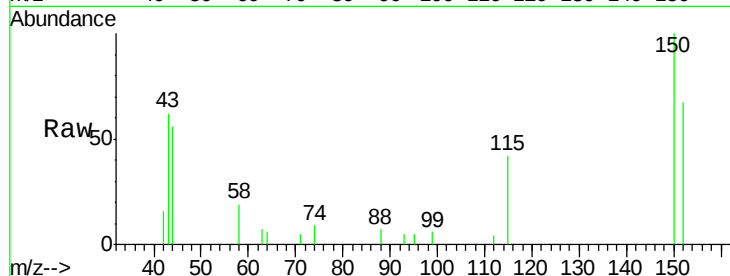


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

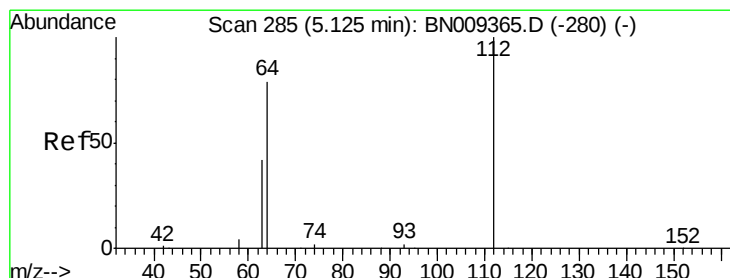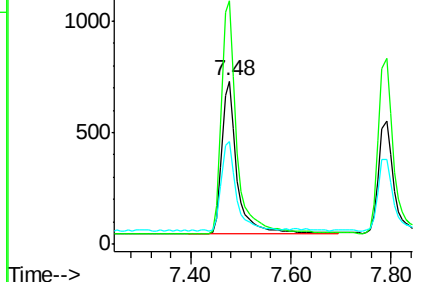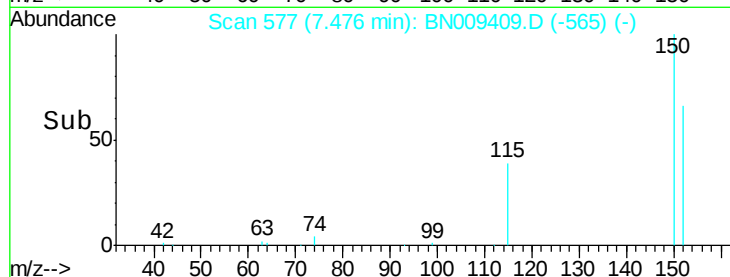



#4


2-Fluorophenol  
Concen: 0.295 ng  
RT: 5.12 min Scan# 285  
Delta R.T. -0.00 min  
Lab File: BN009409.D  
Acq: 21 Jan 2020 11:41

Tgt Ion:112 Resp: 968  
Ion Ratio Lower Upper  
112 100  
64 78.1 61.5 92.3  
63 43.5 35.0 52.4

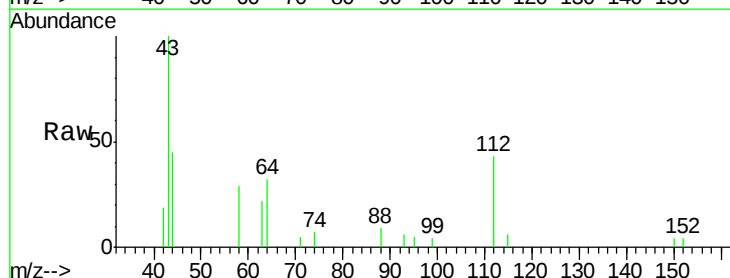

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BNC  
Ion 63.00 (62.70 to 63.70): BNC

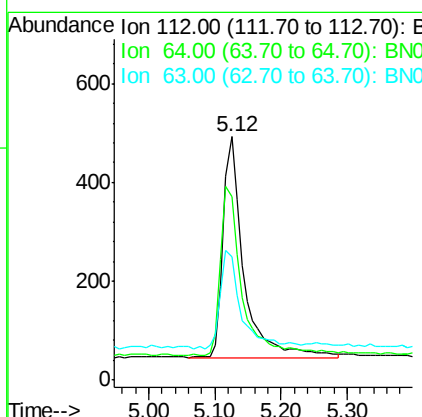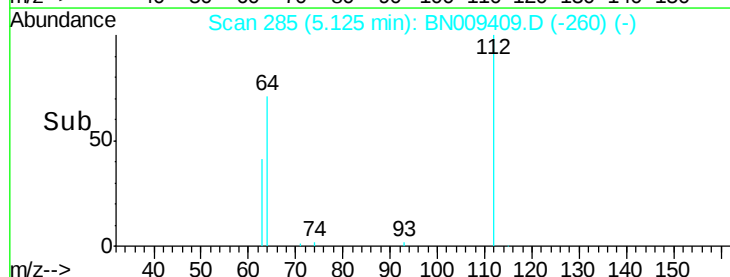

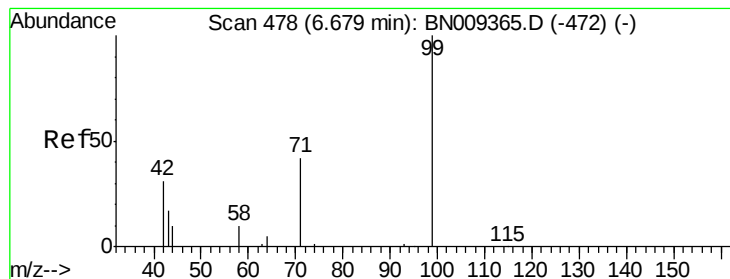

#5

Phenol-d6

Concen: 0.305 ng

RT: 6.68 min Scan# 478

Delta R.T. -0.00 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41

Instrument :

BNA\_N

ClientSampleId :

PB125983BL


Tot Ion: 99 Resp: 1156

Ion Ratio Lower Upper


99 100

42 31.8 27.6 41.4



71 42.8 33.0 49.6

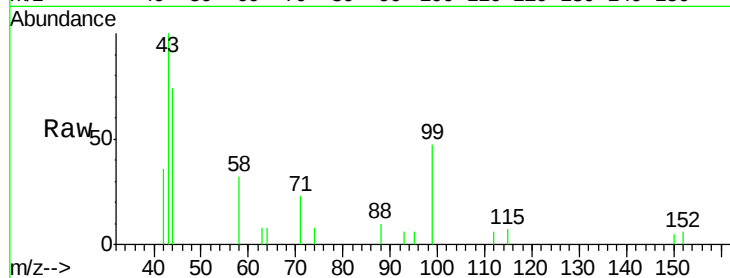

Abundance Ion 99.00 (98.70 to 99.70): BN009409.D (-466) (-)

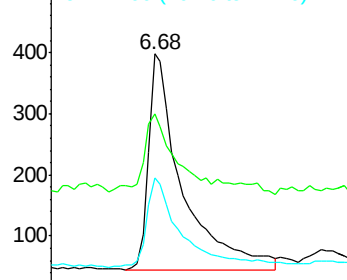

Time-->

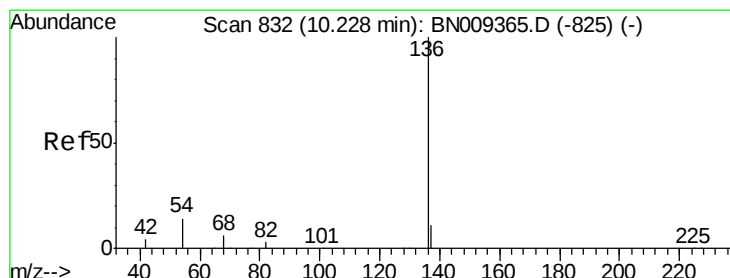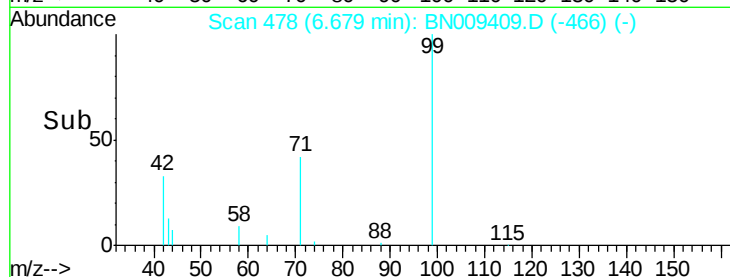

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.23 min Scan# 832

Delta R.T. -0.00 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41

Tgt Ion: 136 Resp: 4606


Ion Ratio Lower Upper

136 100


137 13.2 10.3 15.5

54 18.4 12.6 19.0


68 9.7 6.5 9.7

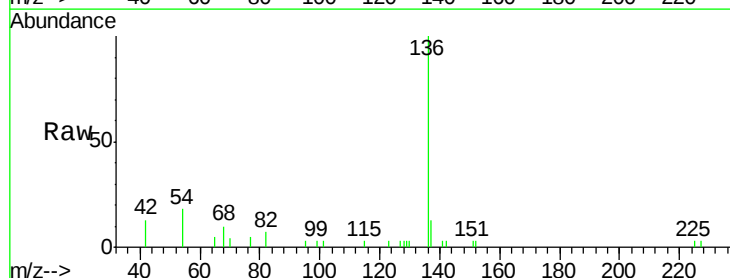


Abundance Ion 136.00 (135.70 to 136.70): BN009409.D (-816) (-)

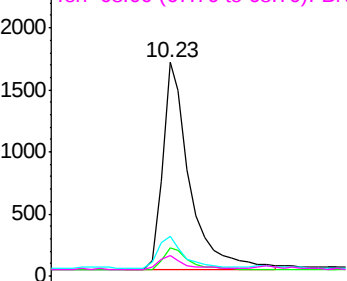

Time-->

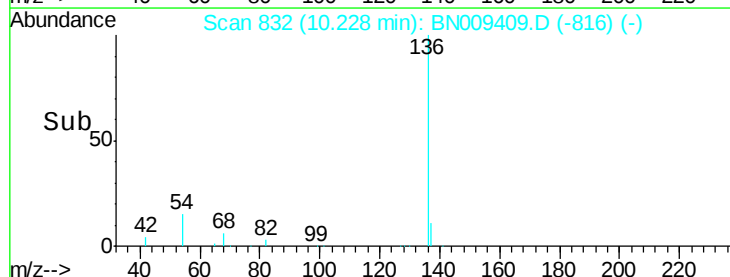

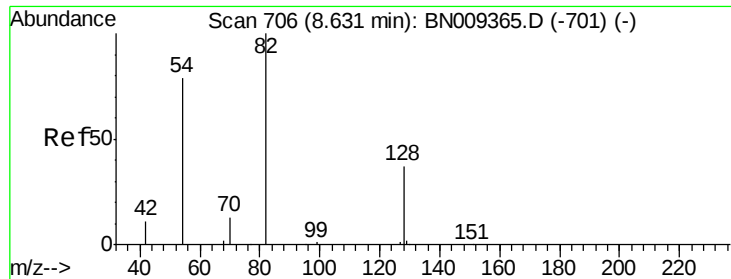

#8

Nitrobenzene-d5

Concen: 0.281 ng

RT: 8.64 min Scan# 707

Delta R.T. 0.01 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41

Instrument :

BNA\_N

ClientSampleId :

PB125983BL


Tot Ion: 82 Resp: 1032

Ion Ratio Lower Upper

82 100

128 46.1 34.8 52.2




54 86.7 65.8 98.6

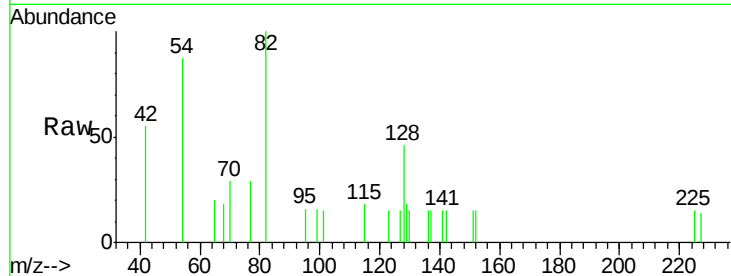

Abundance Ion 82.00 (81.70 to 82.70): BN009409.D (-698) (-)

Ion 128.00 (127.70 to 128.70): BN009409.D (-698) (-)

Ion 54.00 (53.70 to 54.70): BN009409.D (-698) (-)

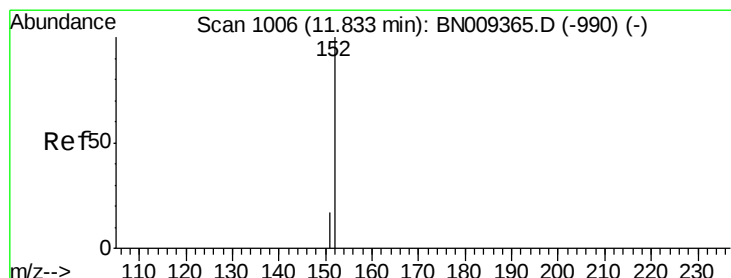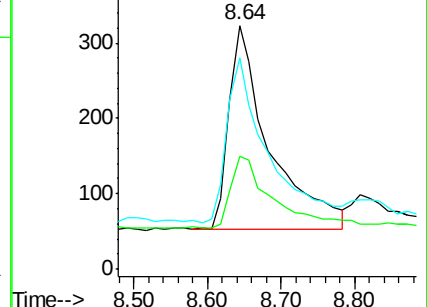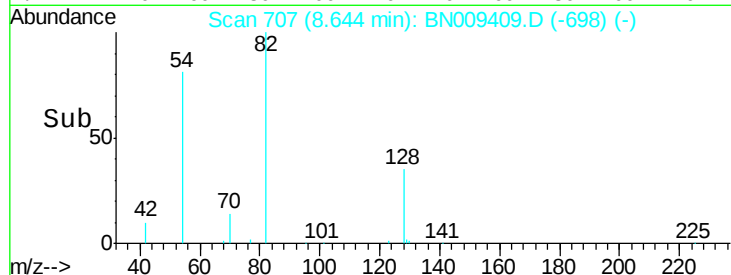

#11

2-Methylnaphthalene-d10

Concen: 0.266 ng

RT: 11.83 min Scan# 1006

Delta R.T. -0.00 min

Lab File: BN009409.D


Acq: 21 Jan 2020 11:41

Tgt Ion: 152 Resp: 2369

Ion Ratio Lower Upper



152 100


151 19.1 14.8 22.2

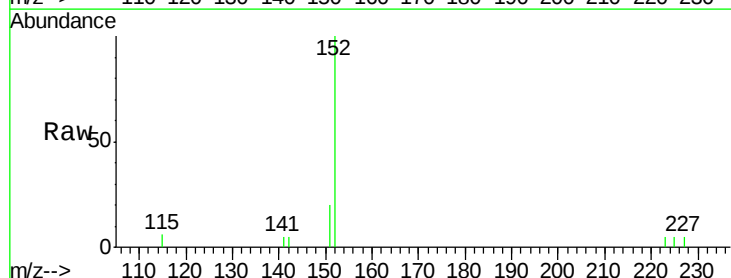

Abundance Ion 152.00 (151.70 to 152.70): BN009409.D (-961) (-)

Ion 151.00 (150.70 to 151.70): BN009409.D (-961) (-)

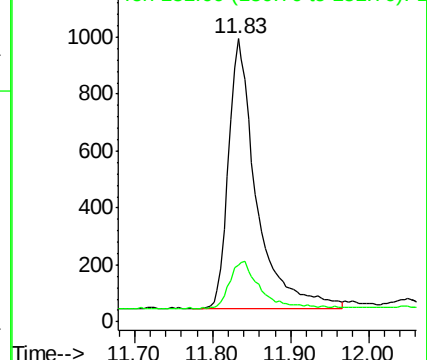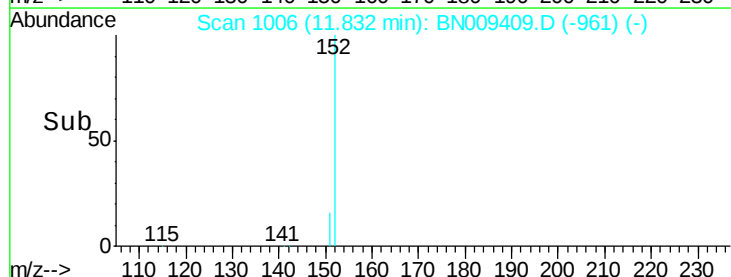

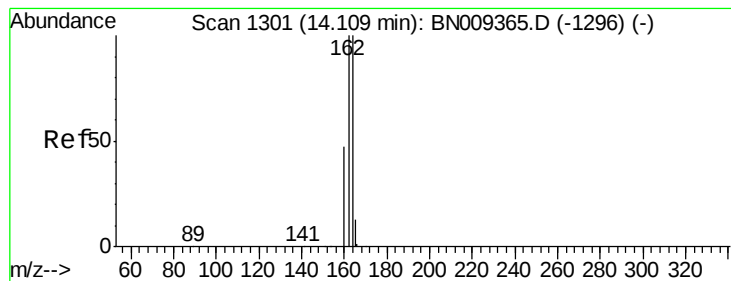

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.10 min Scan# 1301

Delta R.T. -0.01 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41

Instrument :

BNA\_N

ClientSampleId :

PB125983BL


Tot Ion:164 Resp: 3042

Ion Ratio Lower Upper

164 100

162 99.6 79.8 119.6




160 47.0 38.4 57.6

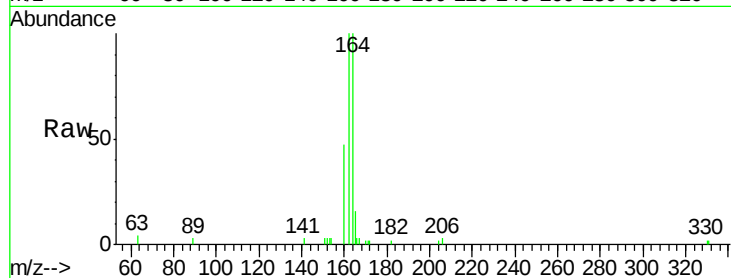

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

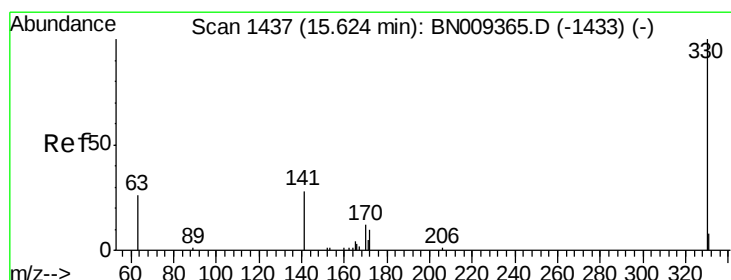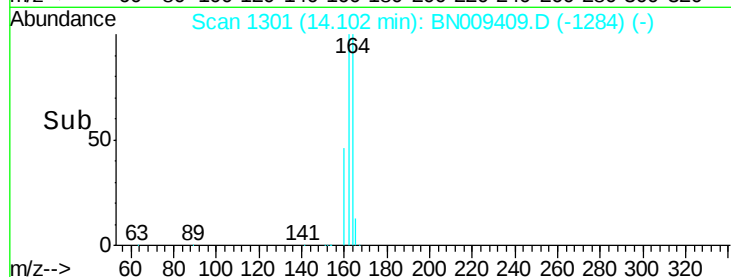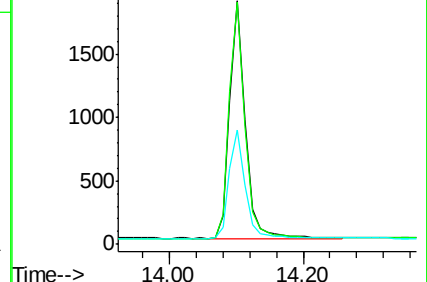

#14

2,4,6-Tribromophenol

Concen: 0.240 ng

RT: 15.62 min Scan# 1437

Delta R.T. -0.01 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41


Tgt Ion:330 Resp: 276

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 48.6 33.1 49.7

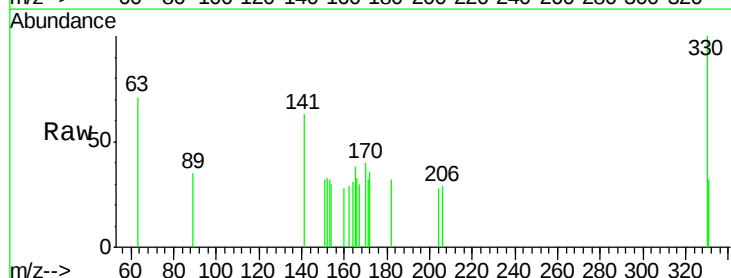


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



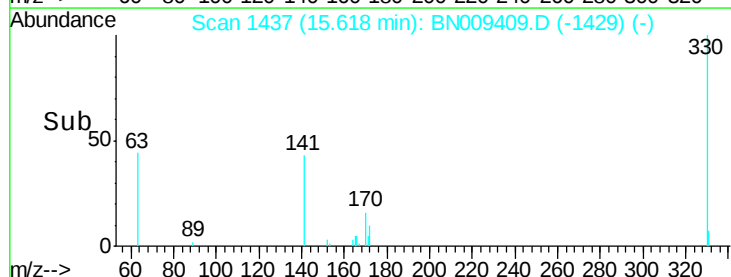
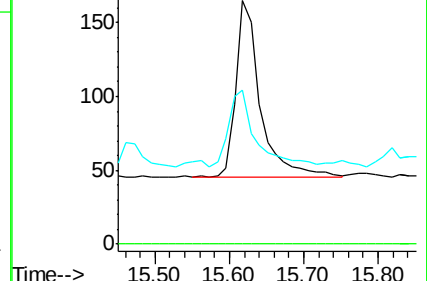


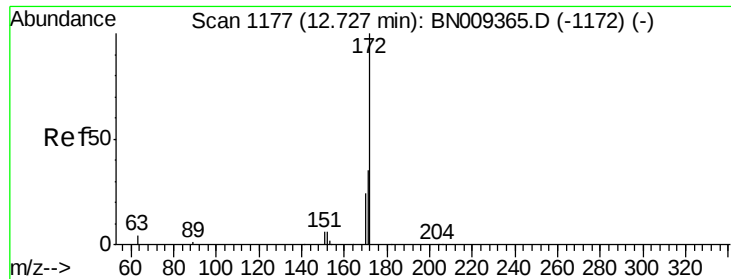

#15  
2-Fluorobiphenyl  
Concen: 0.317 ng  
RT: 12.72 min Scan# 1177  
Delta R.T. -0.01 min  
Lab File: BN009409.D  
Acq: 21 Jan 2020 11:41




Instrument :  
BNA\_N  
ClientSampleId :  
PB125983BL


Tot Ion:172 Resp: 3613  
Ion Ratio Lower Upper  
172 100  
171 36.6 29.5 44.3  
170 24.5 20.7 31.1

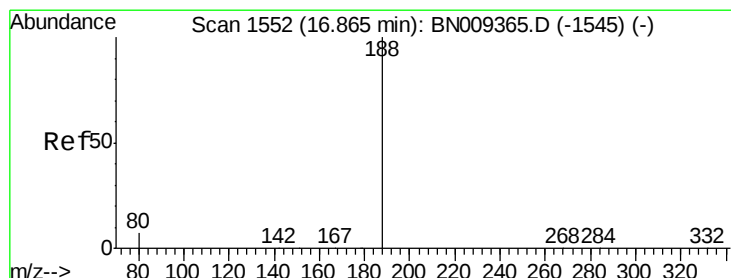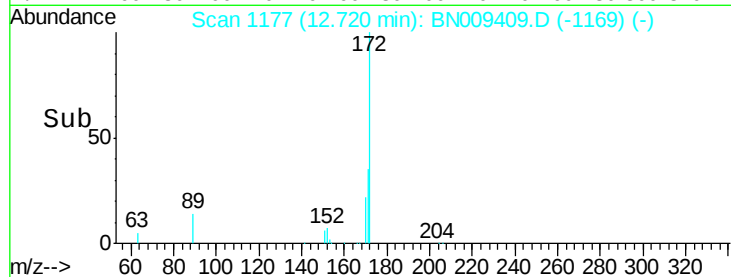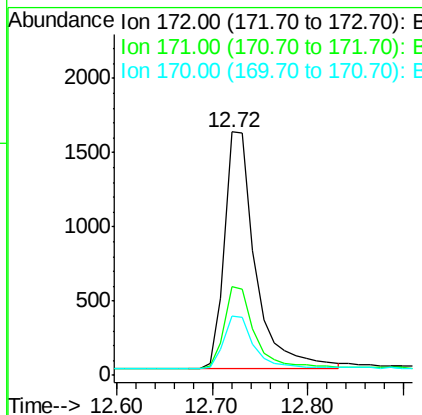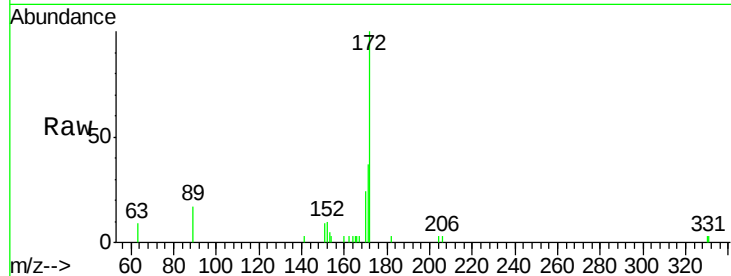

#19  
Phenanthrene-d10  
Concen: 0.400 ng  
RT: 16.86 min Scan# 1552  
Delta R.T. -0.01 min  
Lab File: BN009409.D  
Acq: 21 Jan 2020 11:41

Tgt Ion:188 Resp: 6769  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 11.7 6.6 10.0#

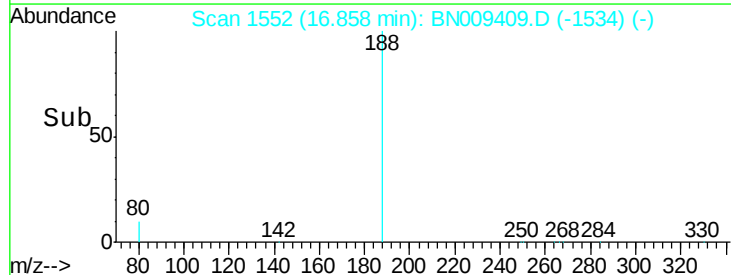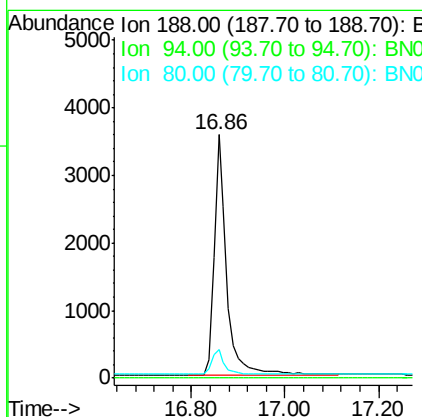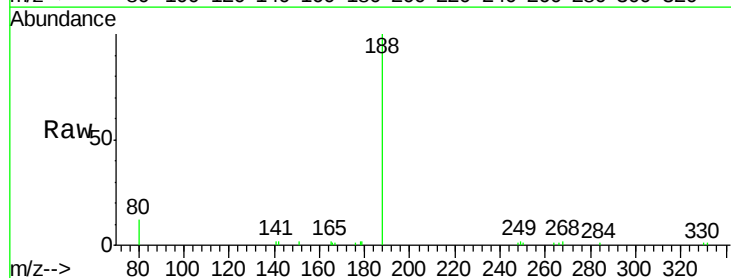

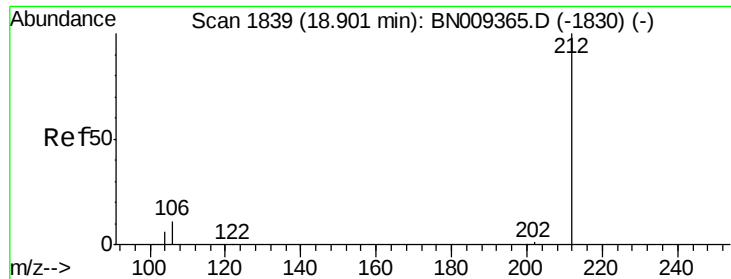

#25

Fluoranthene-d10

Concen: 0.277 ng

RT: 18.90 min Scan# 1840

Delta R.T. -0.00 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41

Instrument :

BNA\_N

ClientSampleId :

PB125983BL


Tot Ion:212 Resp: 6418

Ion Ratio Lower Upper

212 100

106 11.5 9.2 13.8




104 6.6 5.4 8.0

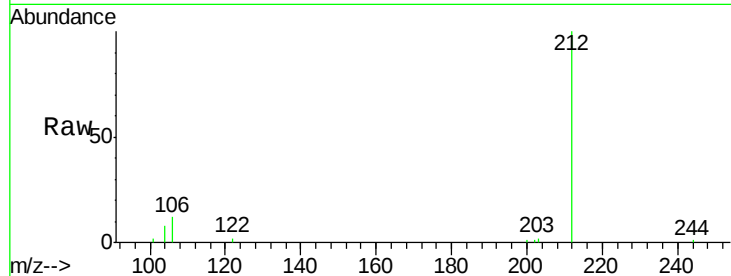

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

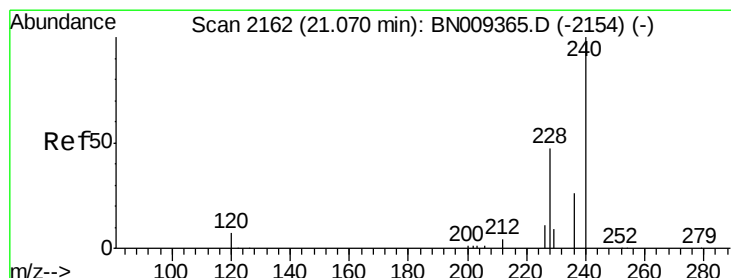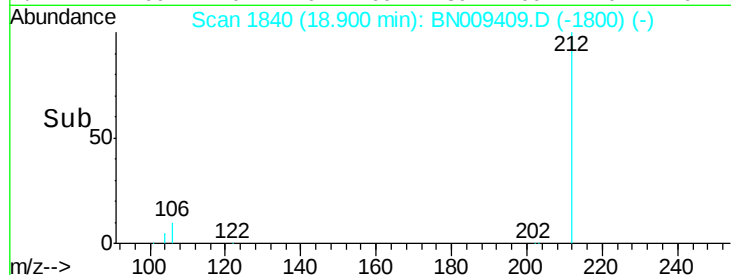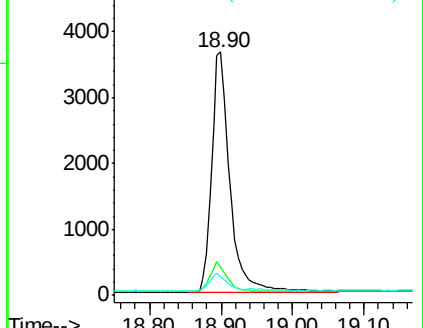

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.07 min Scan# 2163

Delta R.T. -0.00 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41


Tgt Ion:240 Resp: 6121

Ion Ratio Lower Upper

240 100

120 9.8 8.1 12.1



236 27.7 22.2 33.4

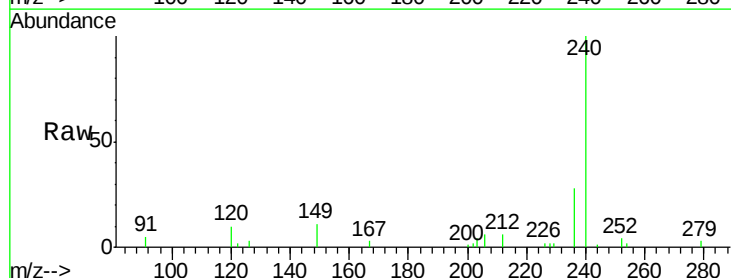


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

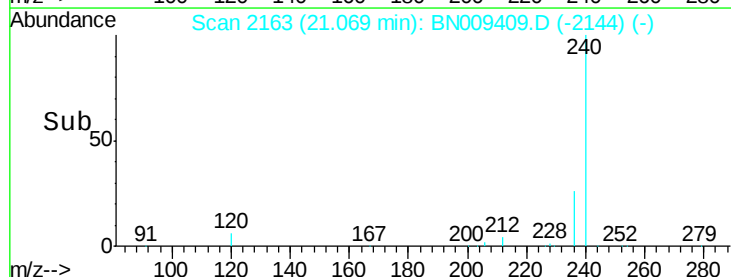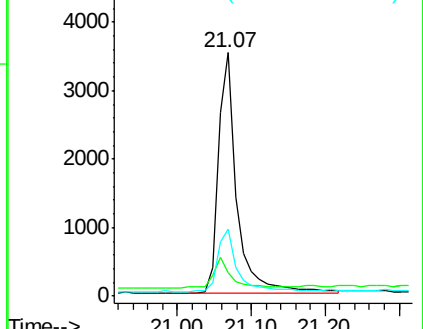

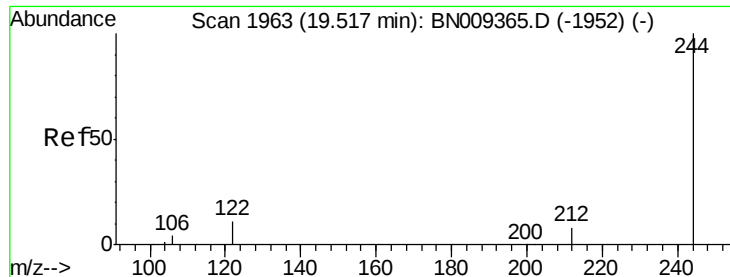

#29

Terphenyl-d14

Concen: 0.330 ng

RT: 19.51 min Scan# 1963

Delta R.T. -0.01 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41

Instrument :

BNA\_N

ClientSampleId :

PB125983BL


Tot Ion:244 Resp: 4783

Ion Ratio Lower Upper

244 100

212 9.9 7.5 11.3




122 12.5 9.8 14.6

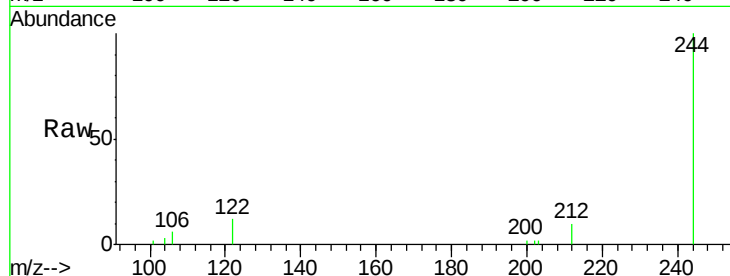

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

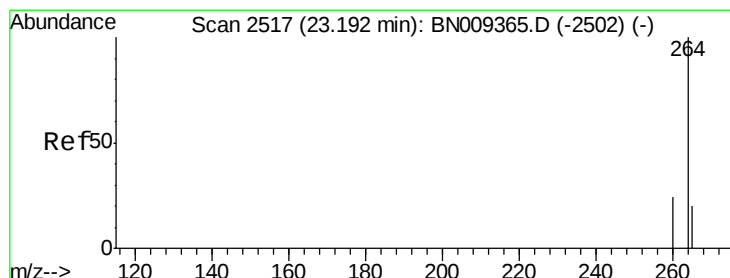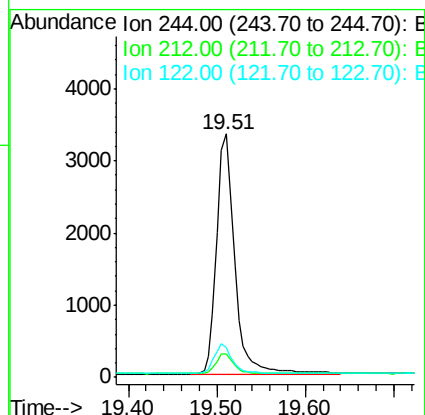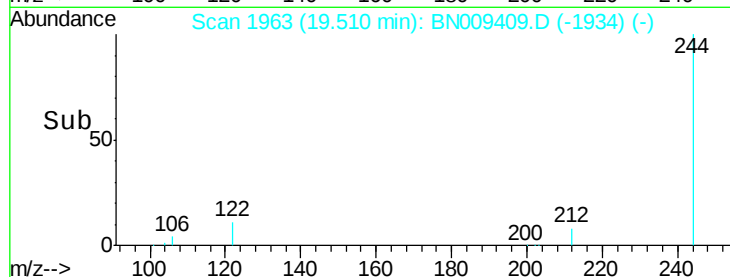

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.19 min Scan# 2517

Delta R.T. -0.01 min

Lab File: BN009409.D

Acq: 21 Jan 2020 11:41


Tgt Ion:264 Resp: 6313

Ion Ratio Lower Upper

264 100

260 25.7 20.1 30.1

265 77.8 68.2 102.4

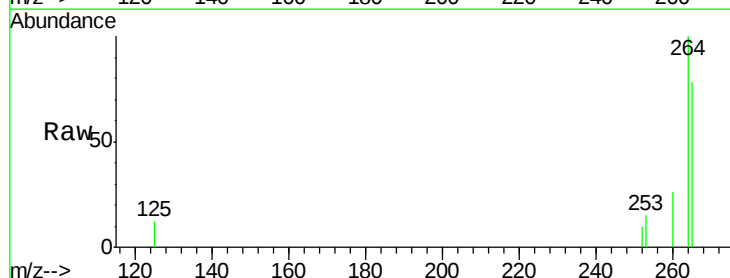

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

