


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012120\
 Data File : BN009406.D
 Acq On : 21 Jan 2020 09:18
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN011420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 09:33:55 2020

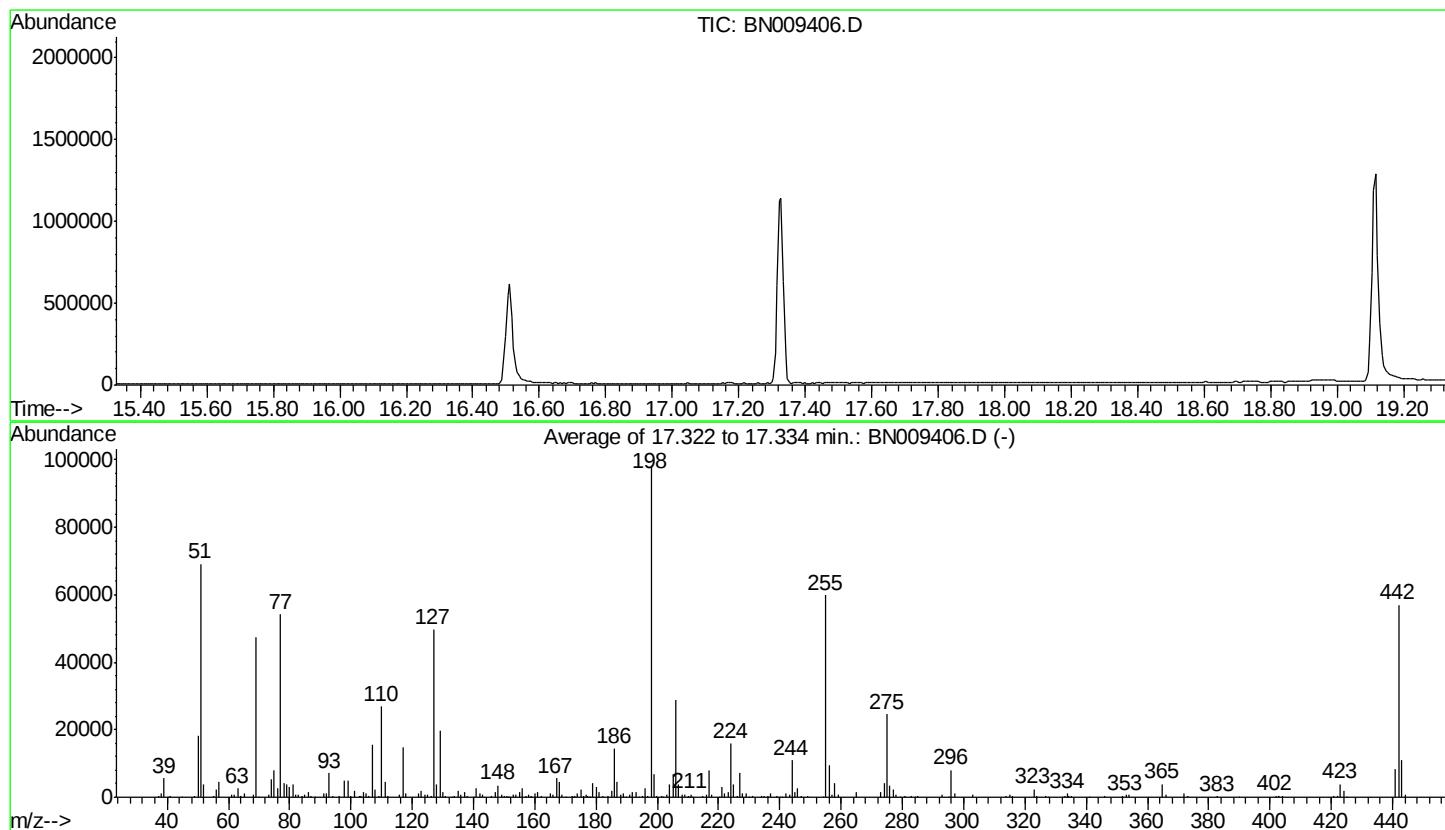

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2430

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.4	69165	PASS
68	69	0.00	2	1.7	802	PASS
69	198	0.00	100	48.2	47389	PASS
70	69	0.00	2	0.4	202	PASS
127	198	10	80	50.5	49605	PASS
197	198	0.00	2	0.3	251	PASS
198	198	100	100	100.0	98253	PASS
199	198	5	9	6.8	6695	PASS
275	198	10	60	25.0	24536	PASS
365	198	1	100	3.9	3852	PASS
441	198	0.01	100	8.7	8534	PASS
442	198	50	100	58.1	57074	PASS
443	442	15	24	19.4	11080	PASS