
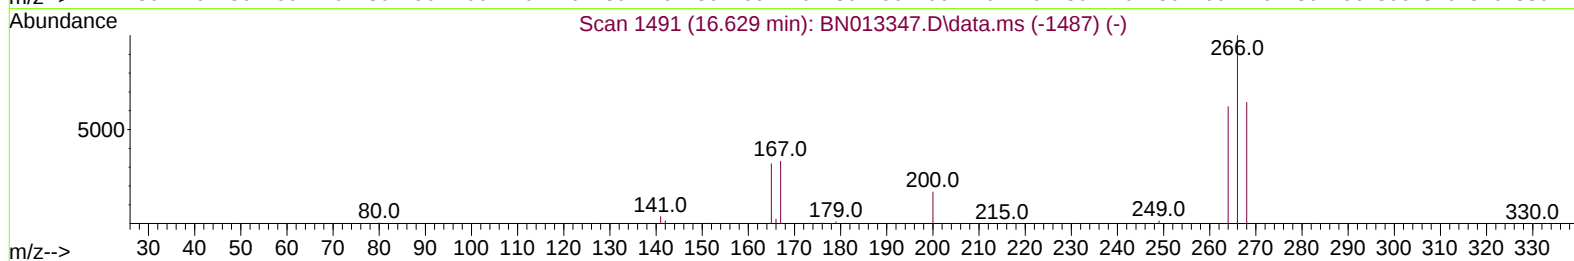
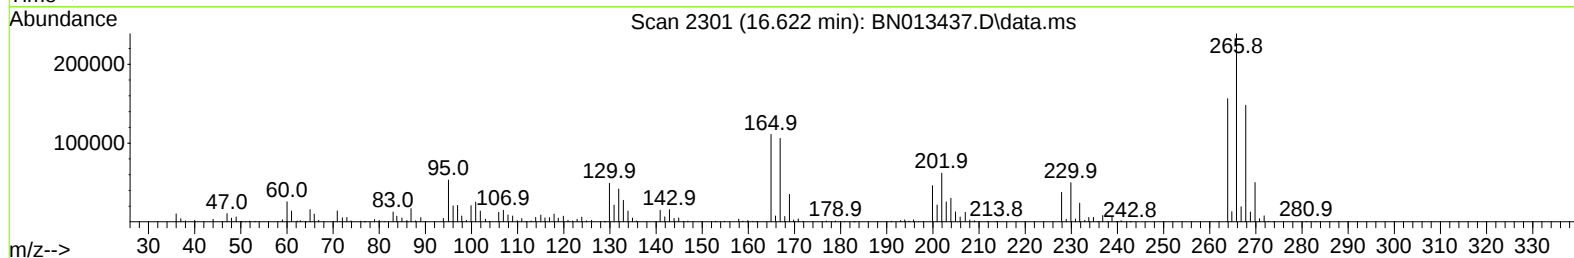


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012121\
Data File : BN013437.D
Acq On : 20 Jan 2021 13:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 01:22:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 20 16:01:28 2021
Response via : Initial Calibration

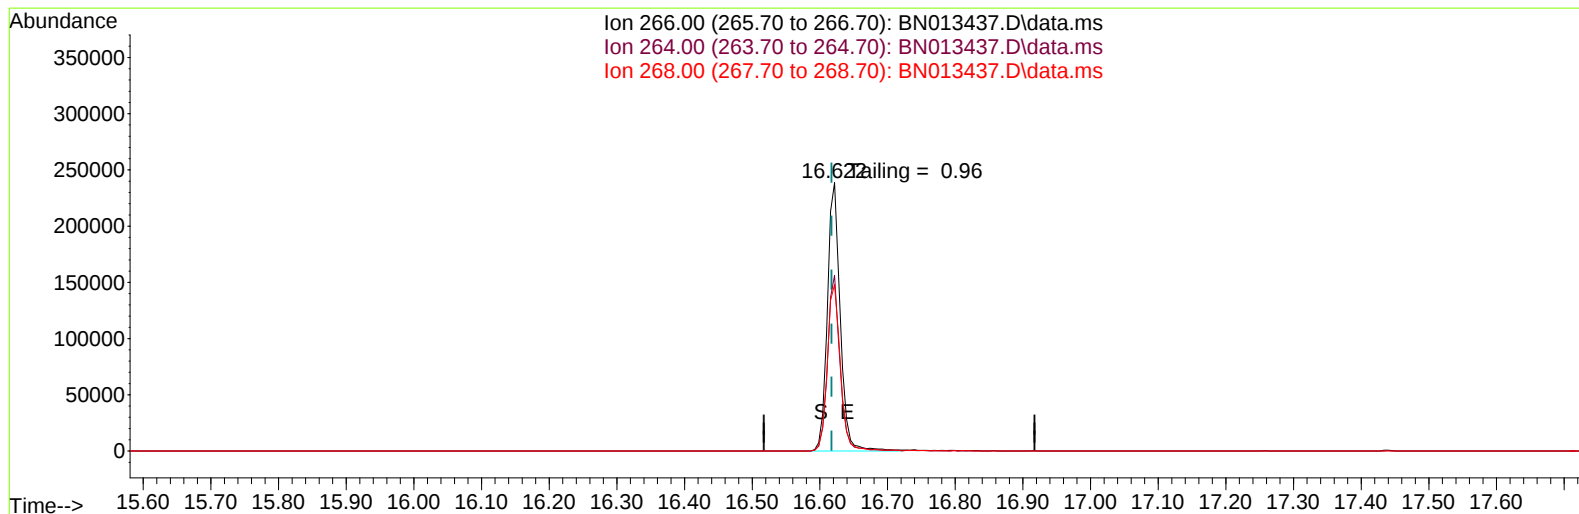

TIC: BN013437.D\data.ms

(24) Pentachlorophenol

16.622min (+ 0.004) 0.00 ng

response 315222

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.70
268.00	68.30	63.25
0.00	0.00	0.00