
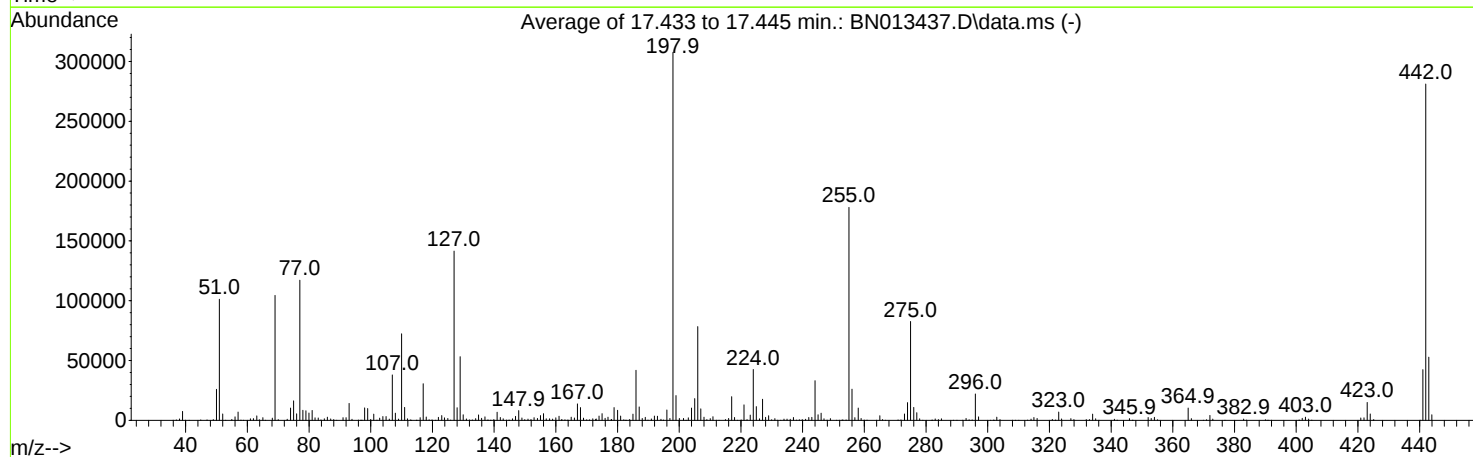


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012121\
 Data File : BN013437.D
 Acq On : 20 Jan 2021 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 20 16:01:28 2021

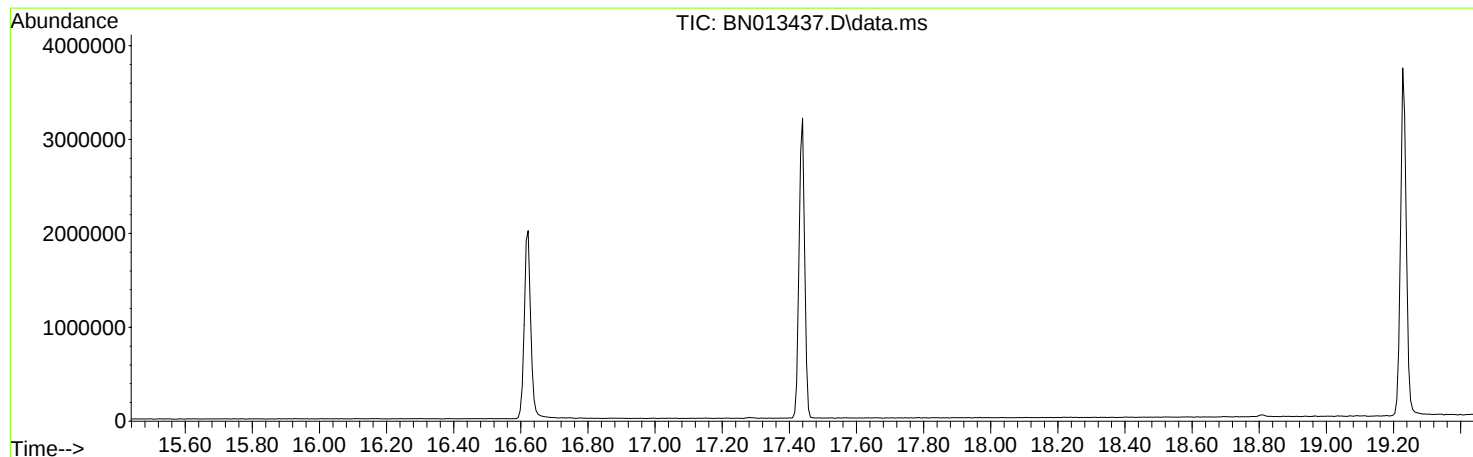

AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	101321	PASS
68	69	0.00	2	1.8	1874	PASS
69	198	0.00	100	34.0	104483	PASS
70	69	0.00	2	0.6	619	PASS
127	198	10	80	46.0	141472	PASS
197	198	0.00	2	0.5	1671	PASS
198	198	100	100	100.0	307477	PASS
199	198	5	9	6.7	20750	PASS
275	198	10	60	26.9	82672	PASS
365	198	1	100	3.4	10361	PASS
441	198	0.01	100	13.8	42349	PASS
442	442	50	100	100.0	281195	PASS
443	442	15	24	18.8	52853	PASS