
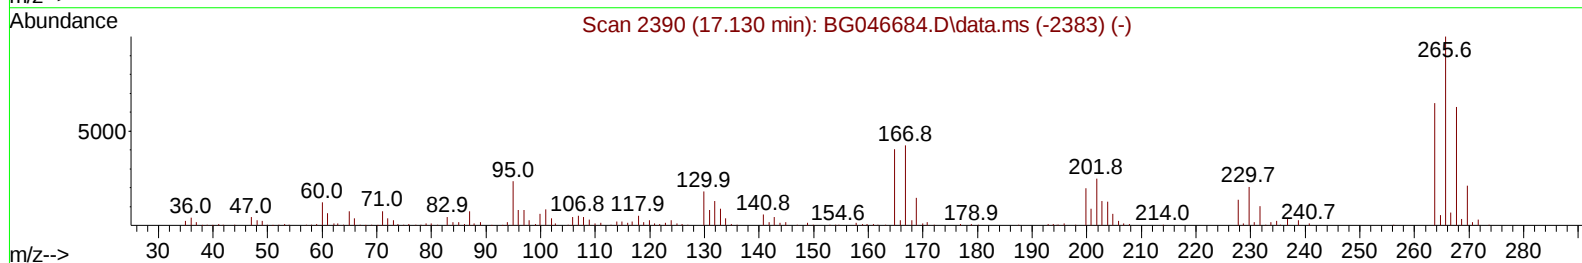
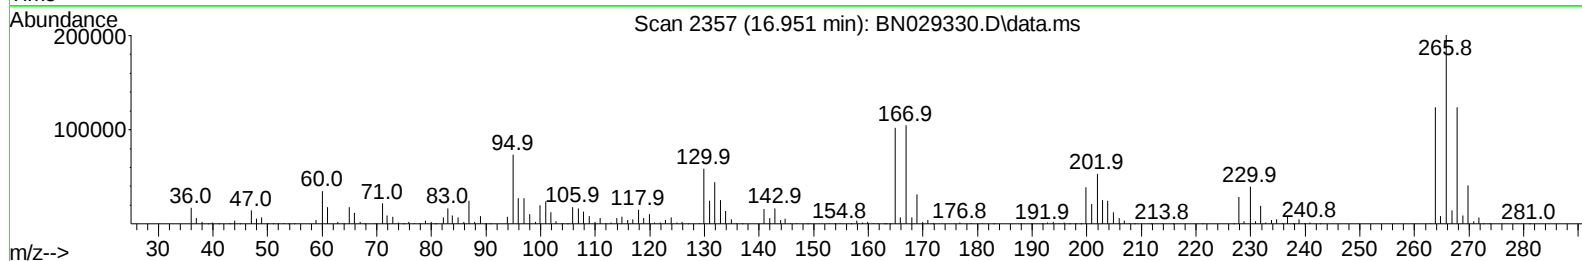


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012224\
Data File : BN029330.D
Acq On : 22 Jan 2024 14:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 02:56:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 02:56:13 2024
Response via : Initial Calibration



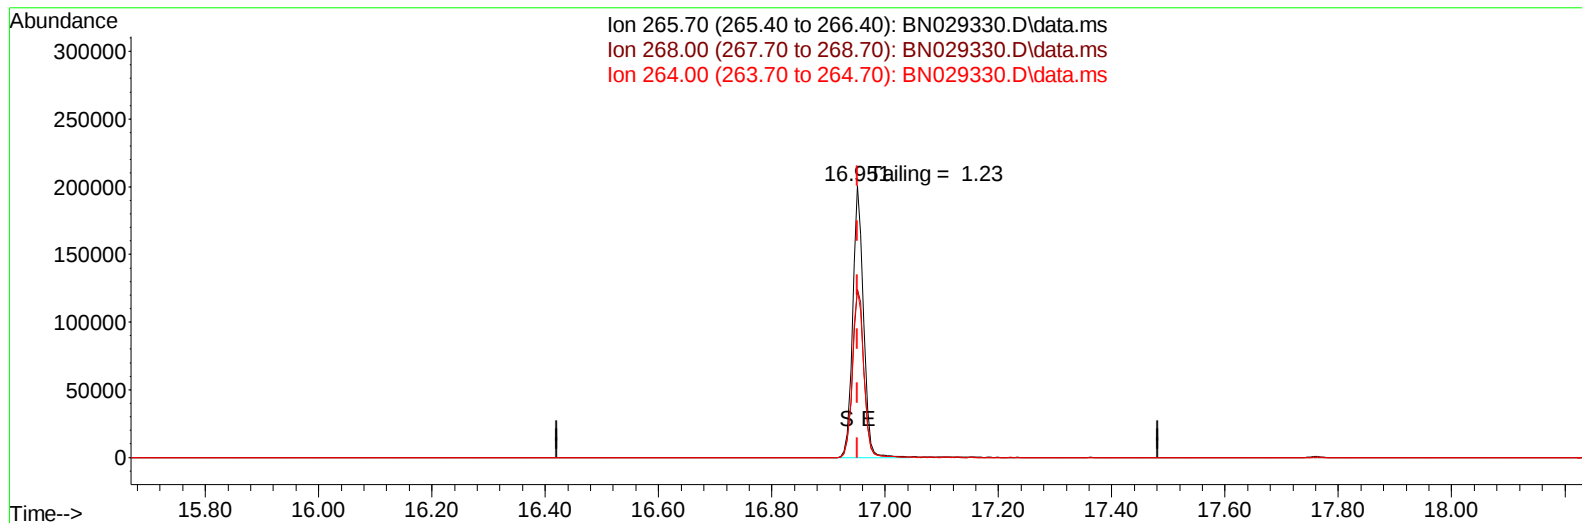


TIC: BN029330.D\data.ms

(70) Pentachlorophenol (C)**16.951min (0.000) 17129.07 ng****response 267505**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.83
264.00	61.60	61.88
0.00	0.00	0.00

Quant Time: Jan 23 02:56:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 02:56:13 2024
Response via : Initial Calibration

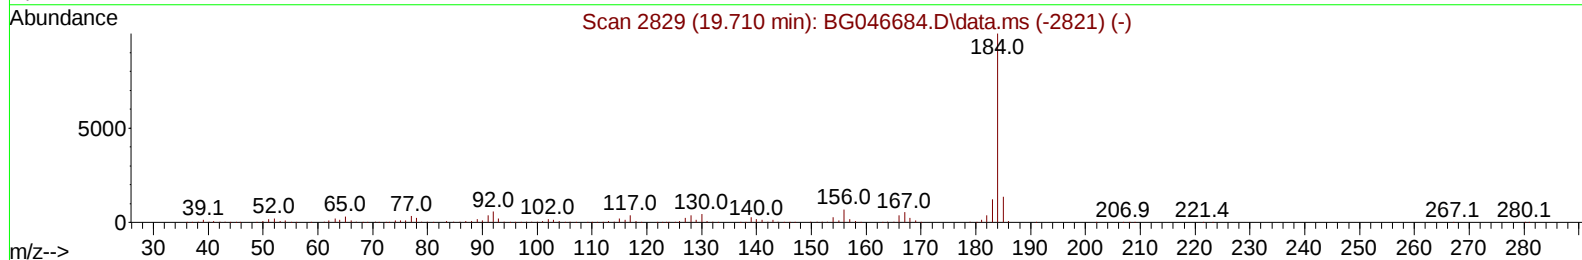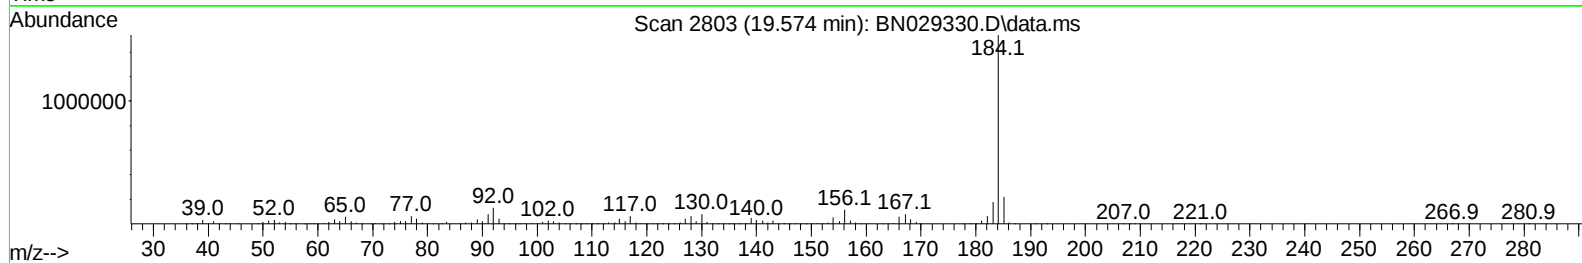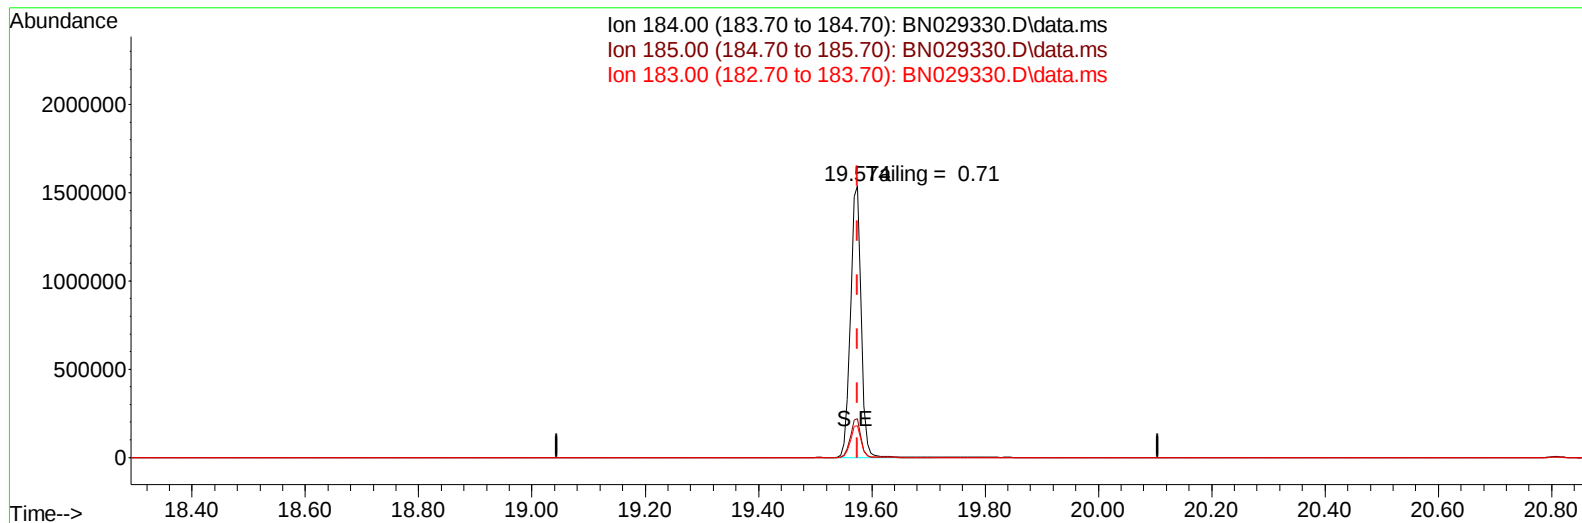

TIC: BN029330.D\data.ms

(77) **Benzidine**

19.574min (0.000) 0.00 ng

response 2024431

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	11.64
0.00	0.00	0.00