


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012224\
Data File : BN029330.D
Acq On : 22 Jan 2024 14:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 23 02:16:14 2024

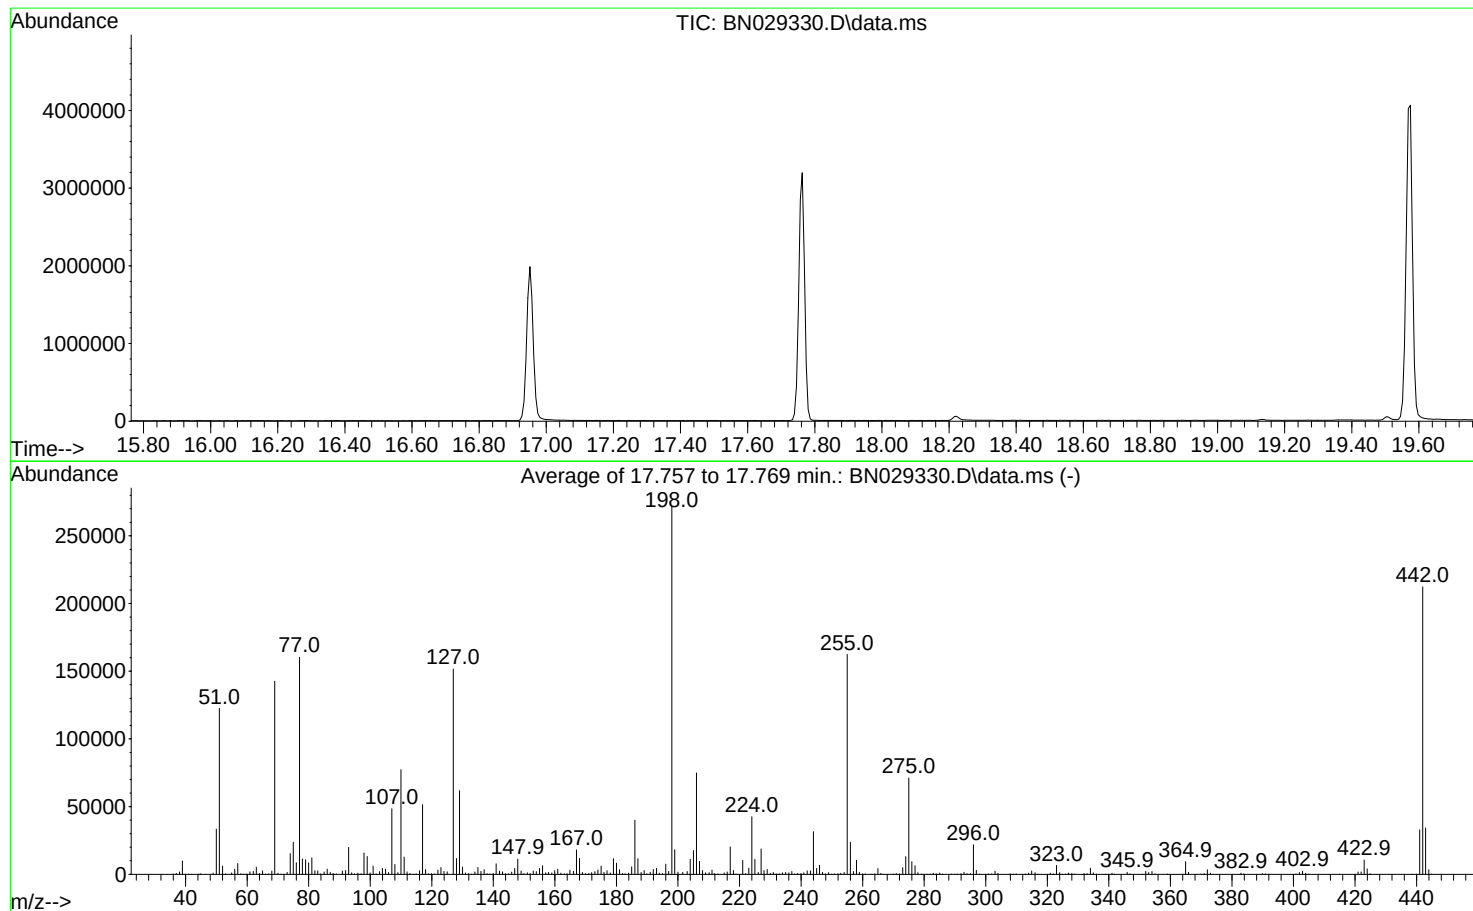




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	122551	PASS
68	69	0.00	2	1.7	2462	PASS
69	198	0.00	100	52.5	142560	PASS
70	69	0.00	2	0.6	878	PASS
127	198	10	80	55.8	151659	PASS
197	198	0.00	2	0.8	2040	PASS
198	198	100	100	100.0	271744	PASS
199	198	5	9	6.7	18180	PASS
275	198	10	60	26.2	71163	PASS
365	198	1	100	3.4	9247	PASS
441	198	0.01	100	12.1	32811	PASS
442	442	50	100	100.0	212309	PASS
443	442	15	24	16.1	34208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012224\
Data File : BN029330.D
Acq On : 22 Jan 2024 14:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 23 02:56:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 02:56:13 2024
Response via : Initial Calibration

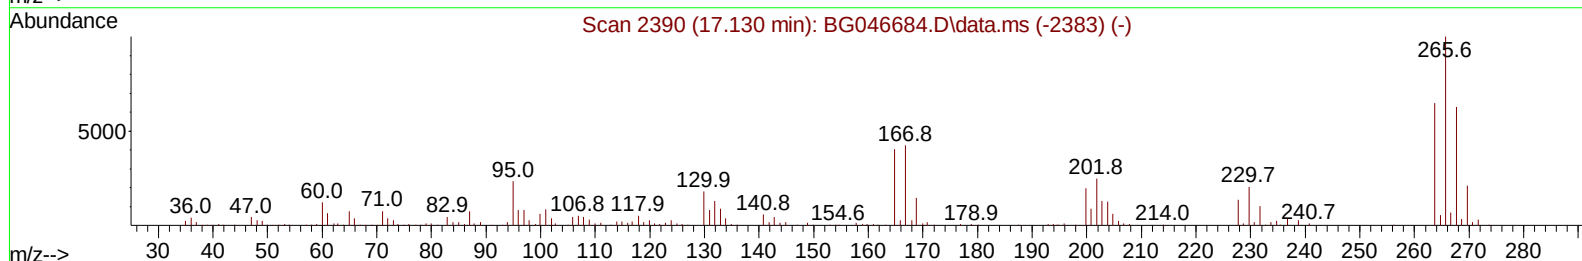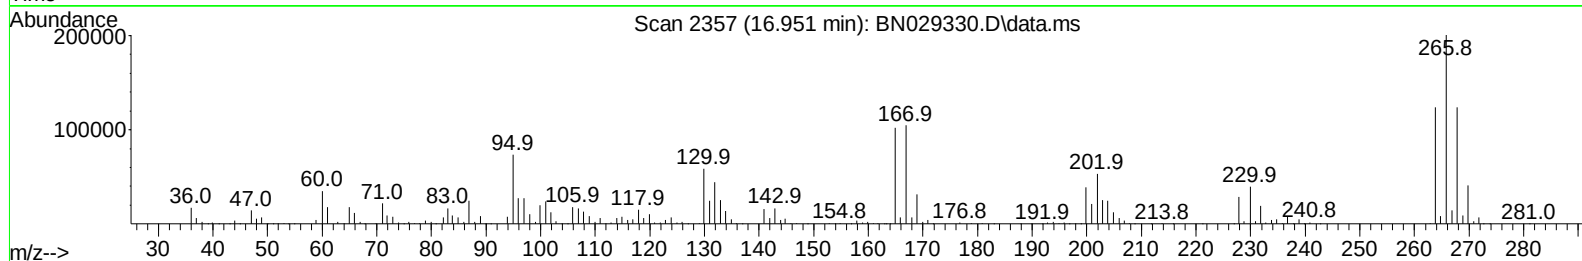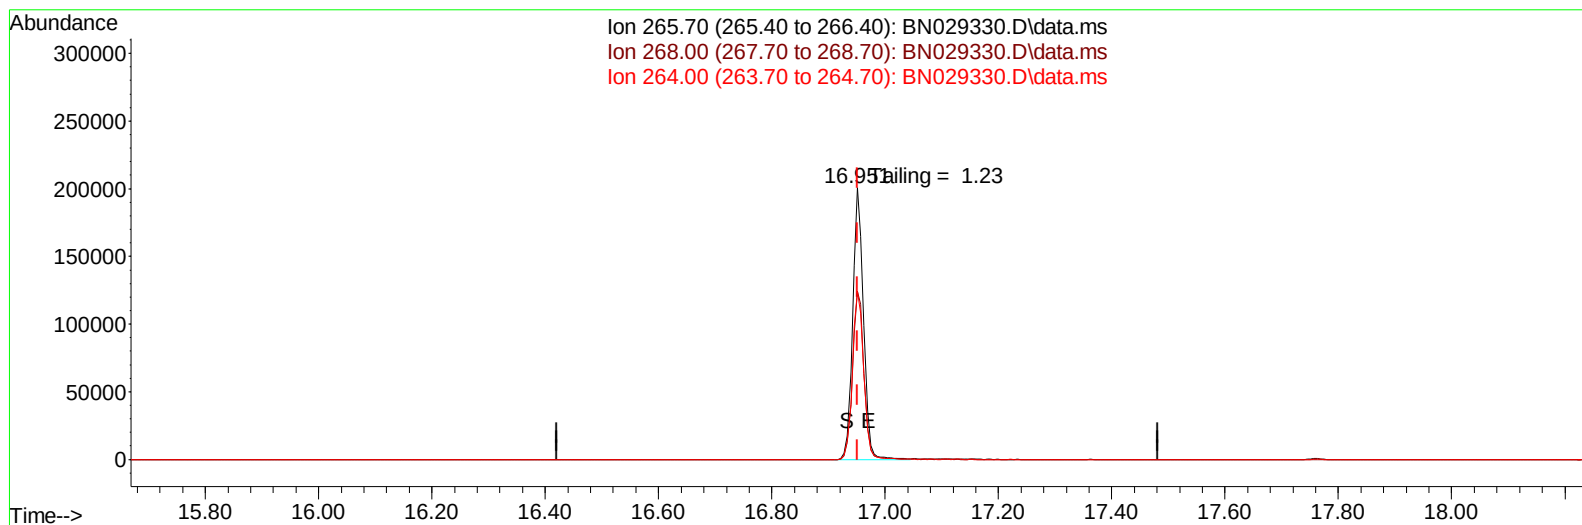

TIC: BN029330.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 17129.07 ng




response 267505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.83
264.00	61.60	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012224\
Data File : BN029330.D
Acq On : 22 Jan 2024 14:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 23 02:56:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 02:56:13 2024
Response via : Initial Calibration

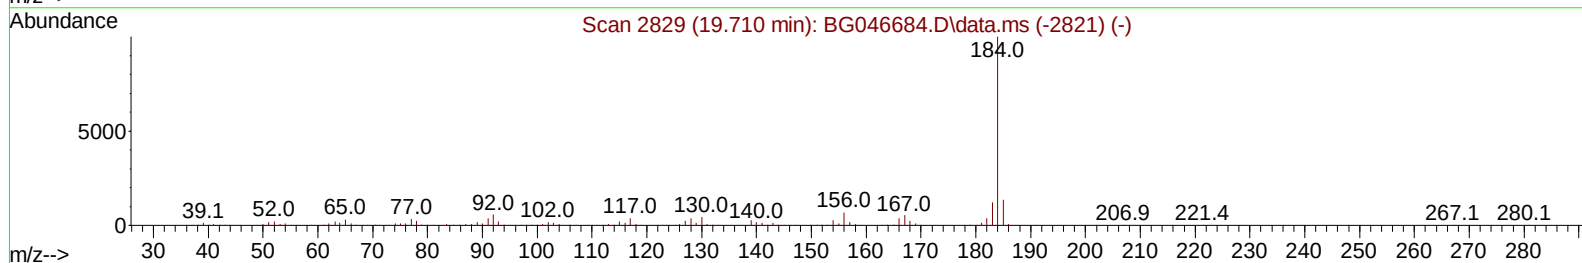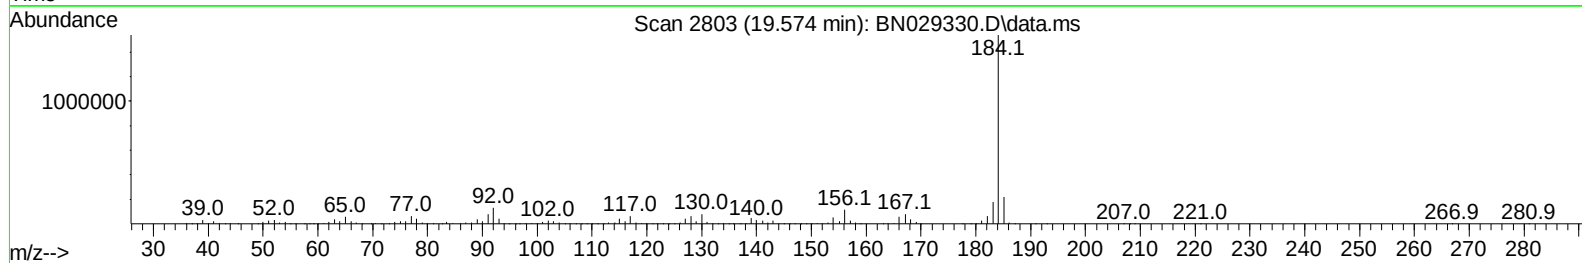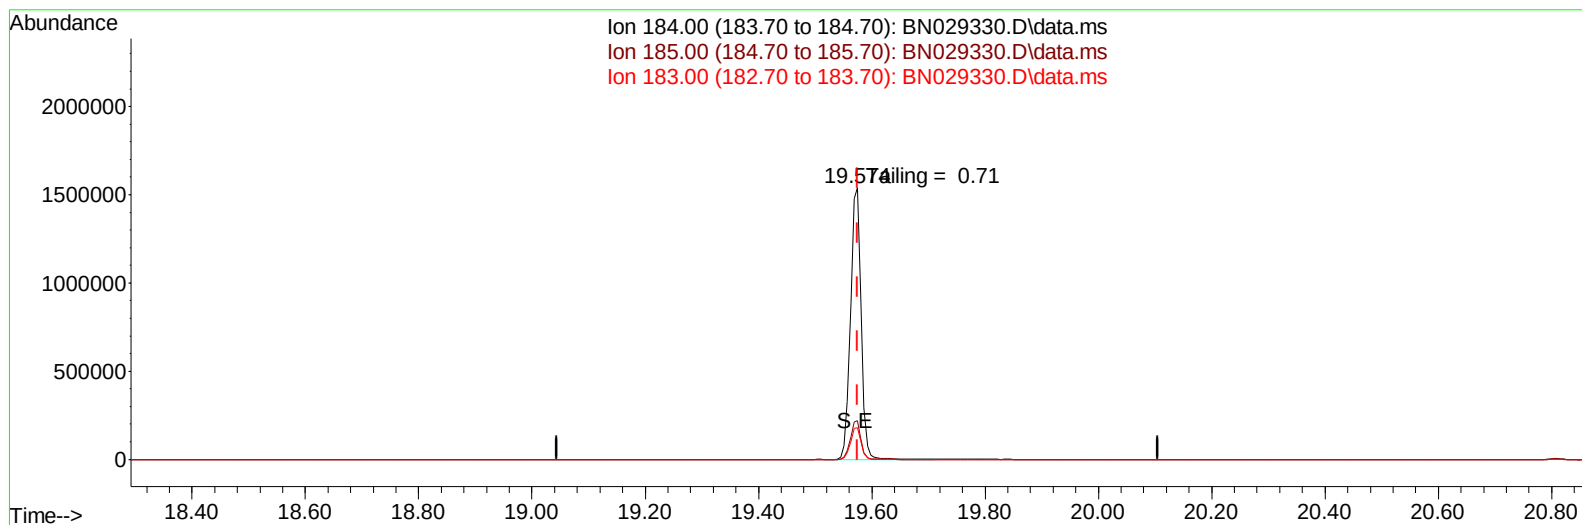

TIC: BN029330.D\data.ms

(77) Benzidine

19.574min (0.000) 0.00 ng

response 2024431

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.30
183.00	13.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/22/2024	BNA_N	<u>BN029330.D</u>
Compound Name	Response	Retention Time
DDT	983480	20.81
DDD	7704	20.416
DDE	146	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7850	991330	0.79

Instrument :
BNA_N
ClientSampleId :
DFTPP