
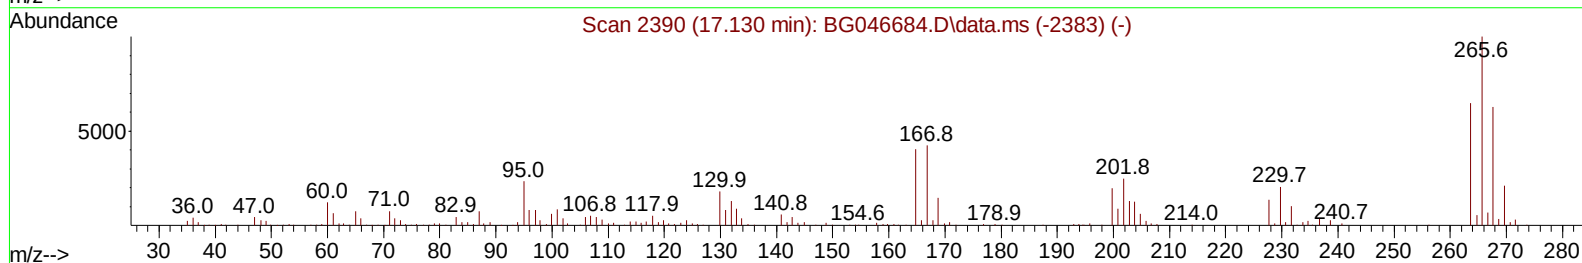
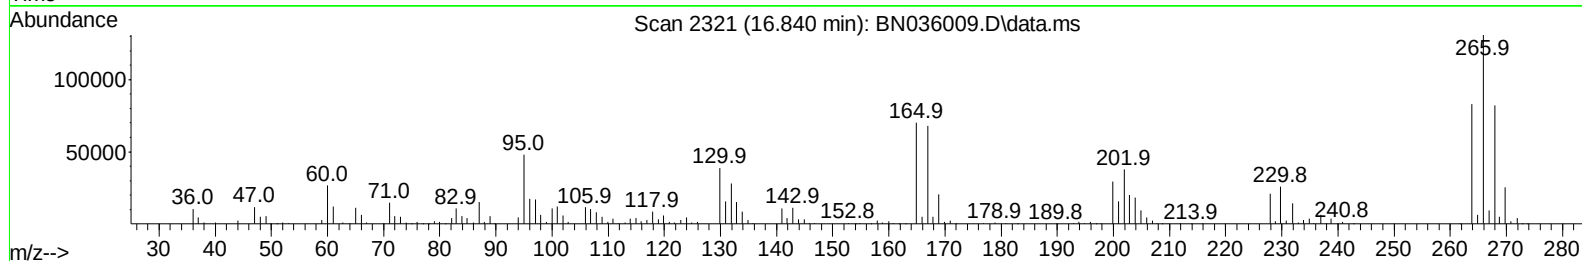


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012225\
Data File : BN036009.D
Acq On : 22 Jan 2025 09:44
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 00:54:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

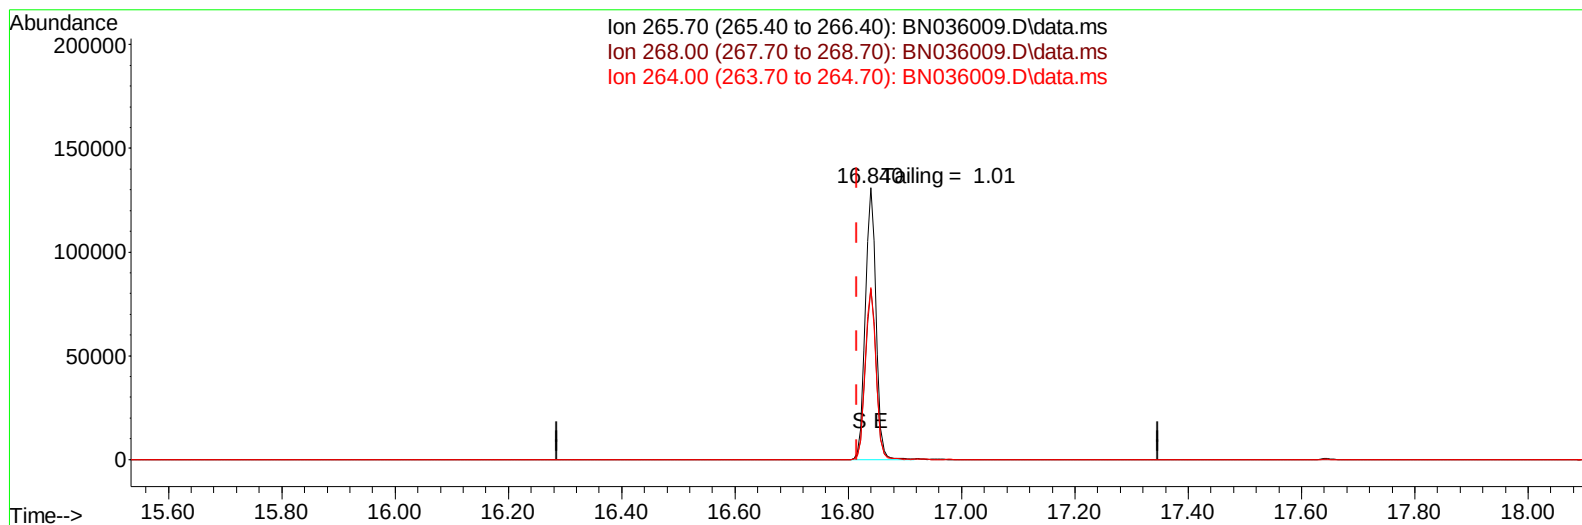

TIC: BN036009.D\data.ms

(70) Pentachlorophenol (C)




16.840min (+ 0.024) 21048.35 ng

response 172285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.84
264.00	61.60	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012225\
Data File : BN036009.D
Acq On : 22 Jan 2025 09:44
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 00:54:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

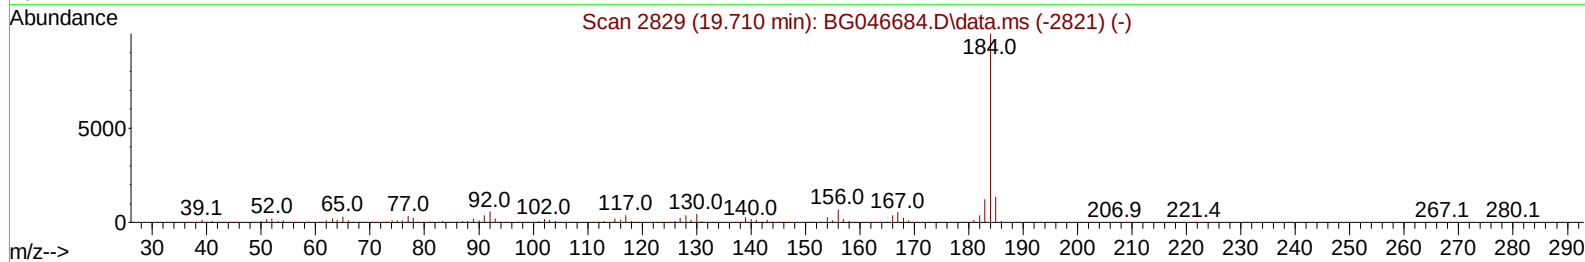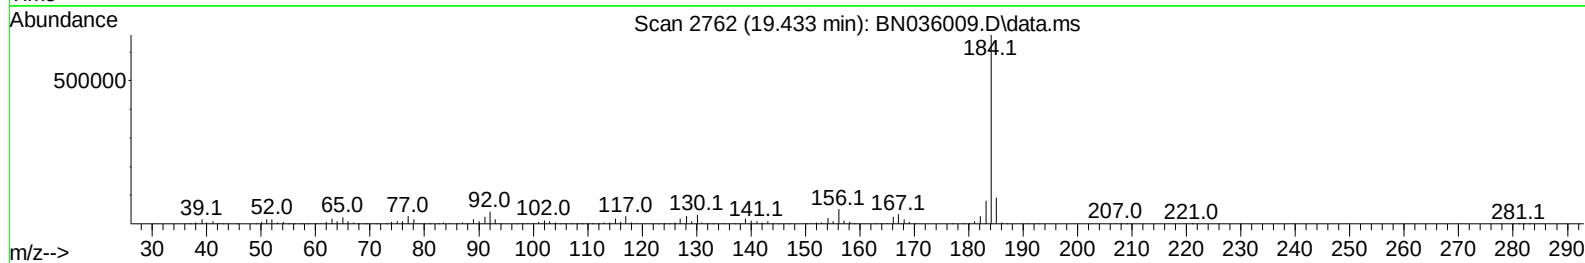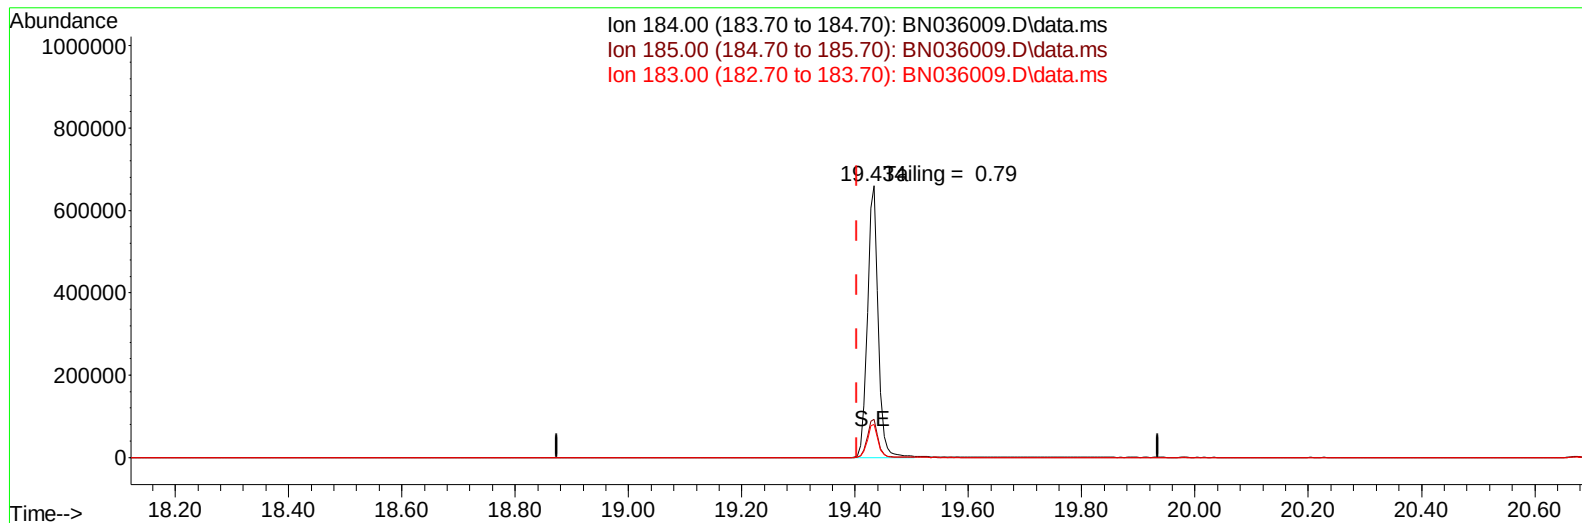

TIC: BN036009.D\data.ms

(77) Benzidine**19.433min (+ 0.029) 0.00 ng****response 875464**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.24
0.00	0.00	0.00