
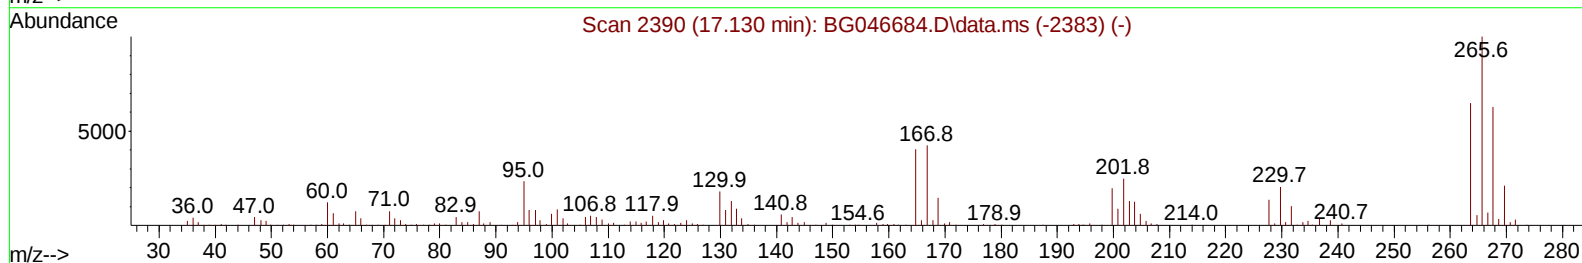
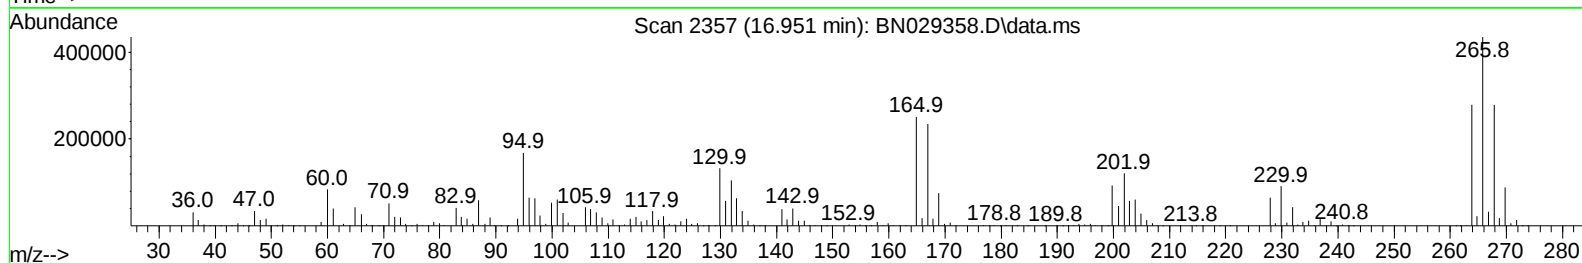


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029358.D
Acq On : 23 Jan 2024 22:48
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 05:23:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

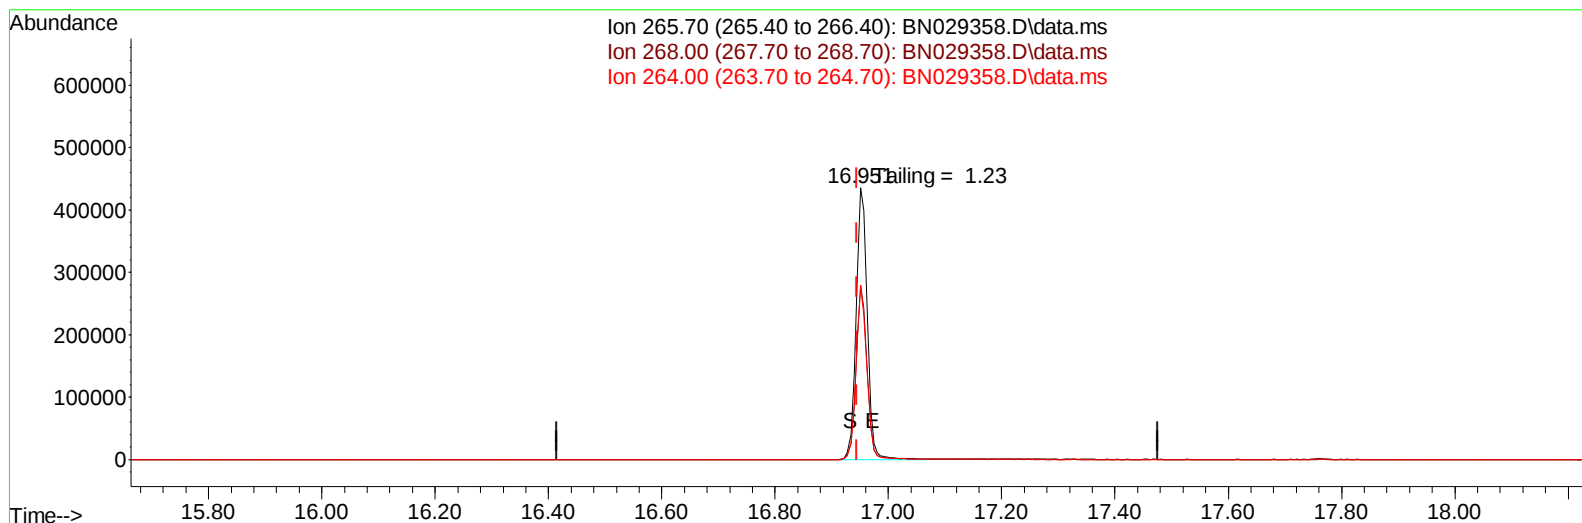




TIC: BN029358.D\data.ms

(70) Pentachlorophenol (C)**16.951min (+ 0.006) 18305.11 ng****response 596020**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.93
264.00	61.60	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029358.D
Acq On : 23 Jan 2024 22:48
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 05:23:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

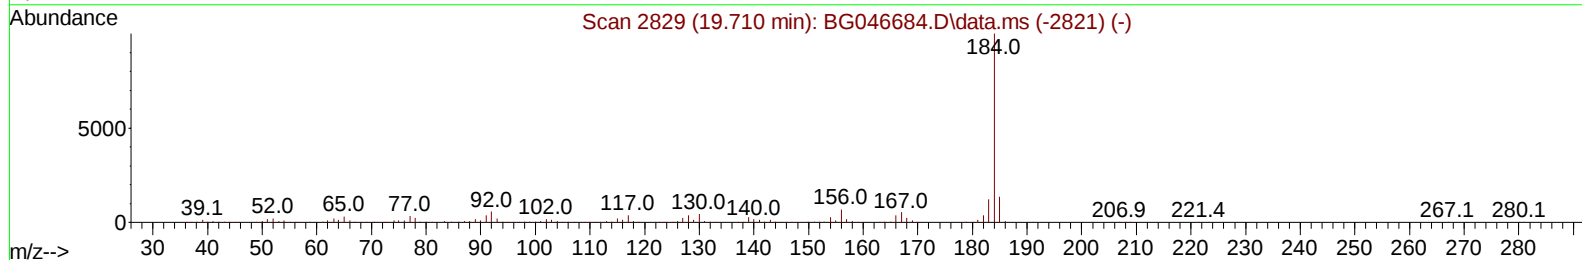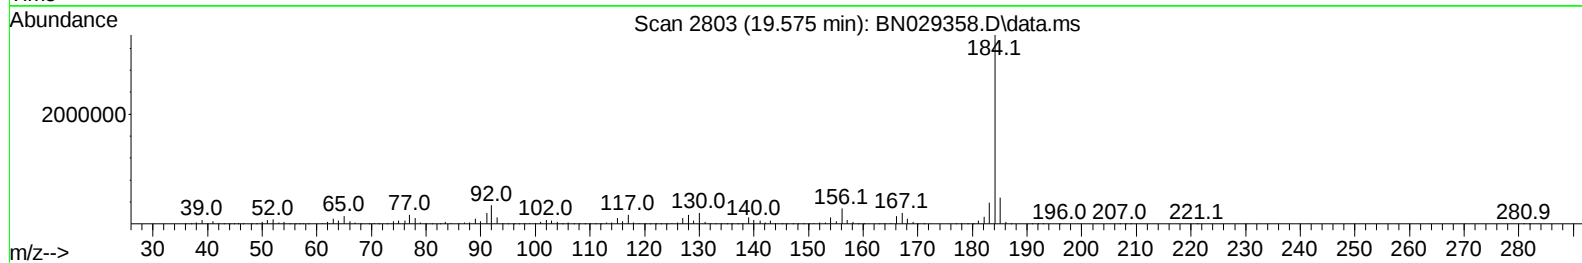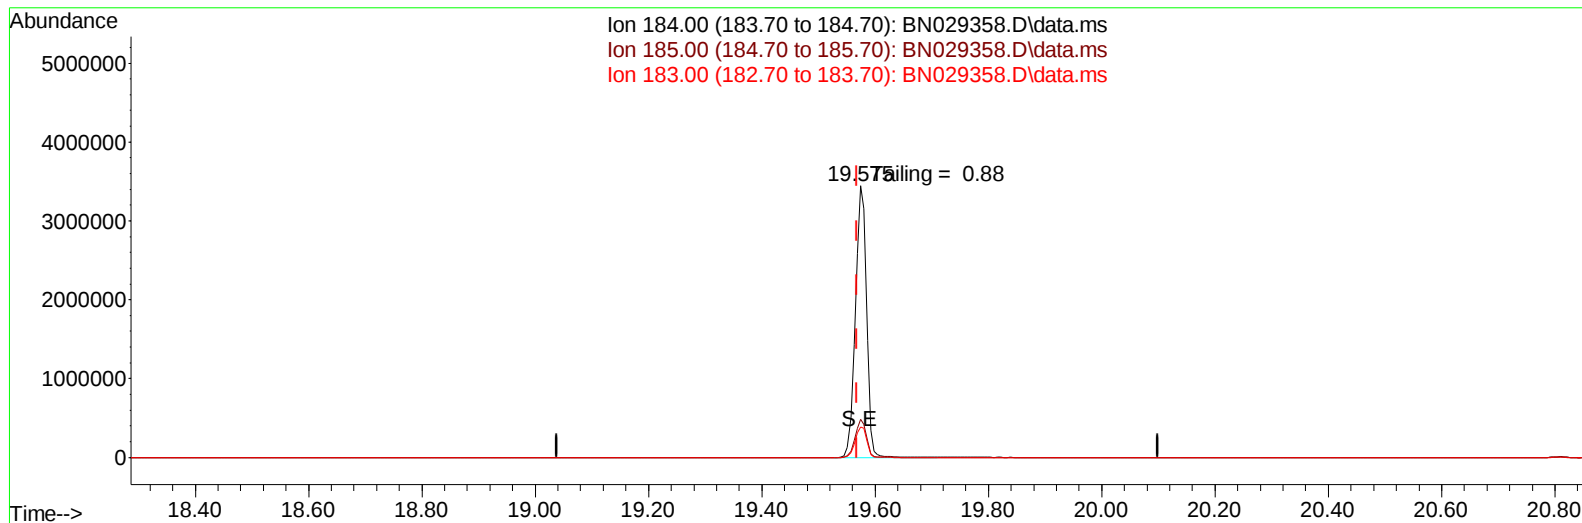

TIC: BN029358.D\data.ms

(77) Benzidine

19.575min (+ 0.006) 0.00 ng

response 4714345

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.32
0.00	0.00	0.00