
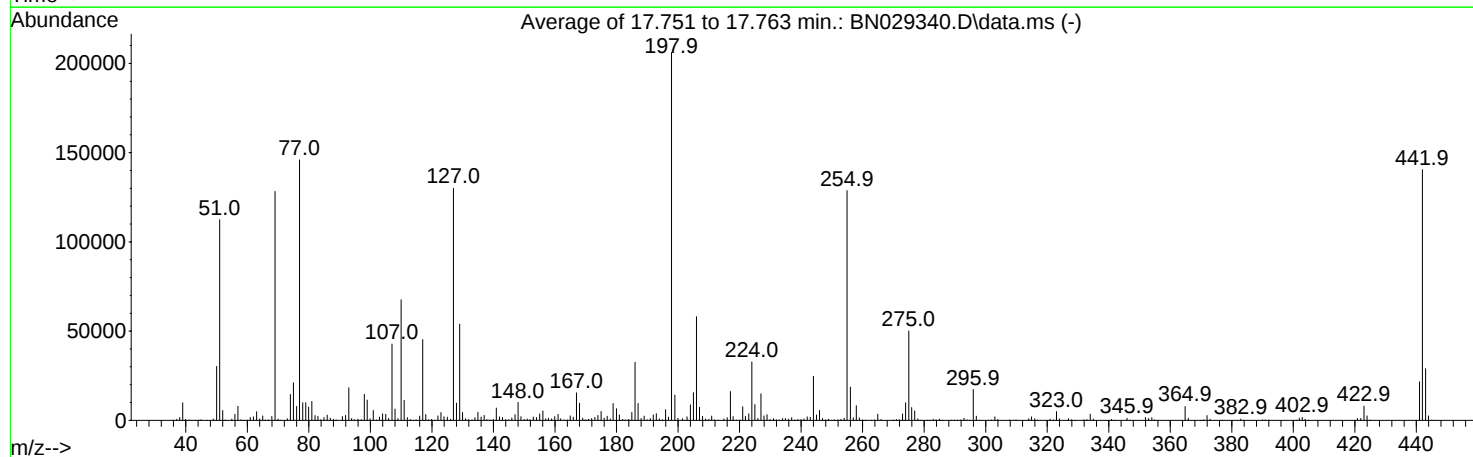


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029340.D
Acq On : 23 Jan 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 23 02:16:14 2024

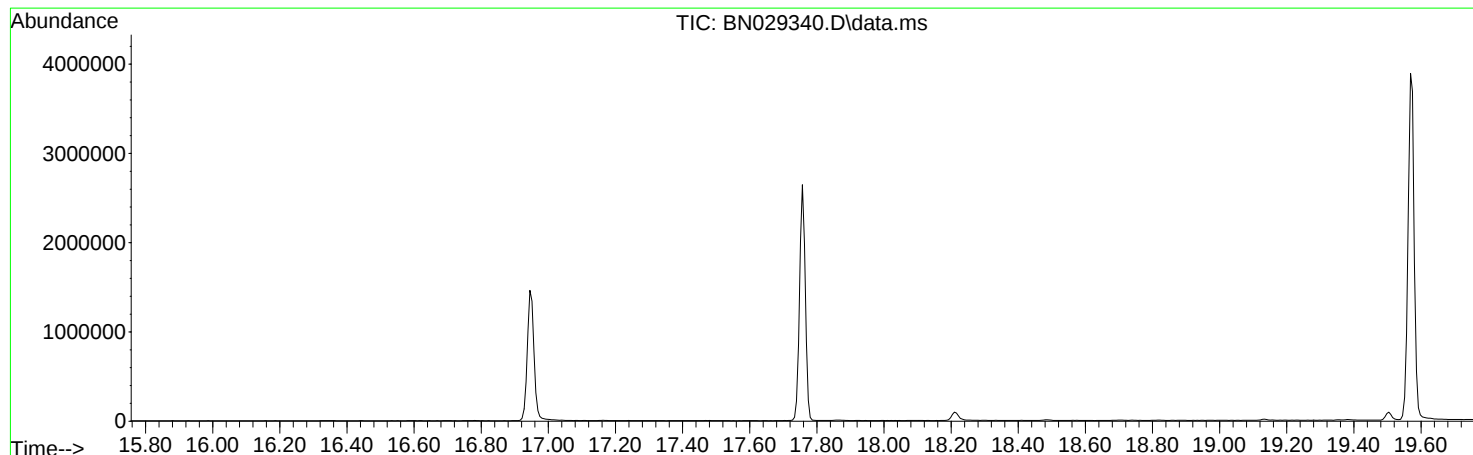




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	112427	PASS
68	69	0.00	2	1.8	2249	PASS
69	198	0.00	100	62.2	128259	PASS
70	69	0.00	2	0.6	751	PASS
127	198	10	80	63.1	130059	PASS
197	198	0.00	2	0.9	1789	PASS
198	198	100	100	100.0	206101	PASS
199	198	5	9	6.9	14214	PASS
275	198	10	60	24.3	50139	PASS
365	198	1	100	3.8	7808	PASS
441	198	0.01	100	10.5	21635	PASS
442	442	50	100	100.0	140507	PASS
443	442	15	24	20.6	28933	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029340.D
Acq On : 23 Jan 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 24 05:21:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

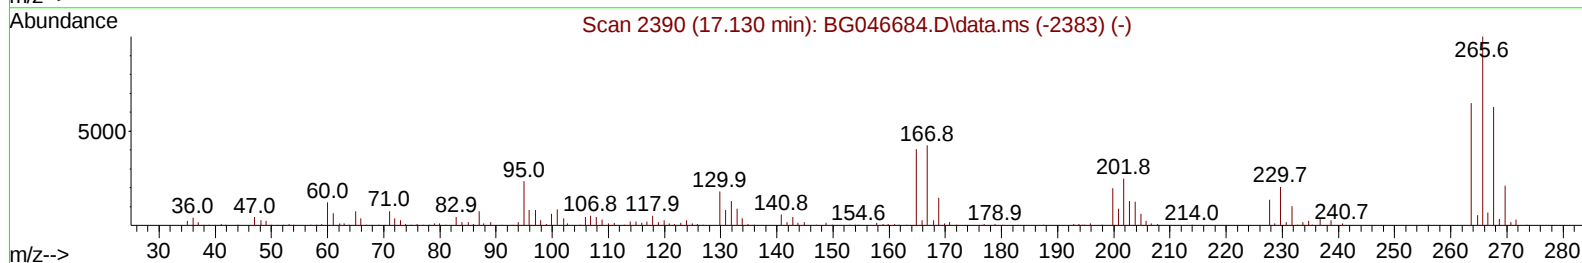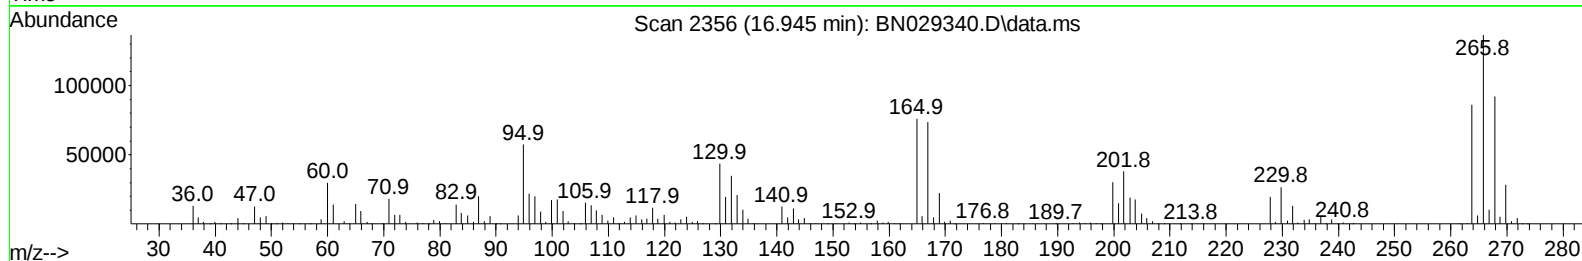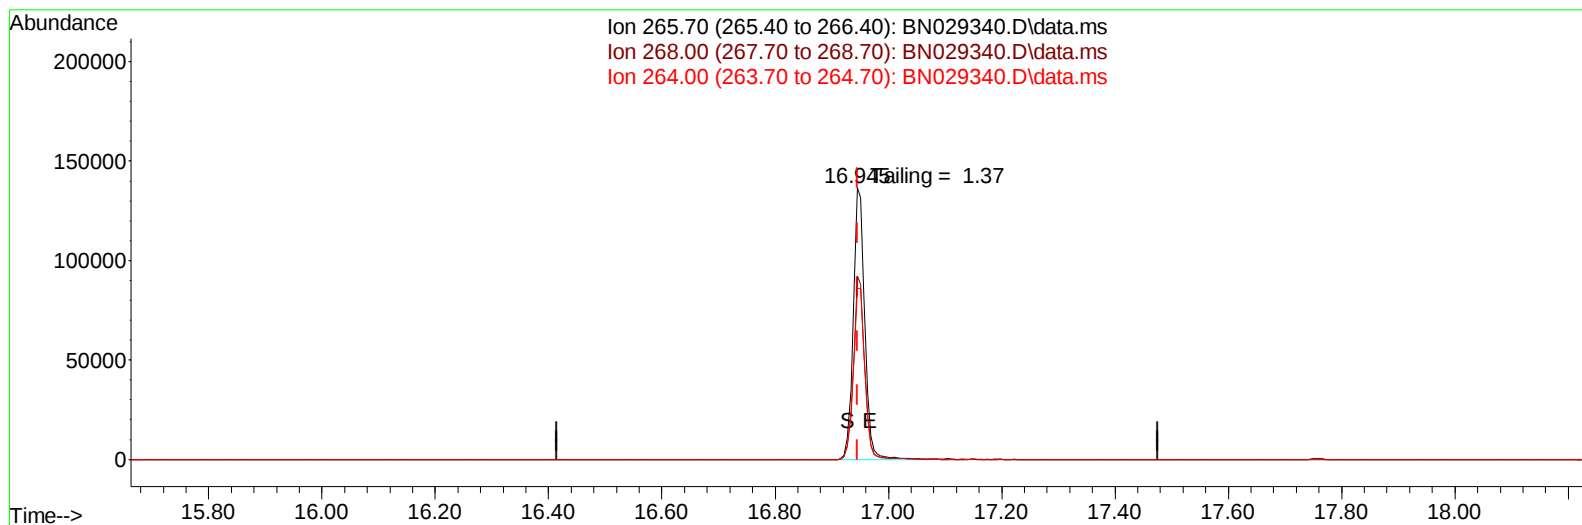

TIC: BN029340.D\data.ms

(70) Pentachlorophenol (C)

16.945min (0.000) 17025.61 ng




response 193872

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.63
264.00	61.60	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029340.D
Acq On : 23 Jan 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 24 05:21:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

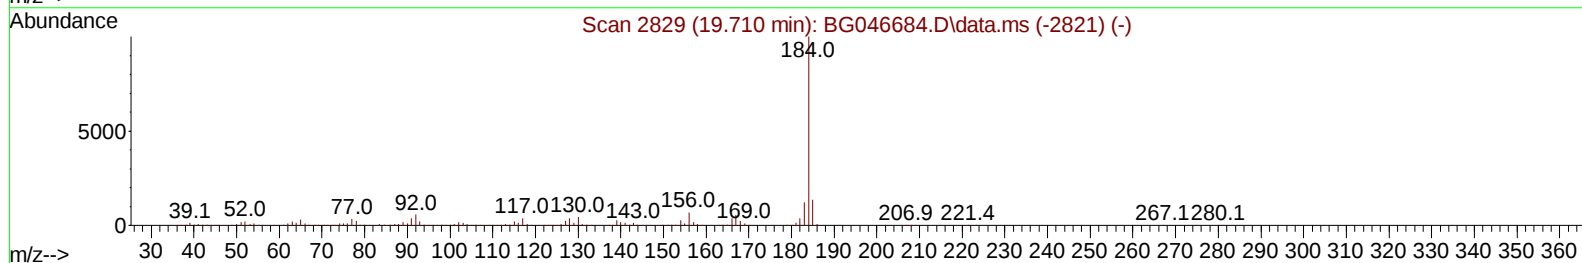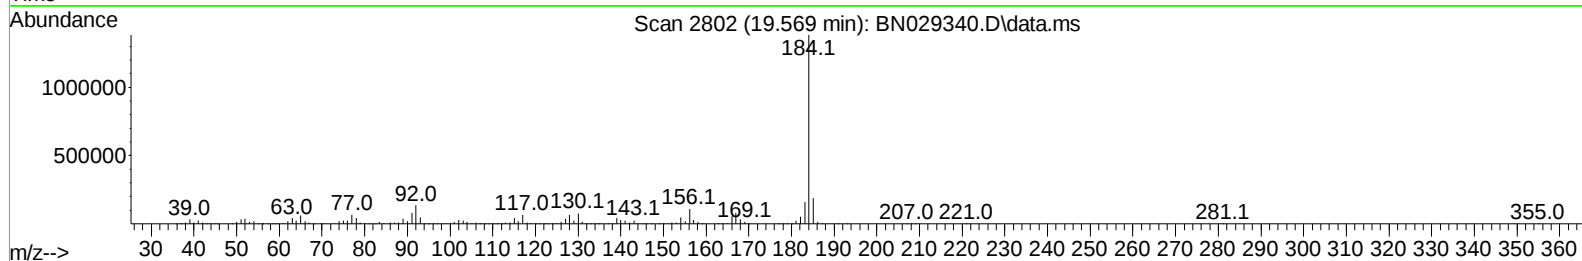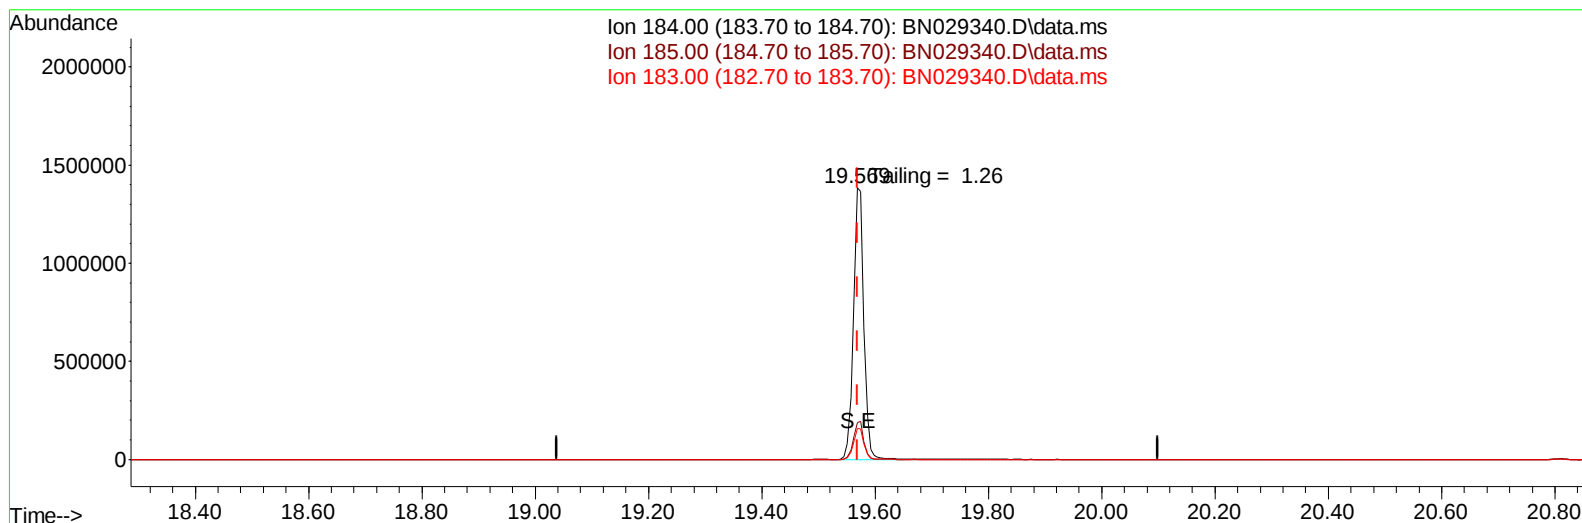

TIC: BN029340.D\data.ms

(77) Benzidine

19.569min (0.000) 0.00 ng

response 1780310

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/23/2024	BNA_N	<u>BN029340.D</u>
Compound Name	Response	Retention Time
DDT	767223	20.81
DDD	6564	20.416
DDE	141	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6705	773928	0.87

Instrument :
BNA_N
ClientSampleId :
DFTPP