
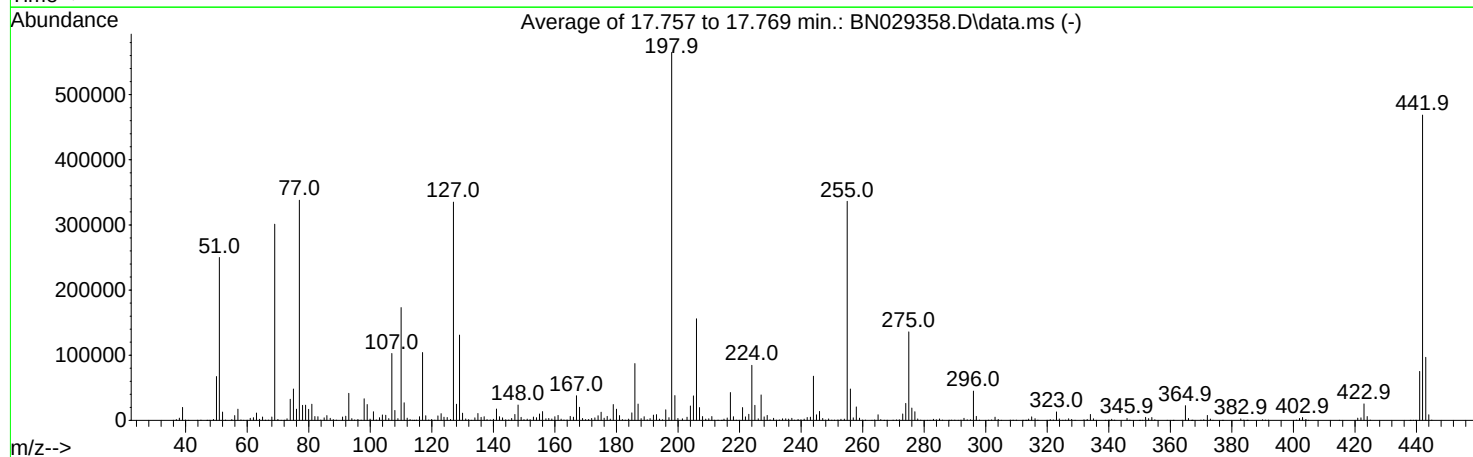


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029358.D
Acq On : 23 Jan 2024 22:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 23 02:16:14 2024

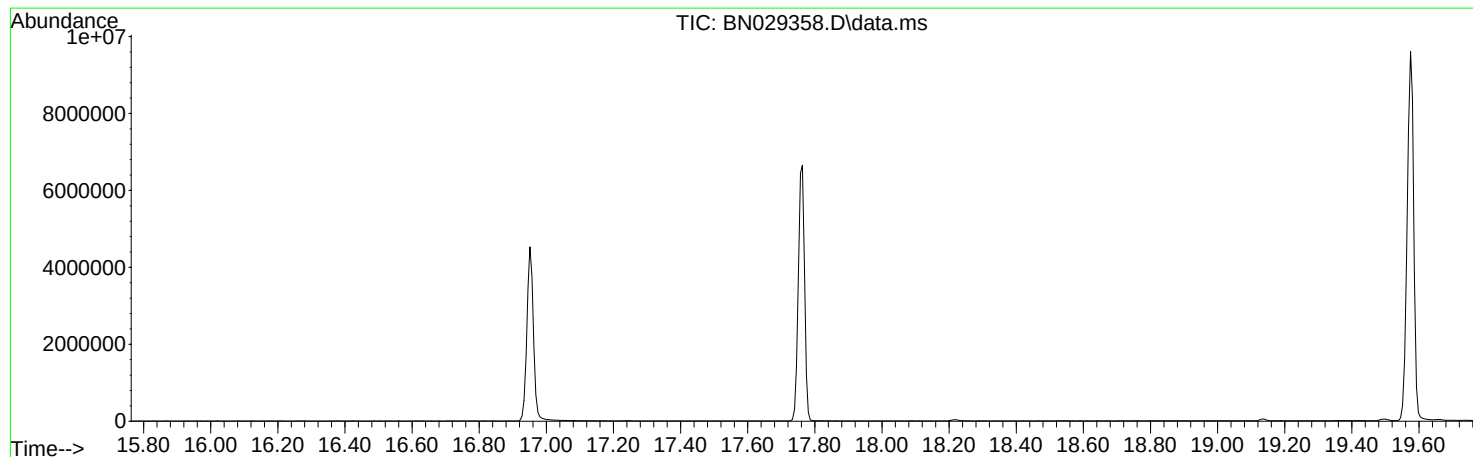




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	44.3	249927	PASS
68	69	0.00	2	1.7	5130	PASS
69	198	0.00	100	53.3	301192	PASS
70	69	0.00	2	0.5	1602	PASS
127	198	10	80	59.3	334976	PASS
197	198	0.00	2	0.7	4119	PASS
198	198	100	100	100.0	564672	PASS
199	198	5	9	6.7	37987	PASS
275	198	10	60	24.0	135784	PASS
365	198	1	100	4.0	22656	PASS
441	198	0.01	100	13.3	75197	PASS
442	442	50	100	100.0	468651	PASS
443	442	15	24	20.7	96819	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029358.D
Acq On : 23 Jan 2024 22:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 24 05:23:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

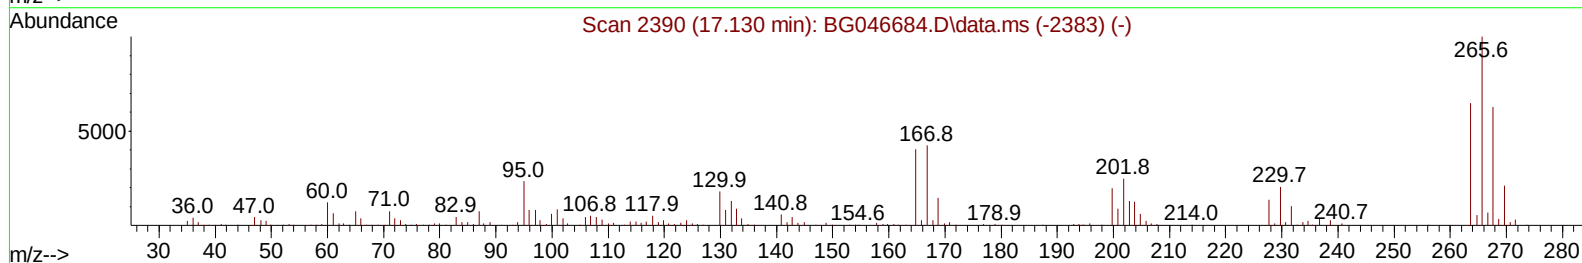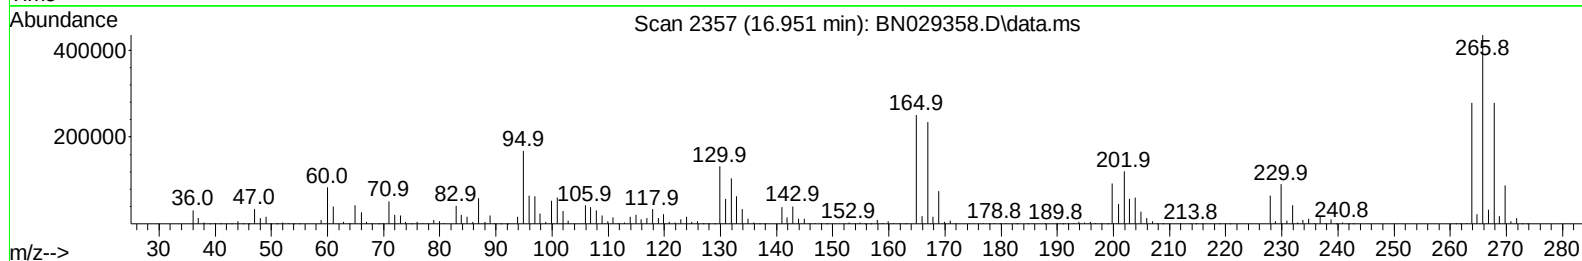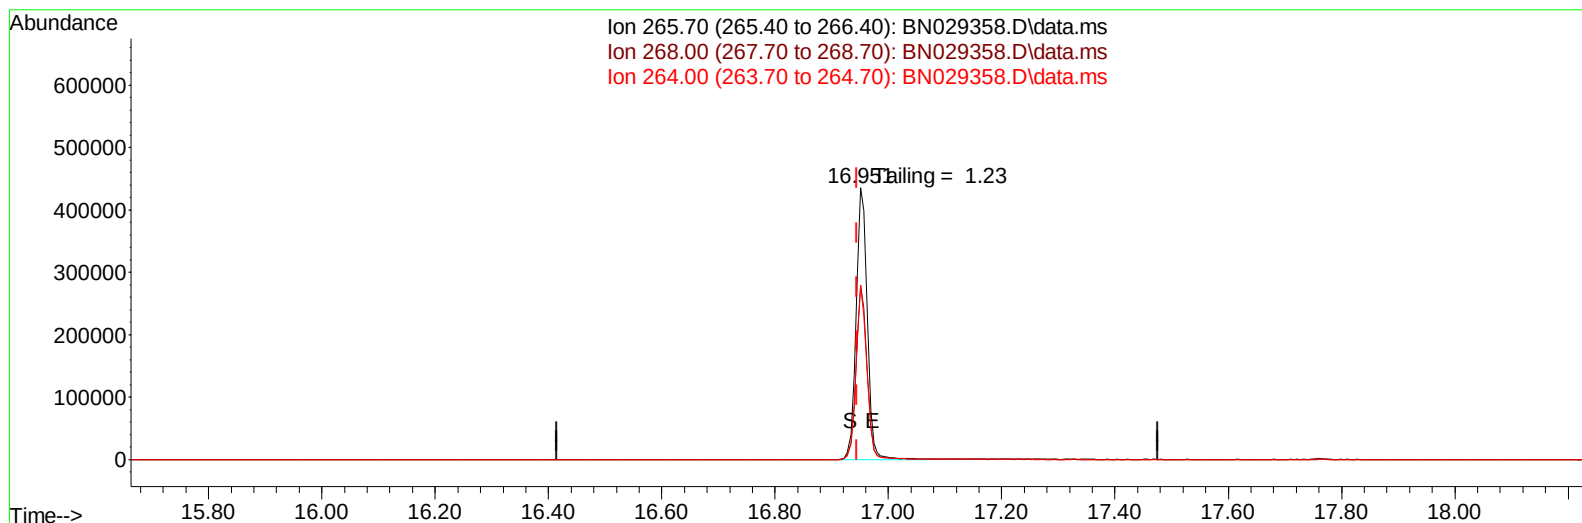

TIC: BN029358.D\data.ms

(70) Pentachlorophenol (C)

16.951min (+ 0.006) 18305.11 ng




response 596020

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.93
264.00	61.60	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012324\
Data File : BN029358.D
Acq On : 23 Jan 2024 22:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 24 05:23:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

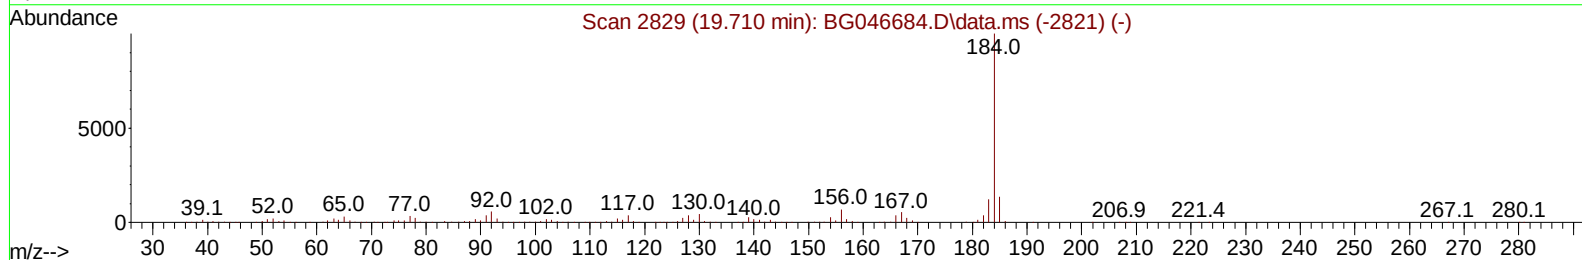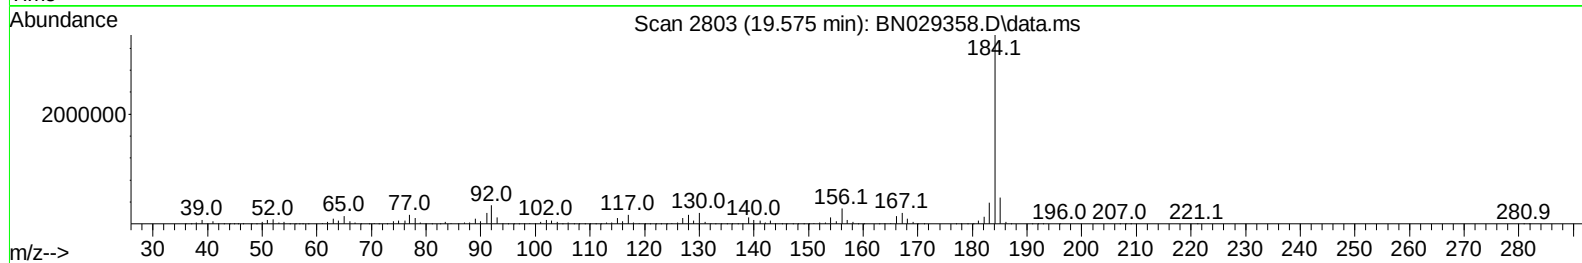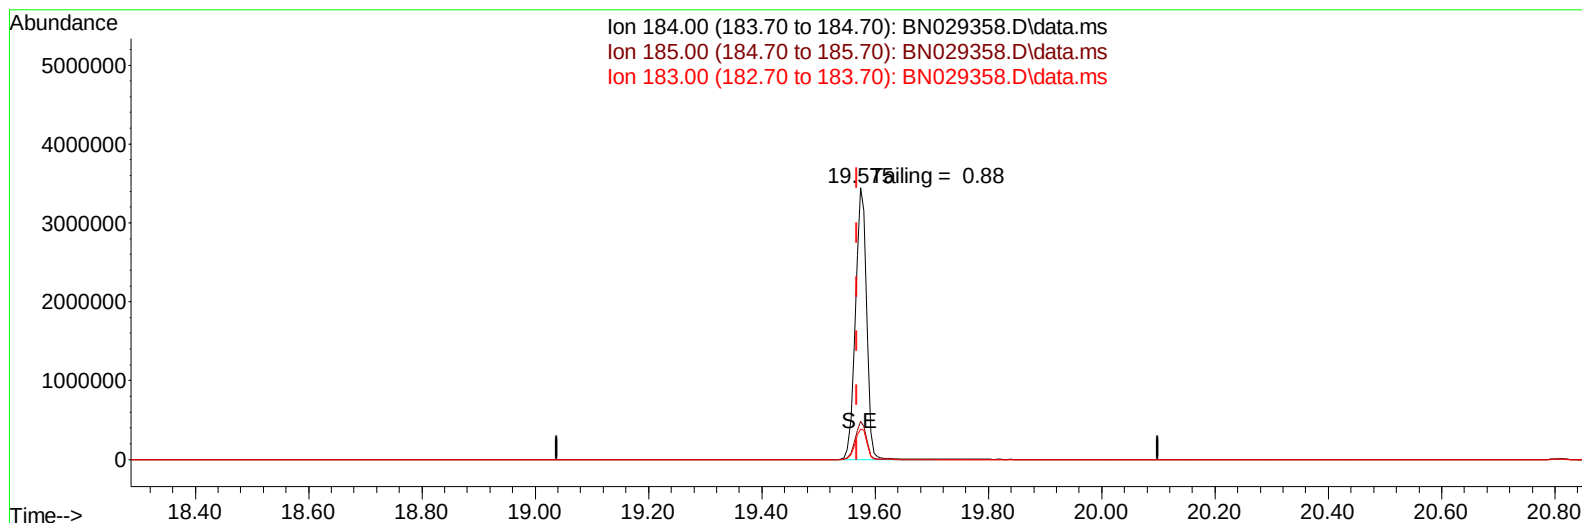

TIC: BN029358.D\data.ms

(77) Benzidine

19.575min (+ 0.006) 0.00 ng

response 4714345

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/23/2024	BNA_N	<u>BN029358.D</u>
Compound Name	Response	Retention Time
DDT	1977838	20.81
DDD	32987	20.363
DDE	462	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33449	2011287	1.66

Instrument :
BNA_N
ClientSampleId :
DFTPP