


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012420\
 Data File : BN009426.D
 Acq On : 23 Jan 2020 15:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN011420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 09:33:55 2020

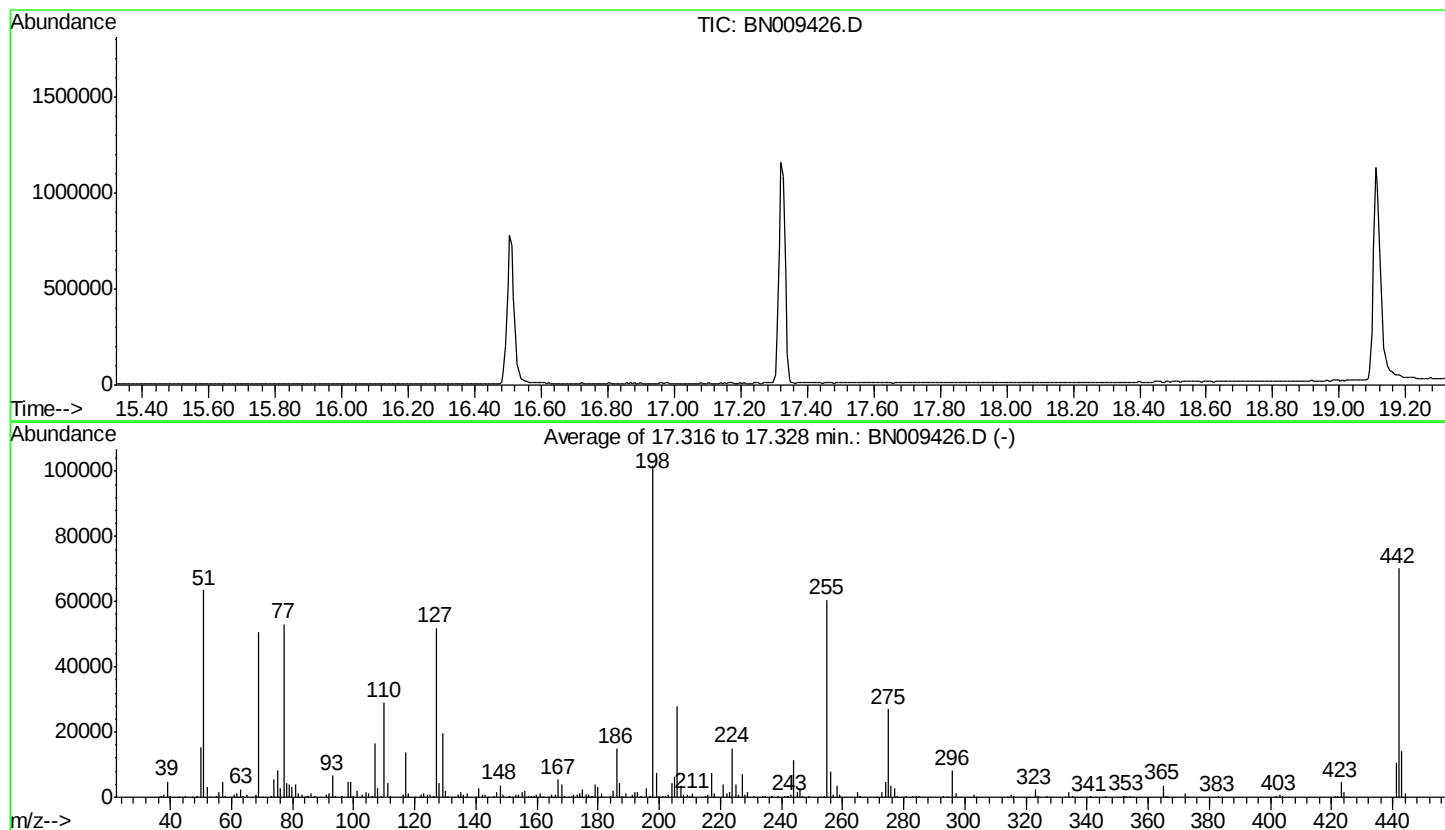

AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2430

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.5	63556	PASS
68	69	0.00	2	1.2	618	PASS
69	198	0.00	100	49.9	50730	PASS
70	69	0.00	2	0.2	102	PASS
127	198	10	80	51.1	52016	PASS
197	198	0.00	2	0.4	357	PASS
198	198	100	100	100.0	101744	PASS
199	198	5	9	7.2	7367	PASS
275	198	10	60	26.5	27010	PASS
365	198	1	100	3.6	3652	PASS
441	198	0.01	100	10.3	10439	PASS
442	198	50	100	69.1	70266	PASS
443	442	15	24	20.2	14173	PASS