


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012420\
 Data File : BN009434.D
 Acq On : 24 Jan 2020 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN011420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 09:33:55 2020

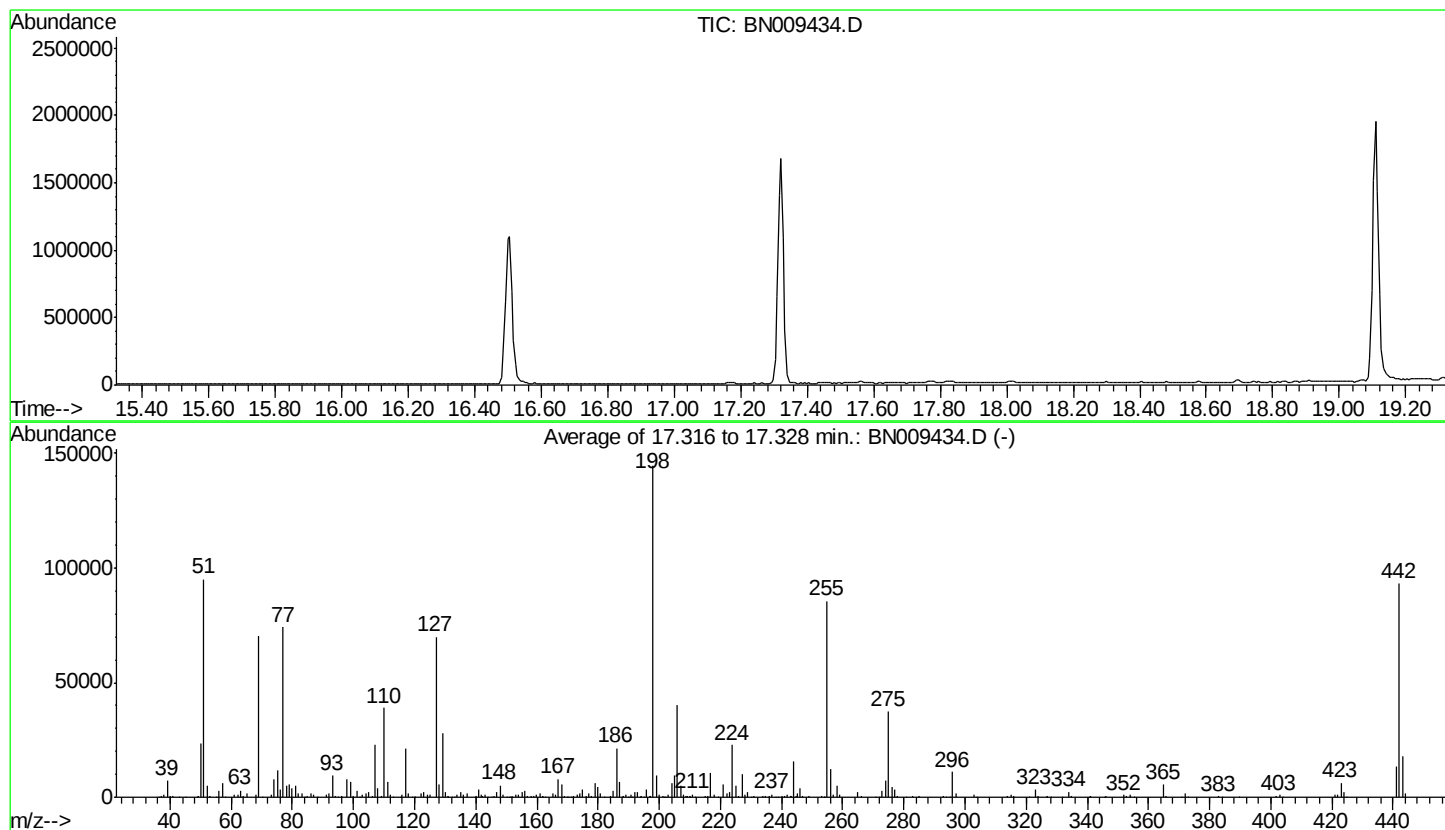

AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2430

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.7	95002	PASS
68	69	0.00	2	1.9	1316	PASS
69	198	0.00	100	48.6	70301	PASS
70	69	0.00	2	0.2	109	PASS
127	198	10	80	48.3	69861	PASS
197	198	0.00	2	0.4	628	PASS
198	198	100	100	100.0	144682	PASS
199	198	5	9	6.7	9627	PASS
275	198	10	60	25.7	37213	PASS
365	198	1	100	3.8	5451	PASS
441	198	0.01	100	9.2	13289	PASS
442	198	50	100	64.4	93208	PASS
443	442	15	24	19.4	18052	PASS