
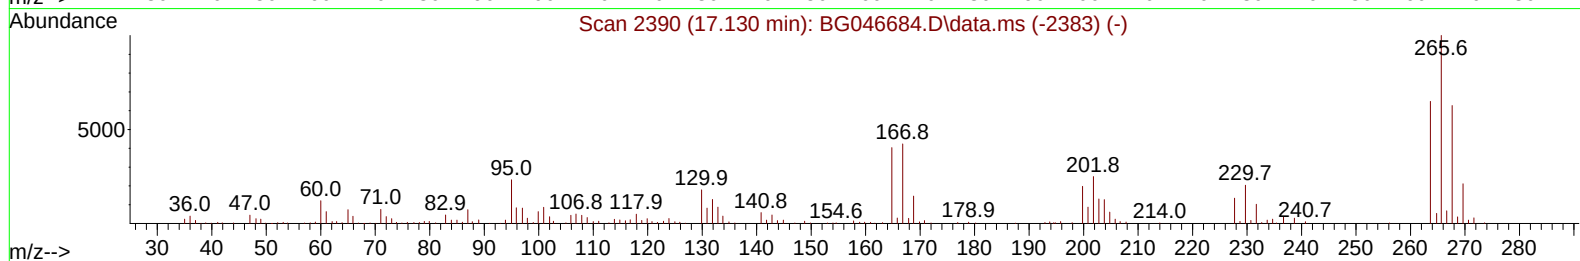
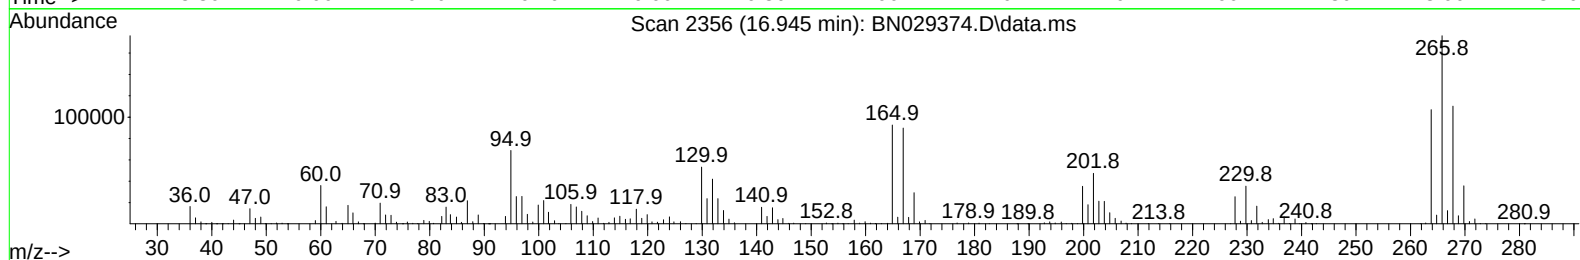


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012424\
Data File : BN029374.D
Acq On : 24 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 18:07:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

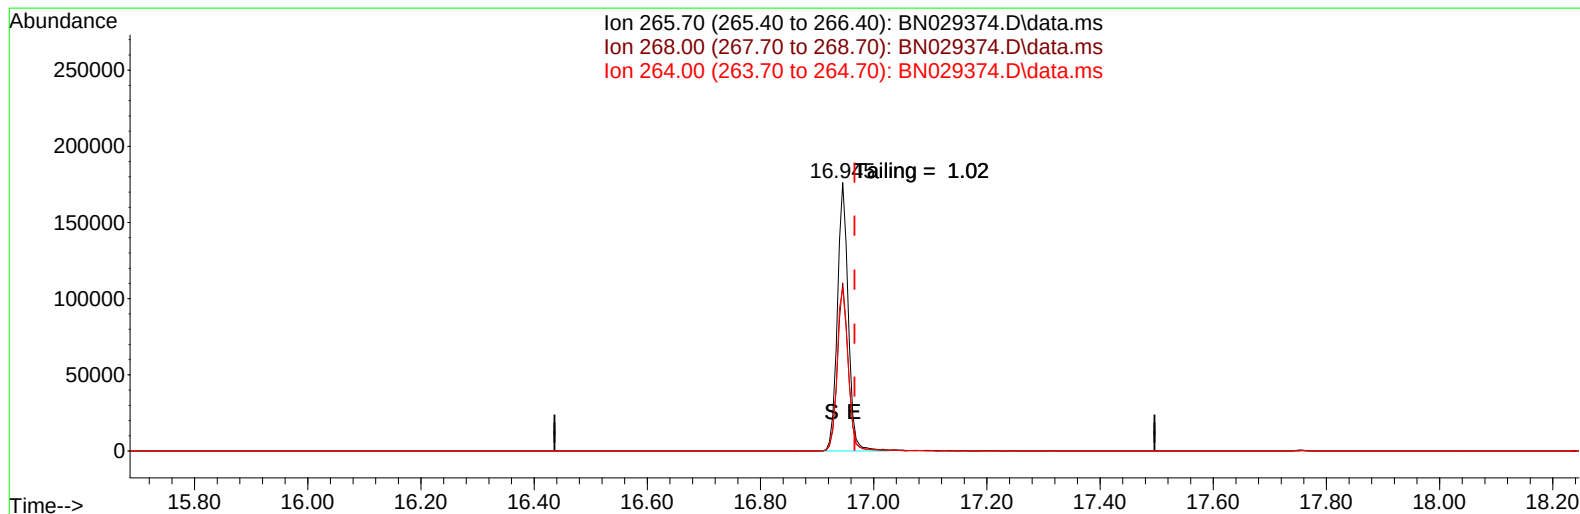

TIC: BN029374.D\data.ms

(70) Pentachlorophenol (C)




16.945min (-0.021) 16390.99 ng

response 234754

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.60
264.00	61.60	60.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012424\
Data File : BN029374.D
Acq On : 24 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 18:07:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

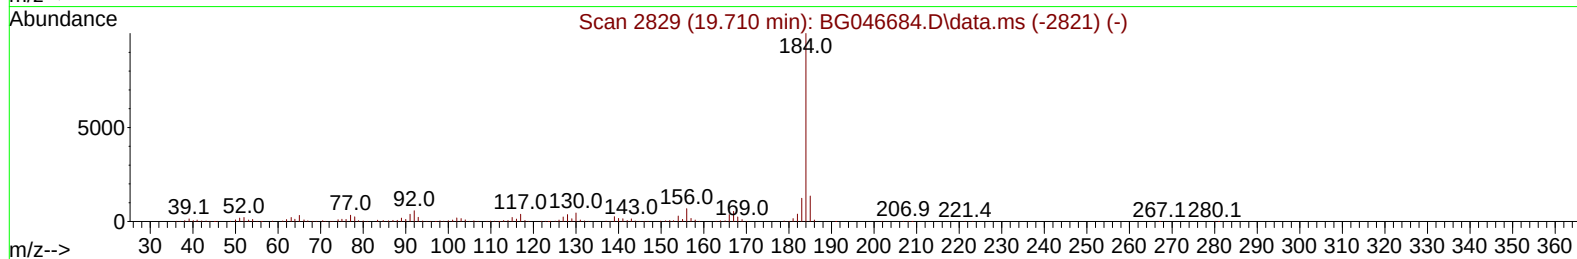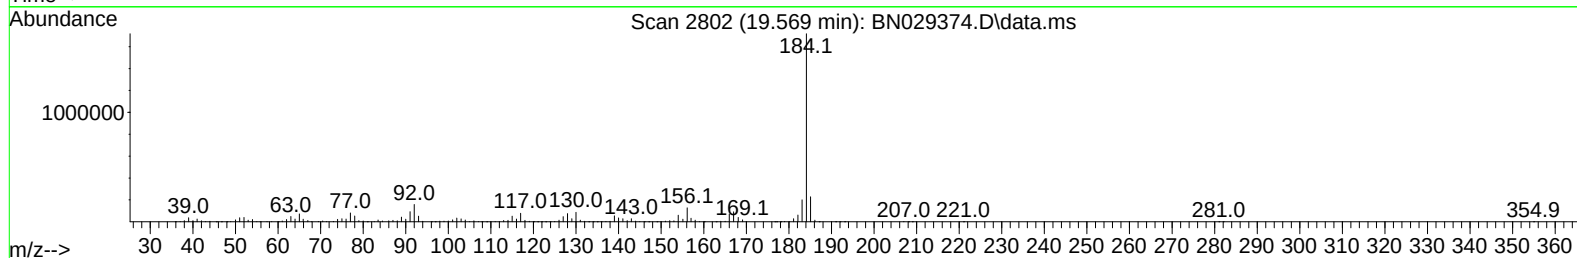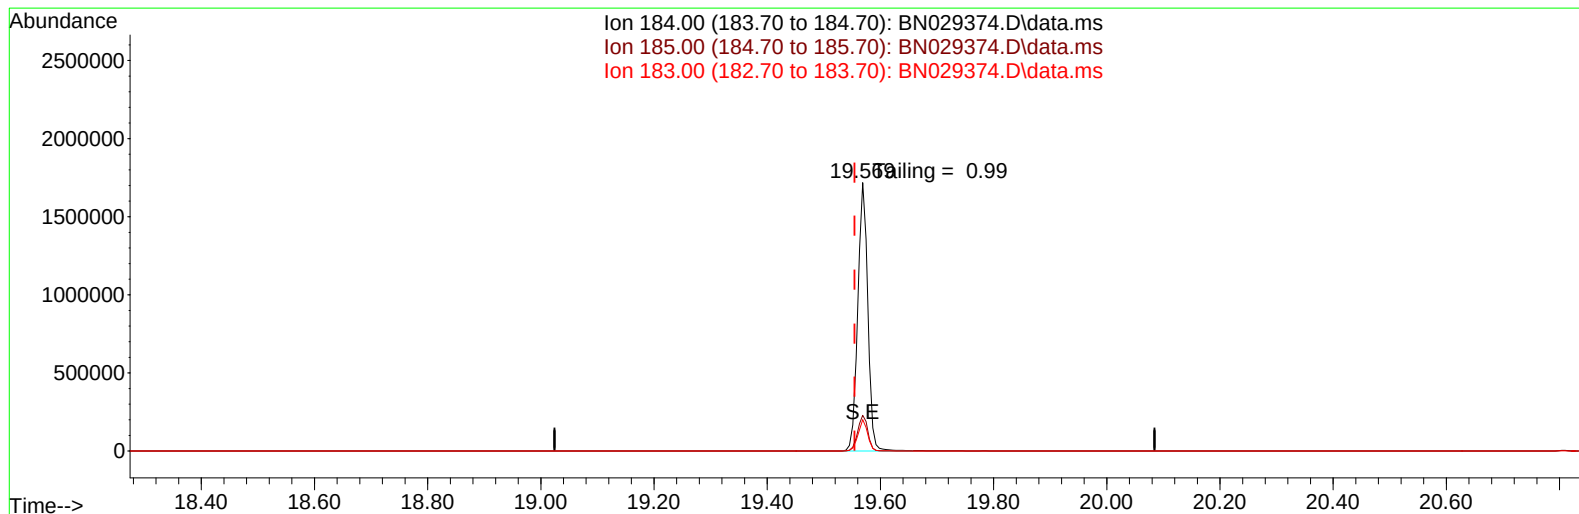

TIC: BN029374.D\data.ms

(77) Benzidine

19.569min (+ 0.015) 0.00 ng

response 2127103

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.31
183.00	13.20	11.69
0.00	0.00	0.00