
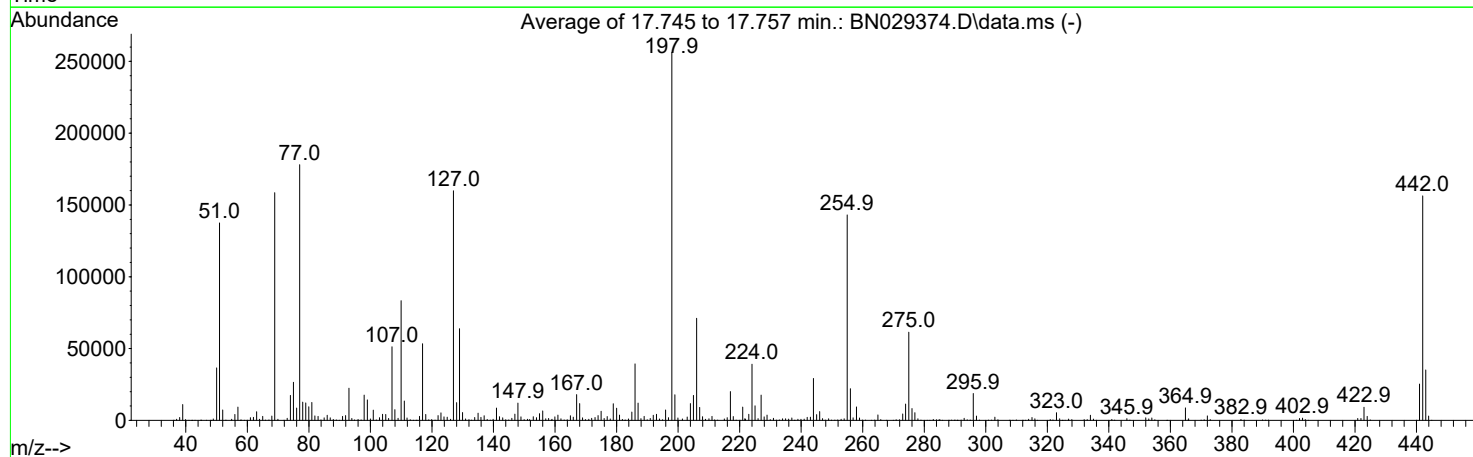


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012424\
Data File : BN029374.D
Acq On : 24 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 23 02:16:14 2024

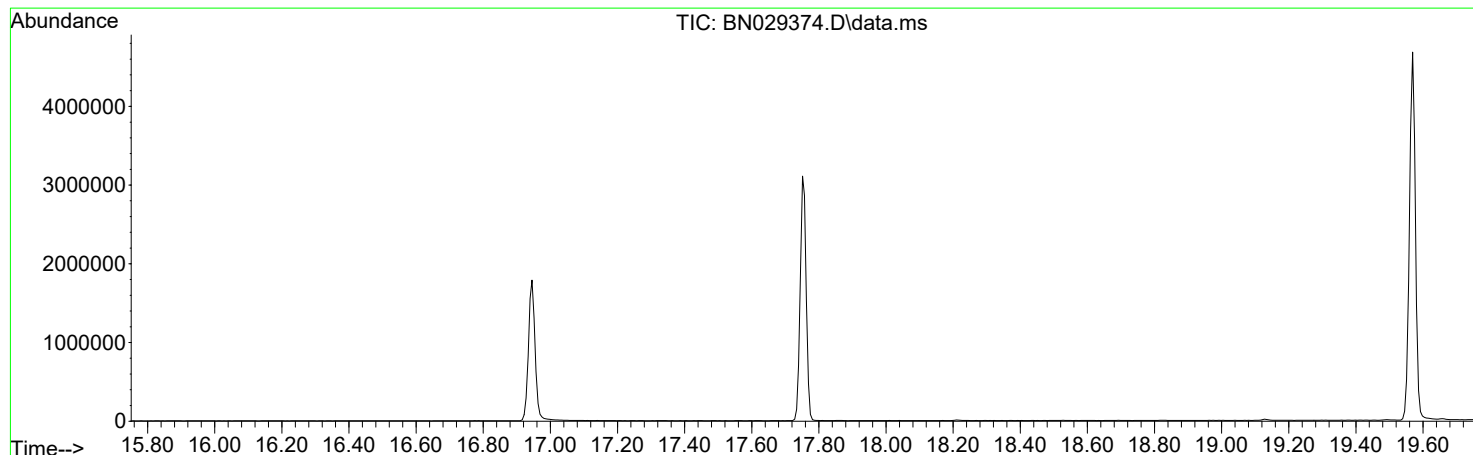

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.7	137559	PASS
68	69	0.00	2	1.9	3011	PASS
69	198	0.00	100	61.9	158592	PASS
70	69	0.00	2	0.5	799	PASS
127	198	10	80	62.4	159936	PASS
197	198	0.00	2	0.7	1894	PASS
198	198	100	100	100.0	256171	PASS
199	198	5	9	7.0	17846	PASS
275	198	10	60	24.0	61397	PASS
365	198	1	100	3.4	8730	PASS
441	198	0.01	100	9.9	25309	PASS
442	442	50	100	100.0	156312	PASS
443	442	15	24	22.5	35149	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/24/2024	BNA_N	<u>BN029374.D</u>
Compound Name	Response	Retention Time
DDT	916001	20.81
DDD	16364	20.363
DDE	421	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16785	932786	1.80

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012424\
Data File : BN029374.D
Acq On : 24 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 24 18:07:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

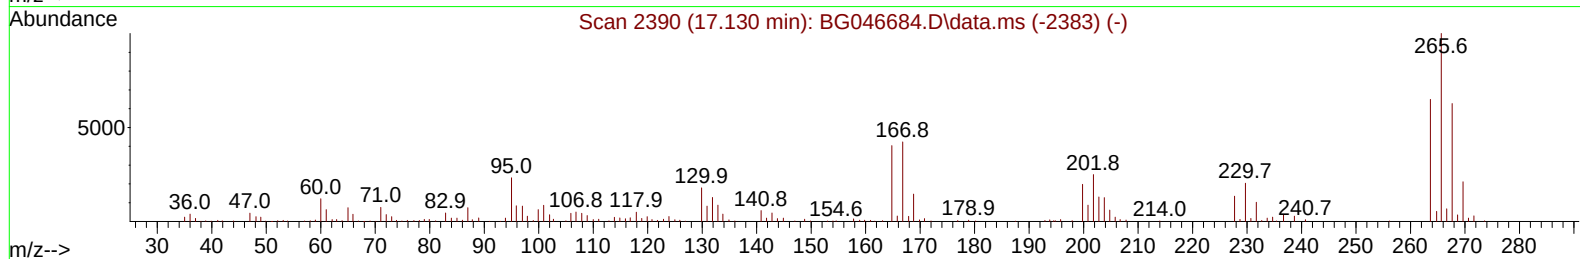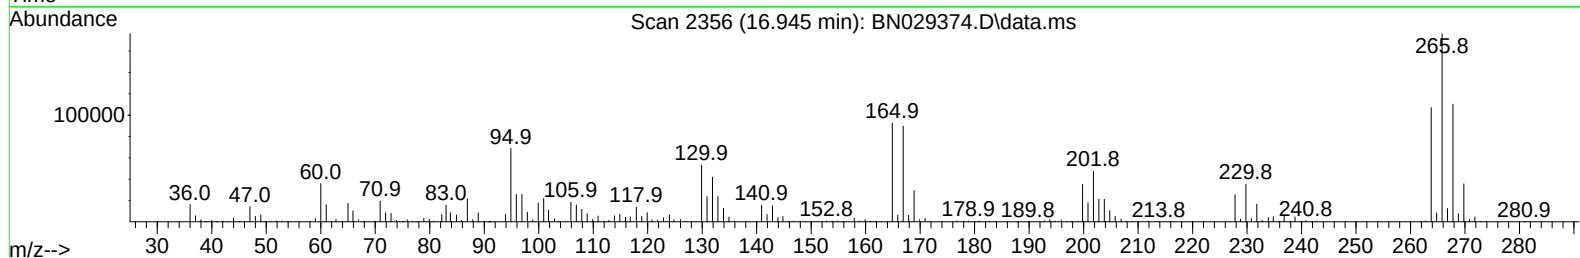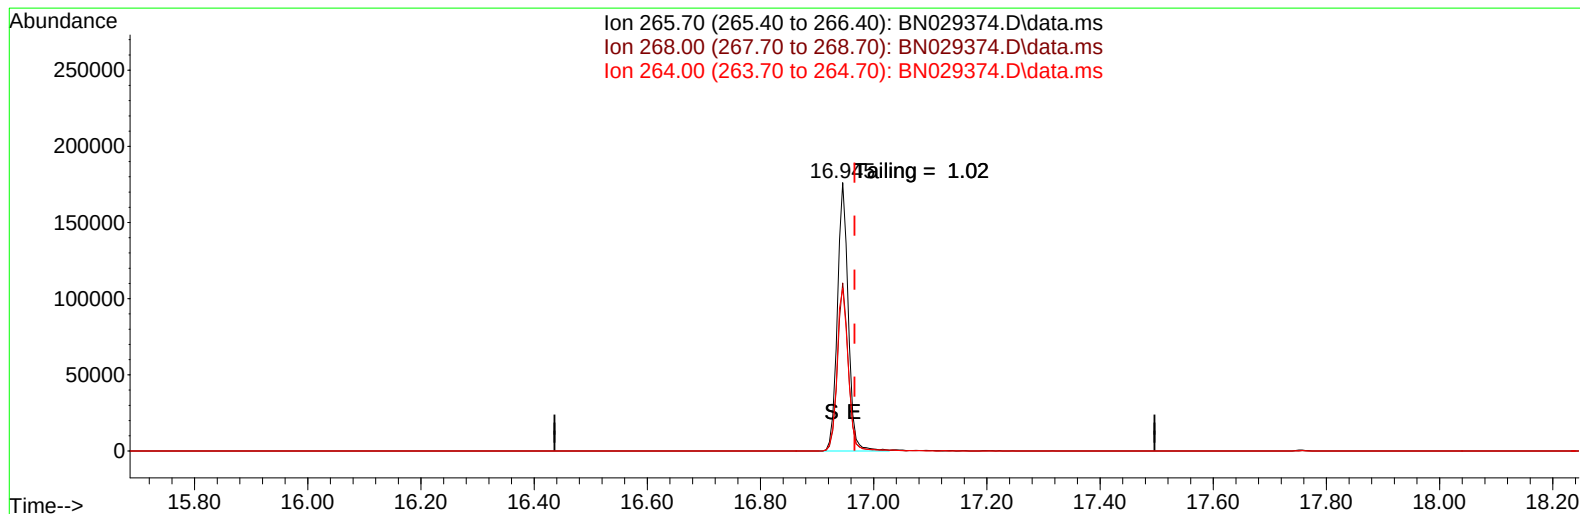

TIC: BN029374.D\data.ms

(70) Pentachlorophenol (C)

16.945min (-0.021) 16390.99 ng




response 234754

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.60
264.00	61.60	60.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012424\
Data File : BN029374.D
Acq On : 24 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 24 18:07:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 05:21:41 2024
Response via : Initial Calibration

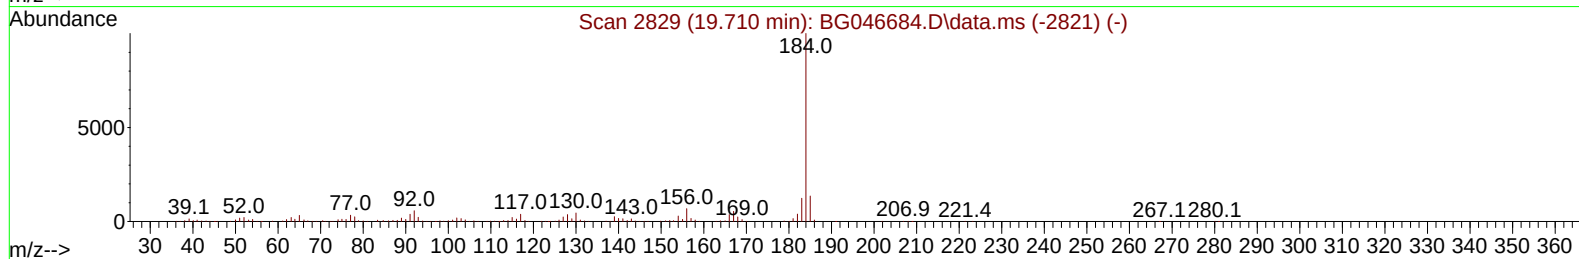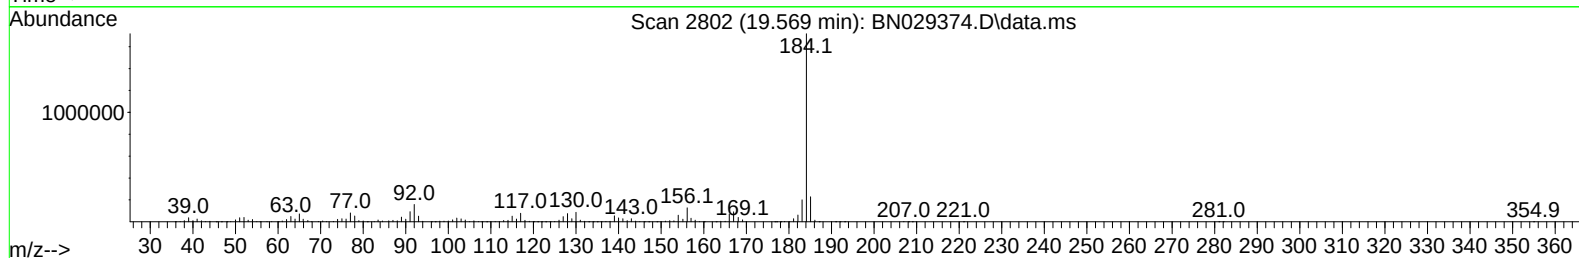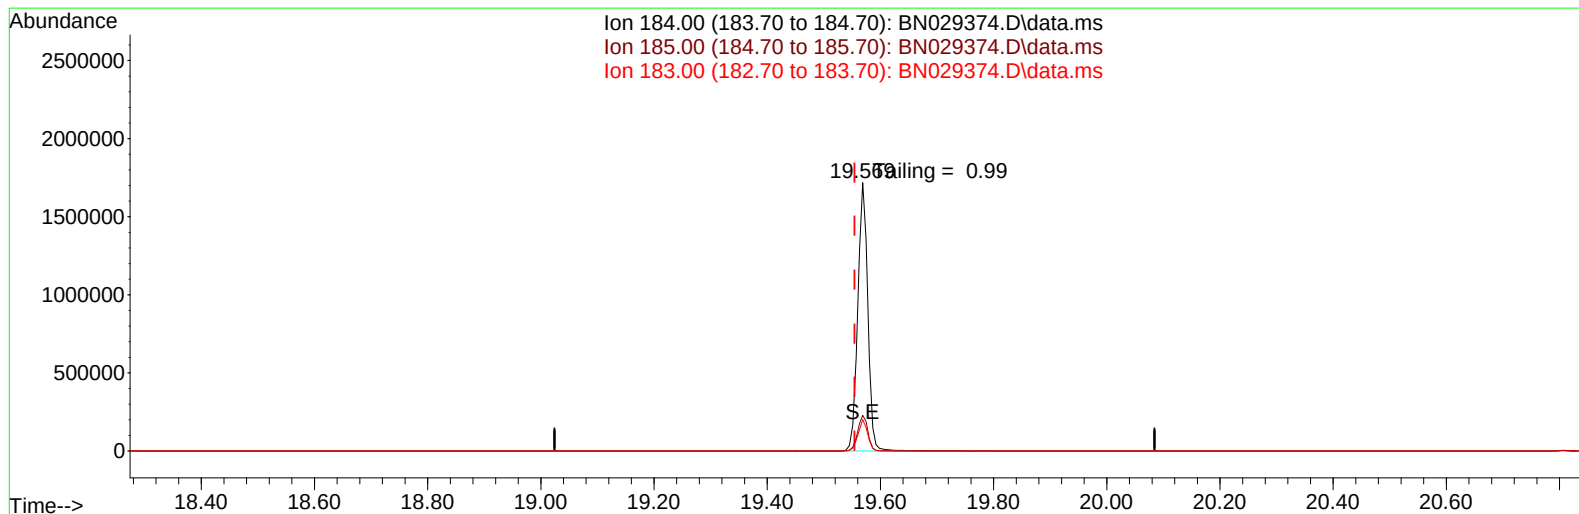

TIC: BN029374.D\data.ms

(77) Benzidine

19.569min (+ 0.015) 0.00 ng

response 2127103

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.31
183.00	13.20	11.69
0.00	0.00	0.00